

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121021\
Data File : FG009191.D
Signal(s) : FID1A.ch
Acq On : 10 Dec 2021 11:00
Operator : AJ\MA
Sample : RT MARKET
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 10 22:43:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112321.M
Quant Title :
QLast Update : Wed Nov 24 00:59:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.462	2660795	17.975 ug/ml
12)	N-OCTACOSANE	16.937	2303083	20.199 ug/ml
13)	N-TRIACONTANE	17.831	101999	0.943 ug/ml
14)	N-DOTRIACONTANE	18.665	130593	1.270 ug/ml
15)	N-TETRATRIACONTANE	19.451	145121	1.467 ug/ml
16)	N-HEXATRIACONTANE	20.199	161710	1.721 ug/ml
17)	N-OCTATRIACONTANE	20.956	187454	2.021 ug/ml
18)	N-TETRACONTANE	21.911	229254	2.330 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121021\
Data File : FG009191.D
Signal(s) : FID1A.ch
Acq On : 10 Dec 2021 11:00
Operator : AJ\MA
Sample : RT MARKET
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 10 22:43:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112321.M
Quant Title :
QLast Update : Wed Nov 24 00:59:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

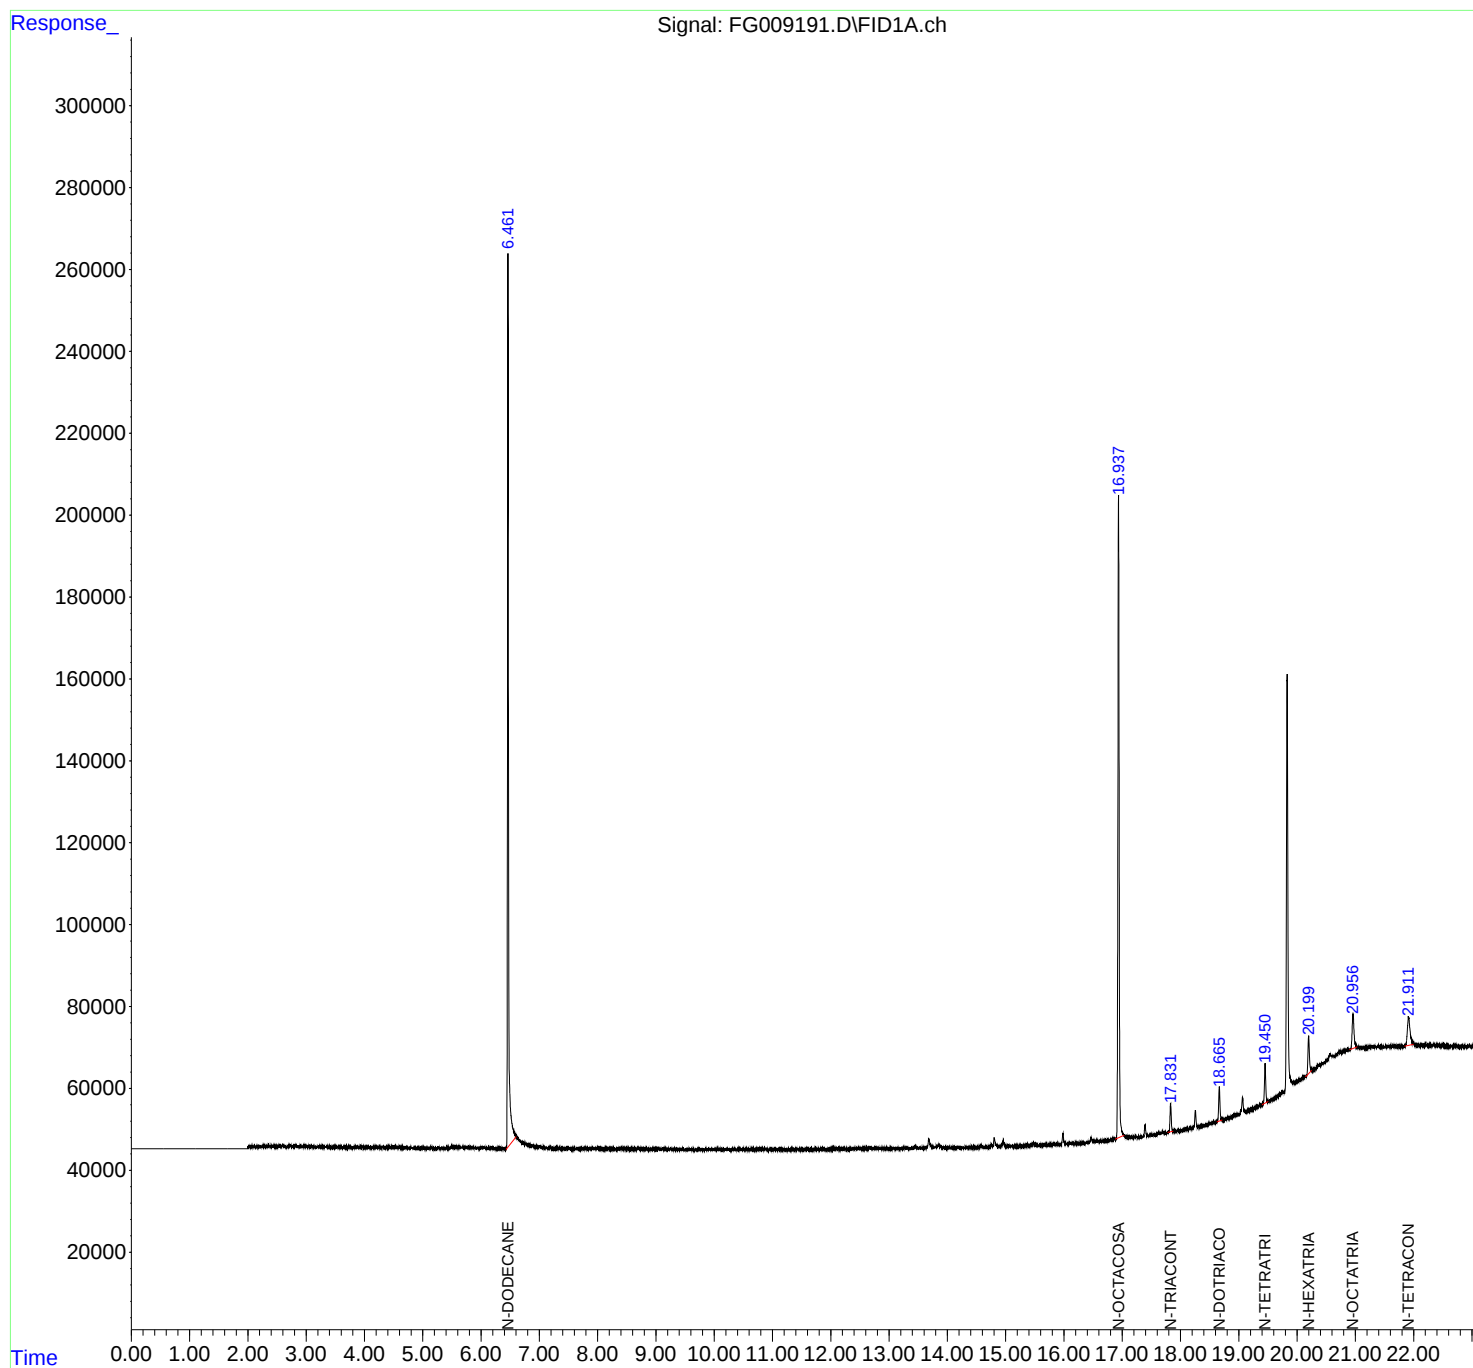


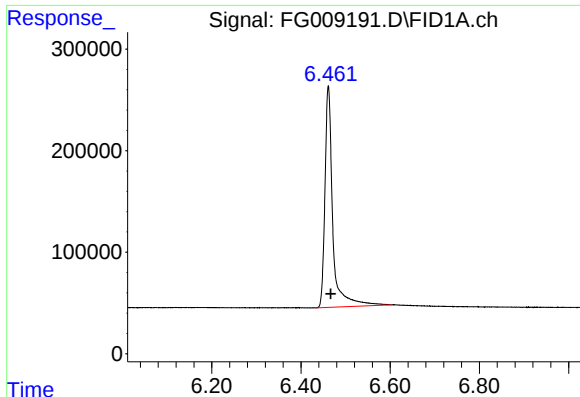

#3 N-DODECANE


R.T.: 6.462 min
Delta R.T.: -0.005 min
Response: 2660795
Conc: 17.98 ug/ml

Instrument :
FID_G
ClientSampleId :

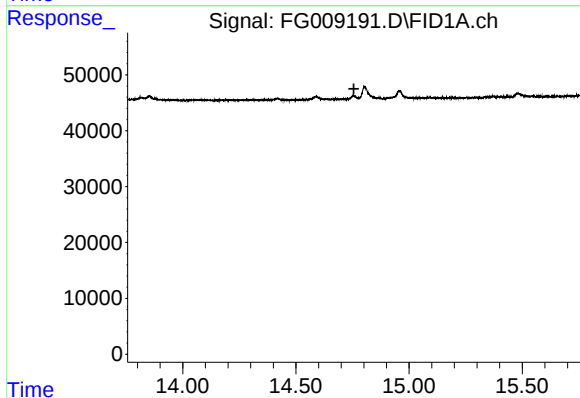


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.756 min
Response: 0
Conc: N.D.

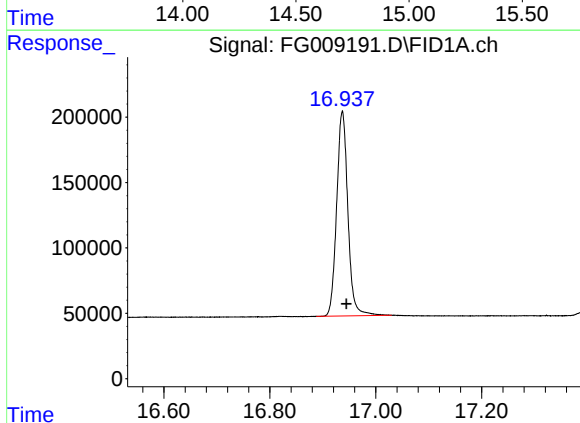


#12 N-OCTACOSANE

R.T.: 16.937 min
Delta R.T.: -0.008 min
Response: 2303083
Conc: 20.20 ug/ml

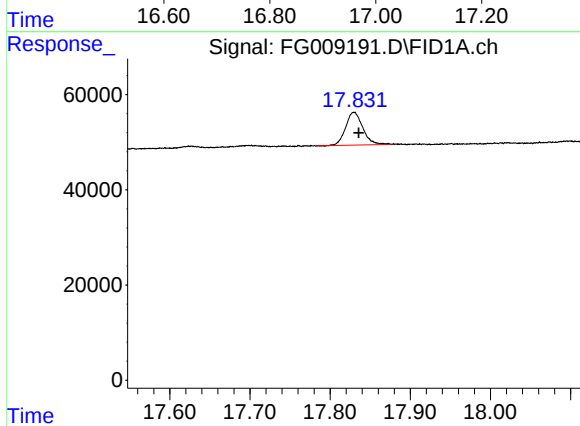

#13 N-TRIACONTANE


R.T.: 17.831 min
Delta R.T.: -0.005 min
Response: 101999
Conc: 0.94 ug/ml

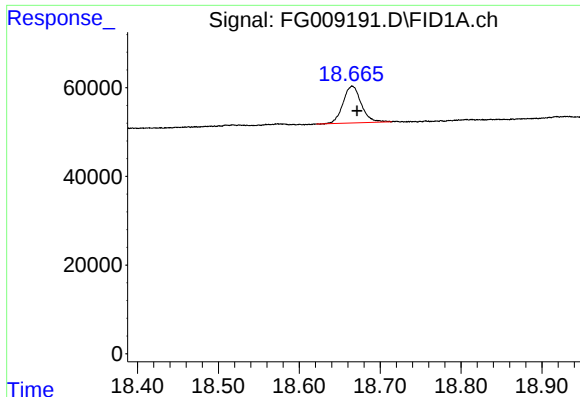

#14 N-DOTRIACONTANE


R.T.: 18.665 min
Delta R.T.: -0.006 min
Response: 130593
Conc: 1.27 ug/ml

Instrument :
FID_G
ClientSampleId :

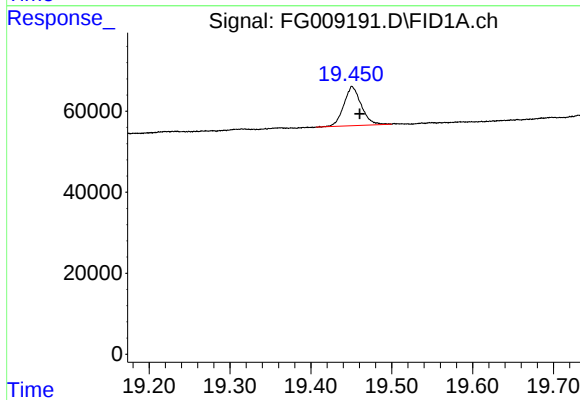


#15 N-TETRATRIACONTANE

R.T.: 19.451 min
Delta R.T.: -0.010 min
Response: 145121
Conc: 1.47 ug/ml

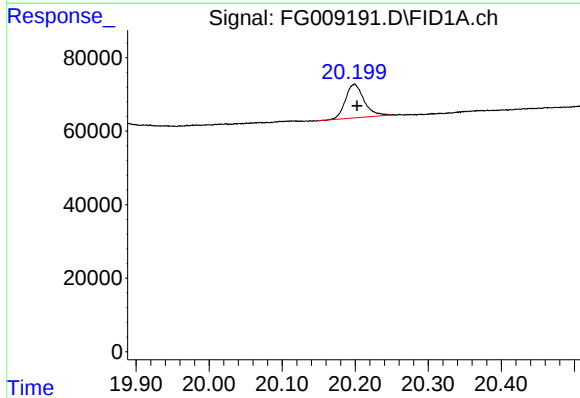


#16 N-HEXATRIACONTANE

R.T.: 20.199 min
Delta R.T.: -0.003 min
Response: 161710
Conc: 1.72 ug/ml

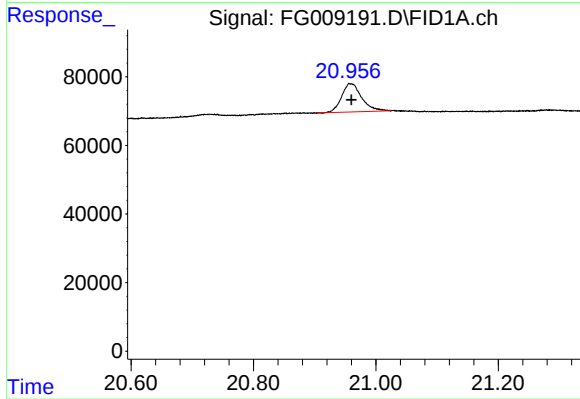

#17 N-OCTATRIACONTANE

R.T.: 20.956 min
Delta R.T.: -0.004 min
Response: 187454
Conc: 2.02 ug/ml

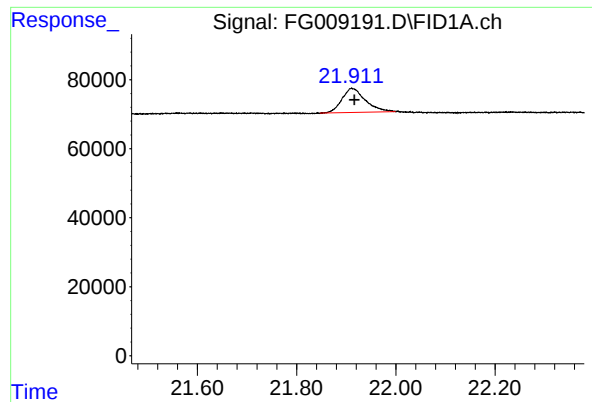

#18 N-TETRACONTANE

R.T.: 21.911 min
Delta R.T.: -0.006 min
Response: 229254
Conc: 2.33 ug/ml

Instrument :

FID_G

ClientSampleId :