

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121021\
 Data File : FG009208.D
 Signal(s) : FID1A.ch
 Acq On : 10 Dec 2021 20:47
 Operator : AJ\MA
 Sample : M4989-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 10 22:48:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112321.M
 Quant Title :
 QLast Update : Wed Nov 24 00:59:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.746	1584494	13.586 ug/ml
Target Compounds			
6) N-OCTADECANE	11.323	39820	0.275 ug/ml
7) N-EICOSANE	12.639	55178	0.386 ug/ml
8) N-DOCOSANE	13.839	61967	0.452 ug/ml
10) N-TETRACOSANE	15.008	62884	0.478 ug/ml
14) N-DOTRIACONTANE	18.659	59437	0.578 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121021\
Data File : FG009208.D
Signal(s) : FID1A.ch
Acq On : 10 Dec 2021 20:47
Operator : AJ\MA
Sample : M4989-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 10 22:48:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112321.M
Quant Title :
QLast Update : Wed Nov 24 00:59:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

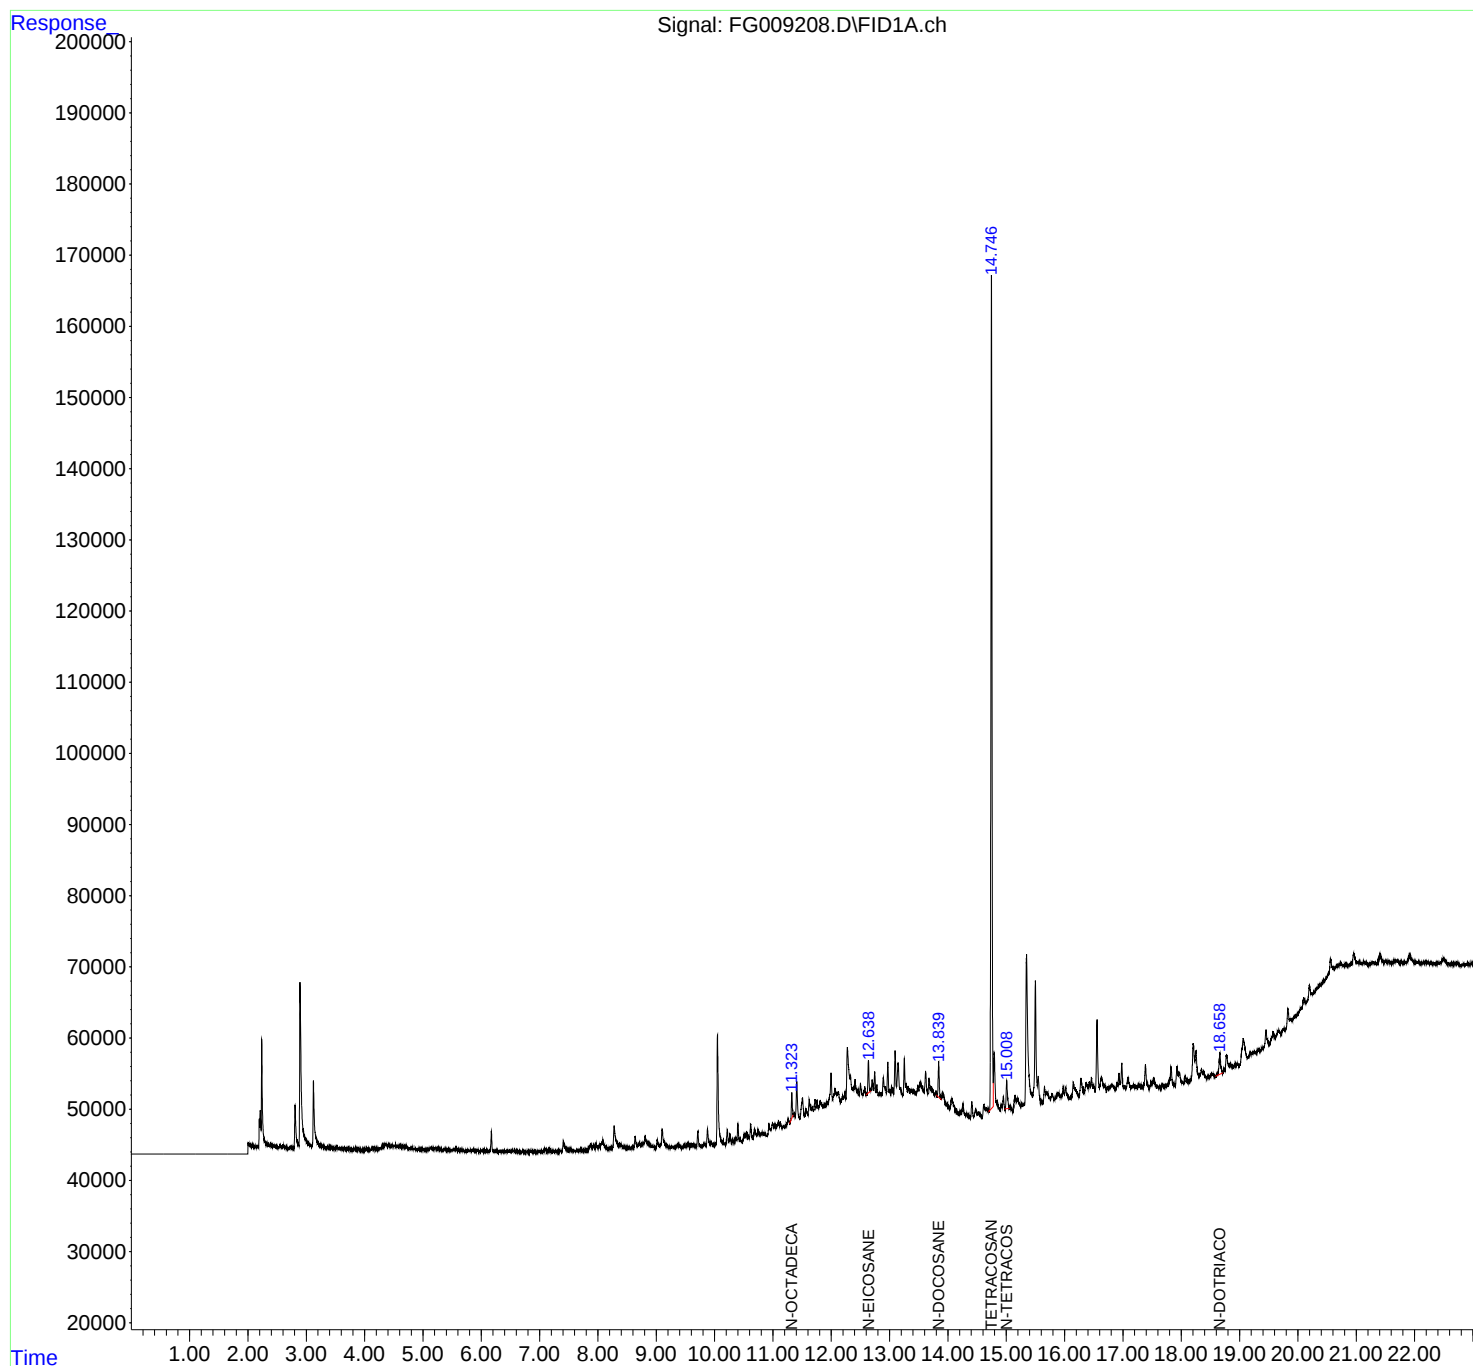


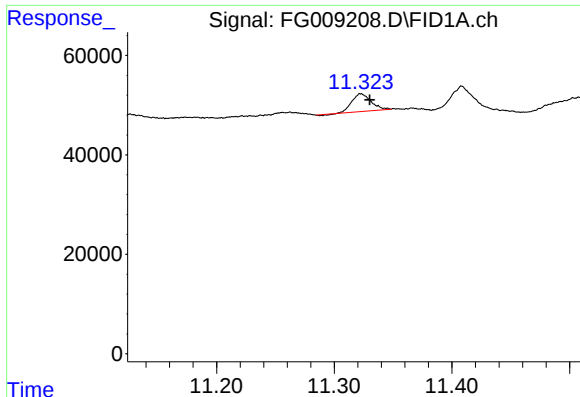

#6 N-OCTADECANE


R.T.: 11.323 min
Delta R.T.: -0.008 min
Response: 39820
Conc: 0.27 ug/ml

Instrument :
FID_G
ClientSampleId :

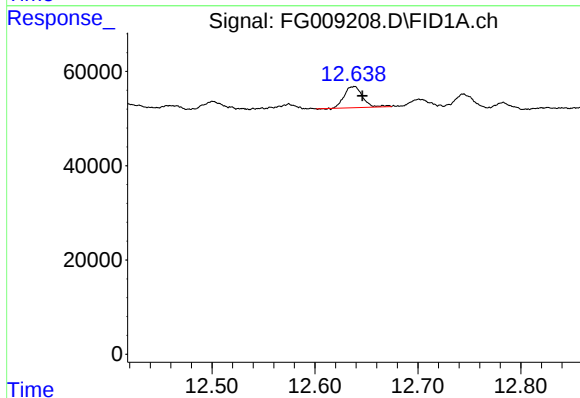


#7 N-EICOSANE

R.T.: 12.639 min
Delta R.T.: -0.008 min
Response: 55178
Conc: 0.39 ug/ml

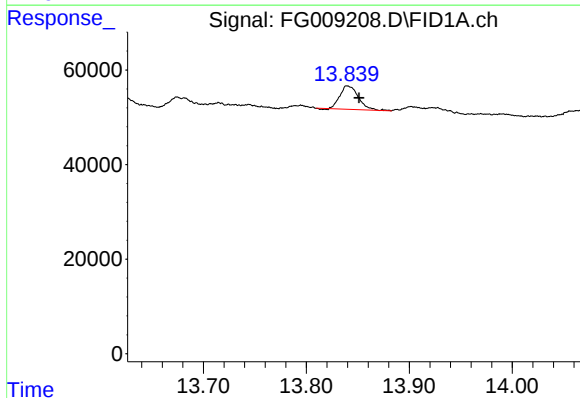


#8 N-DOCOSANE

R.T.: 13.839 min
Delta R.T.: -0.012 min
Response: 61967
Conc: 0.45 ug/ml

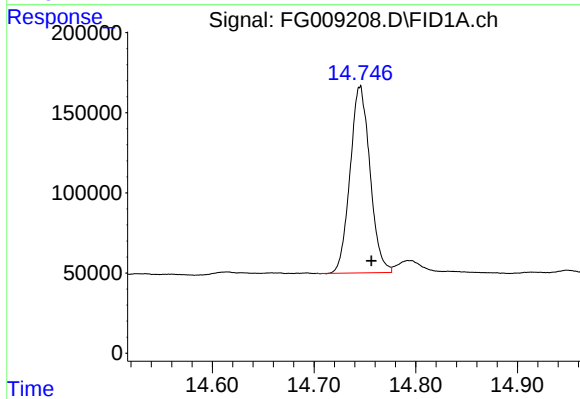

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.746 min
Delta R.T.: -0.011 min
Response: 1584494
Conc: 13.59 ug/ml

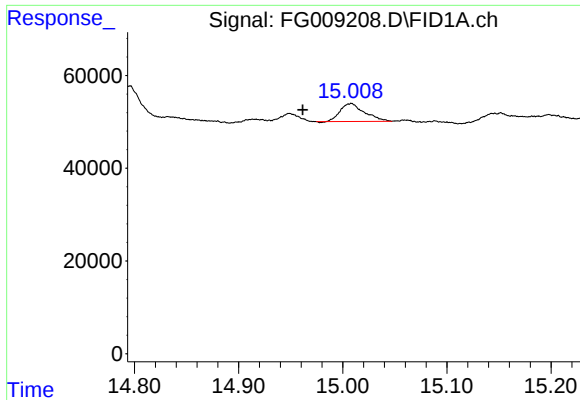

#10 N-TETRACOSANE

R.T.: 15.008 min
Delta R.T.: 0.047 min
Response: 62884
Conc: 0.48 ug/ml

Instrument :
FID_G
ClientSampleId :

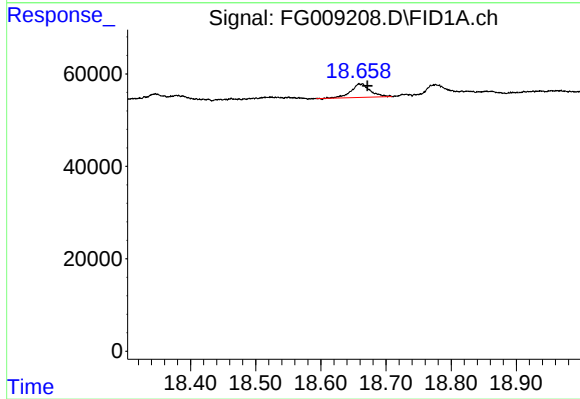

#14 N-DOTRIACONTANE

R.T.: 18.659 min
Delta R.T.: -0.013 min
Response: 59437
Conc: 0.58 ug/ml