

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG121021\  
Data File : FG009204.D  
Signal(s) : FID1A.ch  
Acq On : 10 Dec 2021 18:45  
Operator : AJ\MA  
Sample : M4990-01  
Misc :  
ALS Vial : 9 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :  
R1-8

Manual Integrations  
APPROVED

Reviewed By :Ankita Jodhani 12/11/2021  
Supervised By :mohammad ahmed 12/13/2021

Integration File: autoint1.e  
Quant Time: Dec 10 22:47:51 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG112321.M  
Quant Title :  
QLast Update : Wed Nov 24 00:59:46 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units    |
|-------------------------------|--------|----------|---------------|
| -----                         |        |          |               |
| System Monitoring Compounds   |        |          |               |
| 9) S TETRACOSANE-d50 (SURR... | 14.743 | 1716934  | 14.722 ug/mlm |
| Target Compounds              |        |          |               |
| -----                         |        |          |               |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG121021\  
Data File : FG009204.D  
Signal(s) : FID1A.ch  
Acq On : 10 Dec 2021 18:45  
Operator : AJ\MA  
Sample : M4990-01  
Misc :  
ALS Vial : 9 Sample Multiplier: 1


Instrument :  
FID\_G  
ClientSampleId :  
R1-8


Manual Integrations  
APPROVED

Reviewed By :Ankita Jodhani 12/11/2021  
Supervised By :mohammad ahmed 12/13/2021

Integration File: autoint1.e  
Quant Time: Dec 10 22:47:51 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG112321.M  
Quant Title :  
QLast Update : Wed Nov 24 00:59:46 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

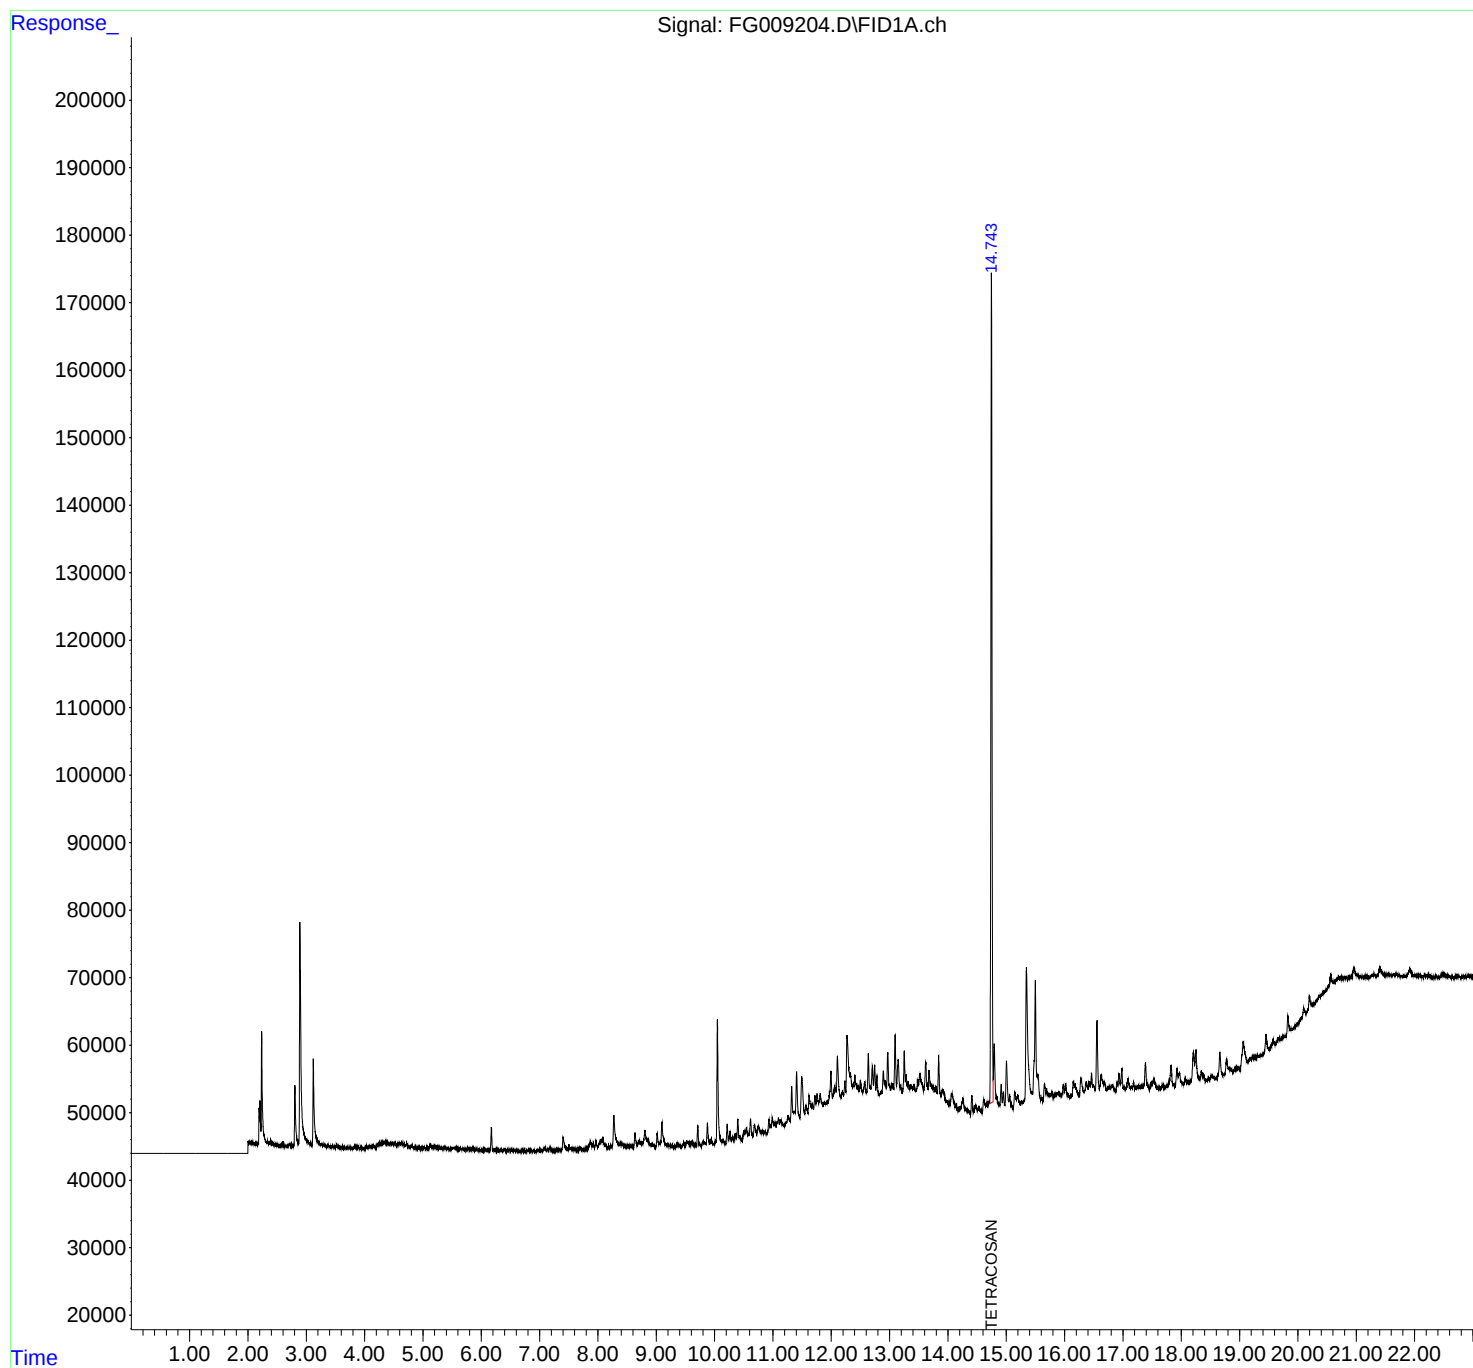

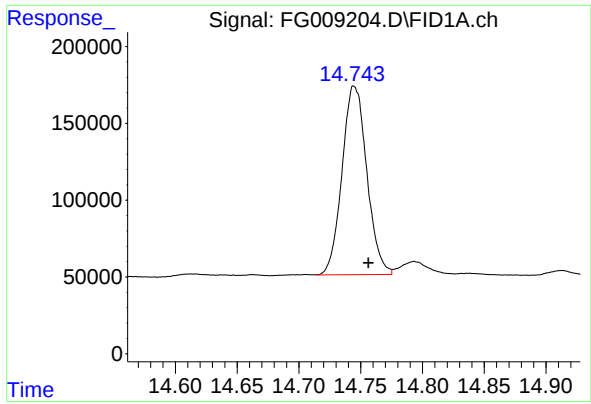

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.743 min  
Delta R.T.: -0.013 min  
Response: 1716934  
Conc: 14.72 ug/ml

Instrument :  
FID\_G  
ClientSampleId :  
R1-8

Manual Integrations  
APPROVED

Reviewed By :Ankita Jodhani 12/11/2021  
Supervised By :mohammad ahmed 12/13/2021