

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF121025\  
Data File : FF016886.D  
Signal(s) : FID2B.ch  
Acq On : 10 Dec 2025 10:07  
Operator : YP\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 54 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Dec 11 00:48:21 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF120125.M  
Quant Title :  
QLast Update : Mon Dec 01 15:05:52 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| Target Compounds            |        |          |              |
| 3) N-DODECANE               | 6.736  | 2725416  | 23.765 ug/ml |
| 12) N-OCTACOSANE            | 17.225 | 2742634  | 25.853 ug/ml |
| 13) N-TRIACONTANE           | 18.115 | 56100    | 0.525 ug/ml  |
| 14) N-DOTRIACONTANE         | 18.951 | 109776   | 1.041 ug/ml  |
| 15) N-TETRATRIACONTANE      | 19.737 | 76555    | 0.771 ug/ml  |
| -----                       |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF121025\  
Data File : FF016886.D  
Signal(s) : FID2B.ch  
Acq On : 10 Dec 2025 10:07  
Operator : YP\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 54 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Dec 11 00:48:21 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF120125.M  
Quant Title :  
QLast Update : Mon Dec 01 15:05:52 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

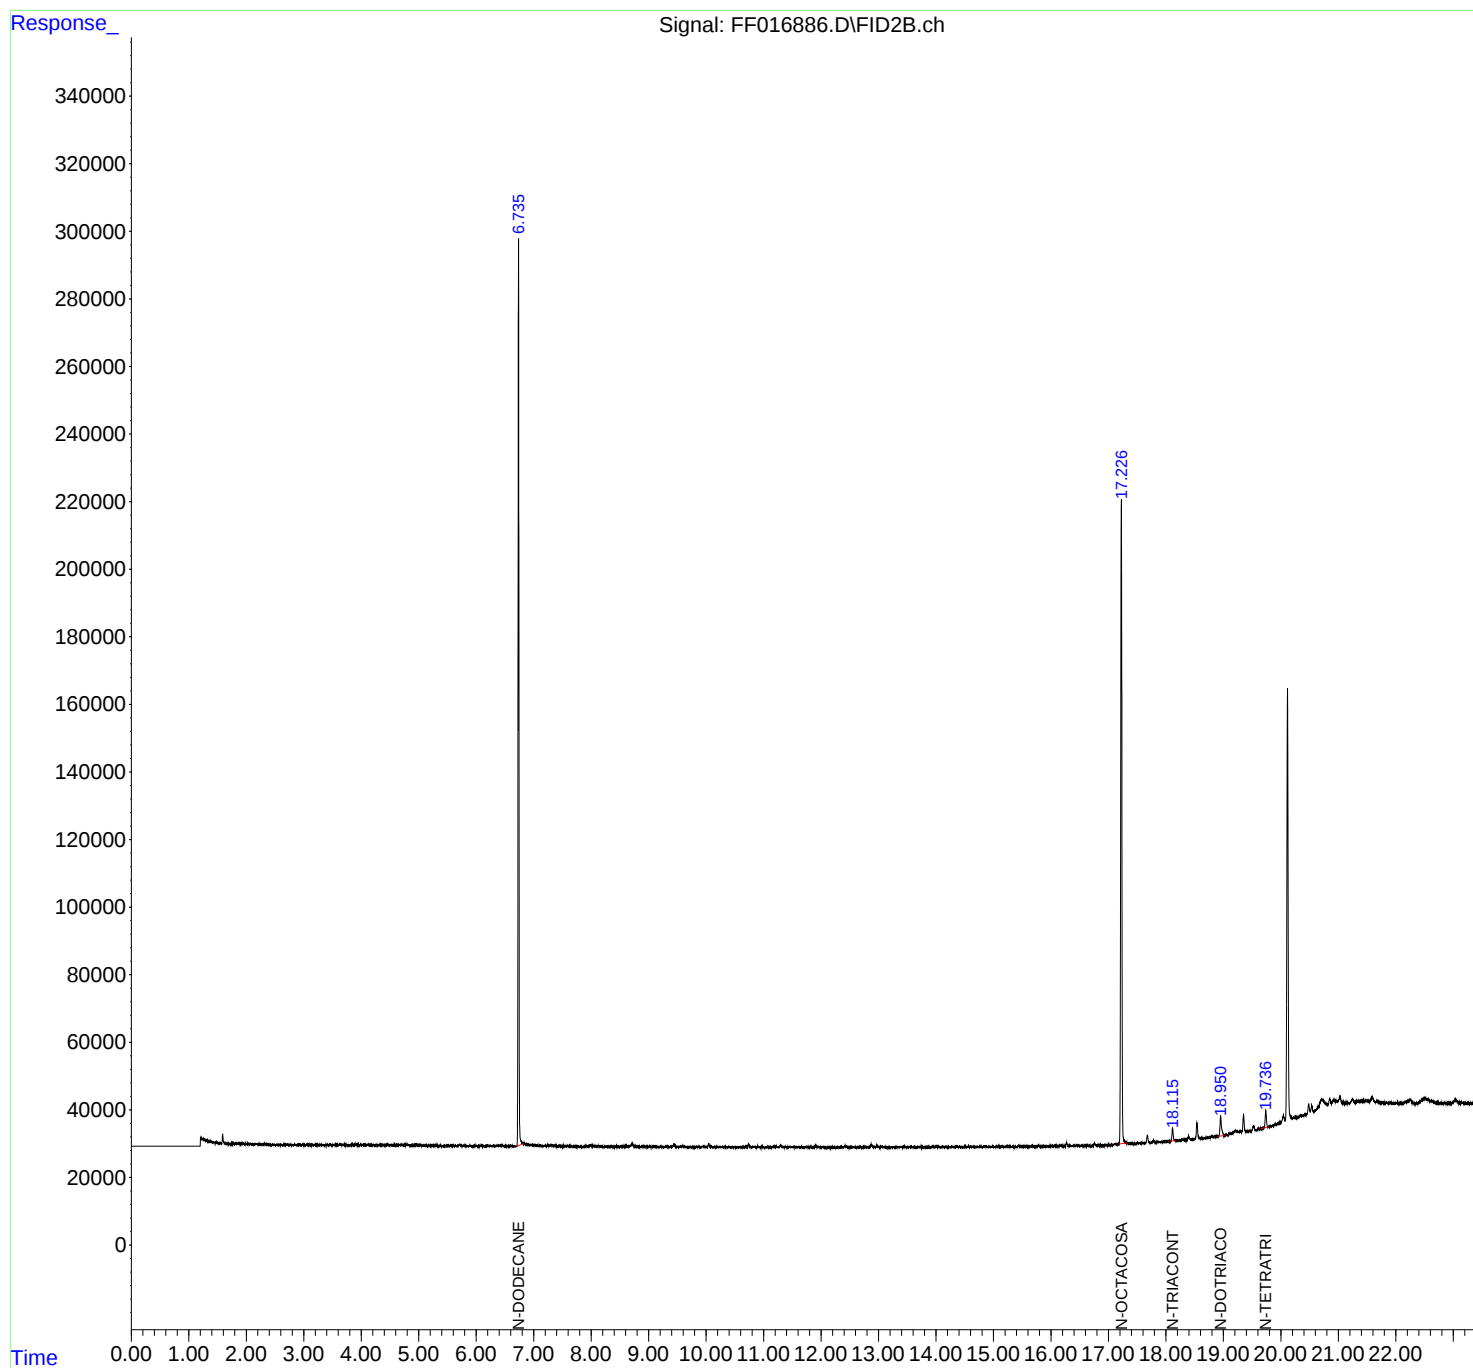


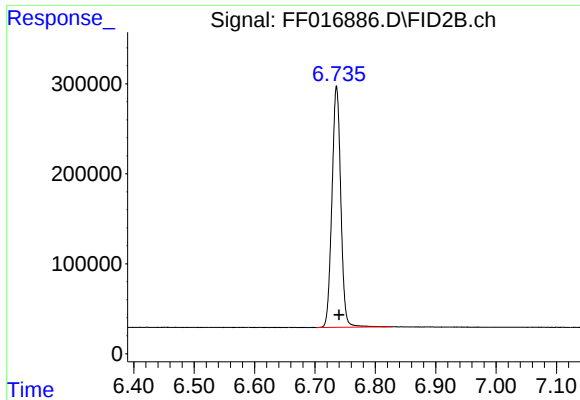

#3 N-DODECANE


R.T.: 6.736 min  
Delta R.T.: -0.004 min  
Response: 2725416  
Conc: 23.77 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

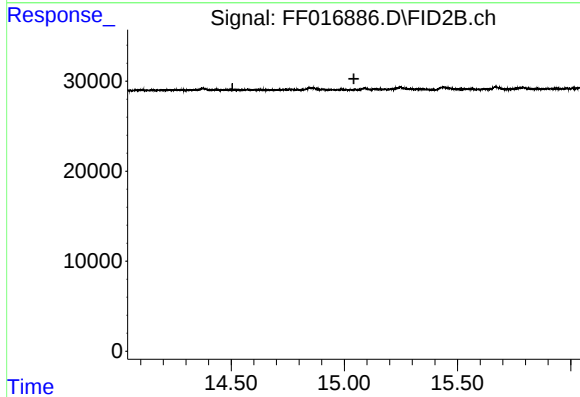


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 15.042 min  
Response: 0  
Conc: N.D.

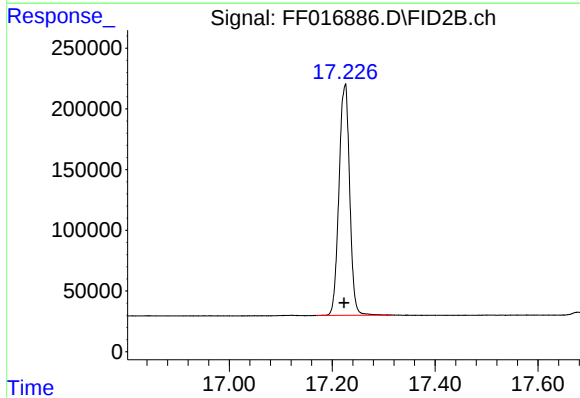


#12 N-OCTACOSANE

R.T.: 17.225 min  
Delta R.T.: 0.002 min  
Response: 2742634  
Conc: 25.85 ug/ml

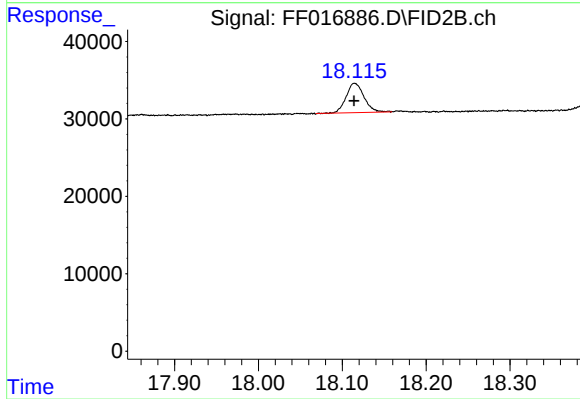

#13 N-TRIACONTANE


R.T.: 18.115 min  
Delta R.T.: 0.000 min  
Response: 56100  
Conc: 0.52 ug/ml

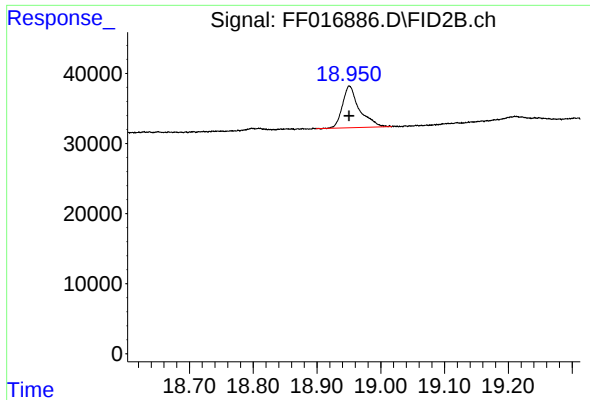

#14 N-DOTRIACONTANE

R.T.: 18.951 min  
Delta R.T.: 0.000 min  
Response: 109776  
Conc: 1.04 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

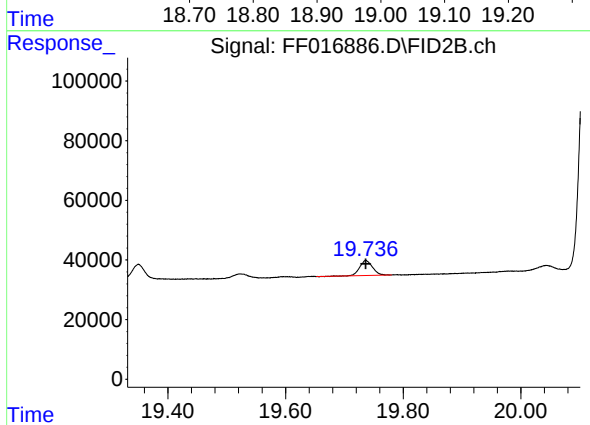

#15 N-TETRATRIACONTANE

R.T.: 19.737 min  
Delta R.T.: 0.000 min  
Response: 76555  
Conc: 0.77 ug/ml