

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121119\
 Data File : FG006344.D
 Signal(s) : FID1A.ch
 Acq On : 11 Dec 2019 20:47
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 12 01:02:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112619.M
 Quant Title :
 QLast Update : Wed Nov 27 02:46:06 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.494	4282534	54.555 ug/ml
Target Compounds			
2) N-DECANE	4.417	5331283	55.245 ug/ml
3) N-DODECANE	6.400	5441985	55.807 ug/ml
4) N-TETRADECANE	8.160	5421881	55.700 ug/ml
5) N-HEXADECANE	9.729	5426010	55.495 ug/ml
6) N-OCTADECANE	11.145	5299767	55.260 ug/ml
7) N-EICOSANE	12.432	5212718	54.722 ug/ml
8) N-DOCOSANE	13.611	5027492	54.141 ug/ml
10) N-TETRACOSANE	14.696	4903130	53.858 ug/ml
11) N-HEXACOSANE	15.698	4832079	53.834 ug/ml
12) N-OCTACOSANE	16.631	4849637	52.745 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121119\
Data File : FG006344.D
Signal(s) : FID1A.ch
Acq On : 11 Dec 2019 20:47
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 12 01:02:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112619.M
Quant Title :
QLast Update : Wed Nov 27 02:46:06 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

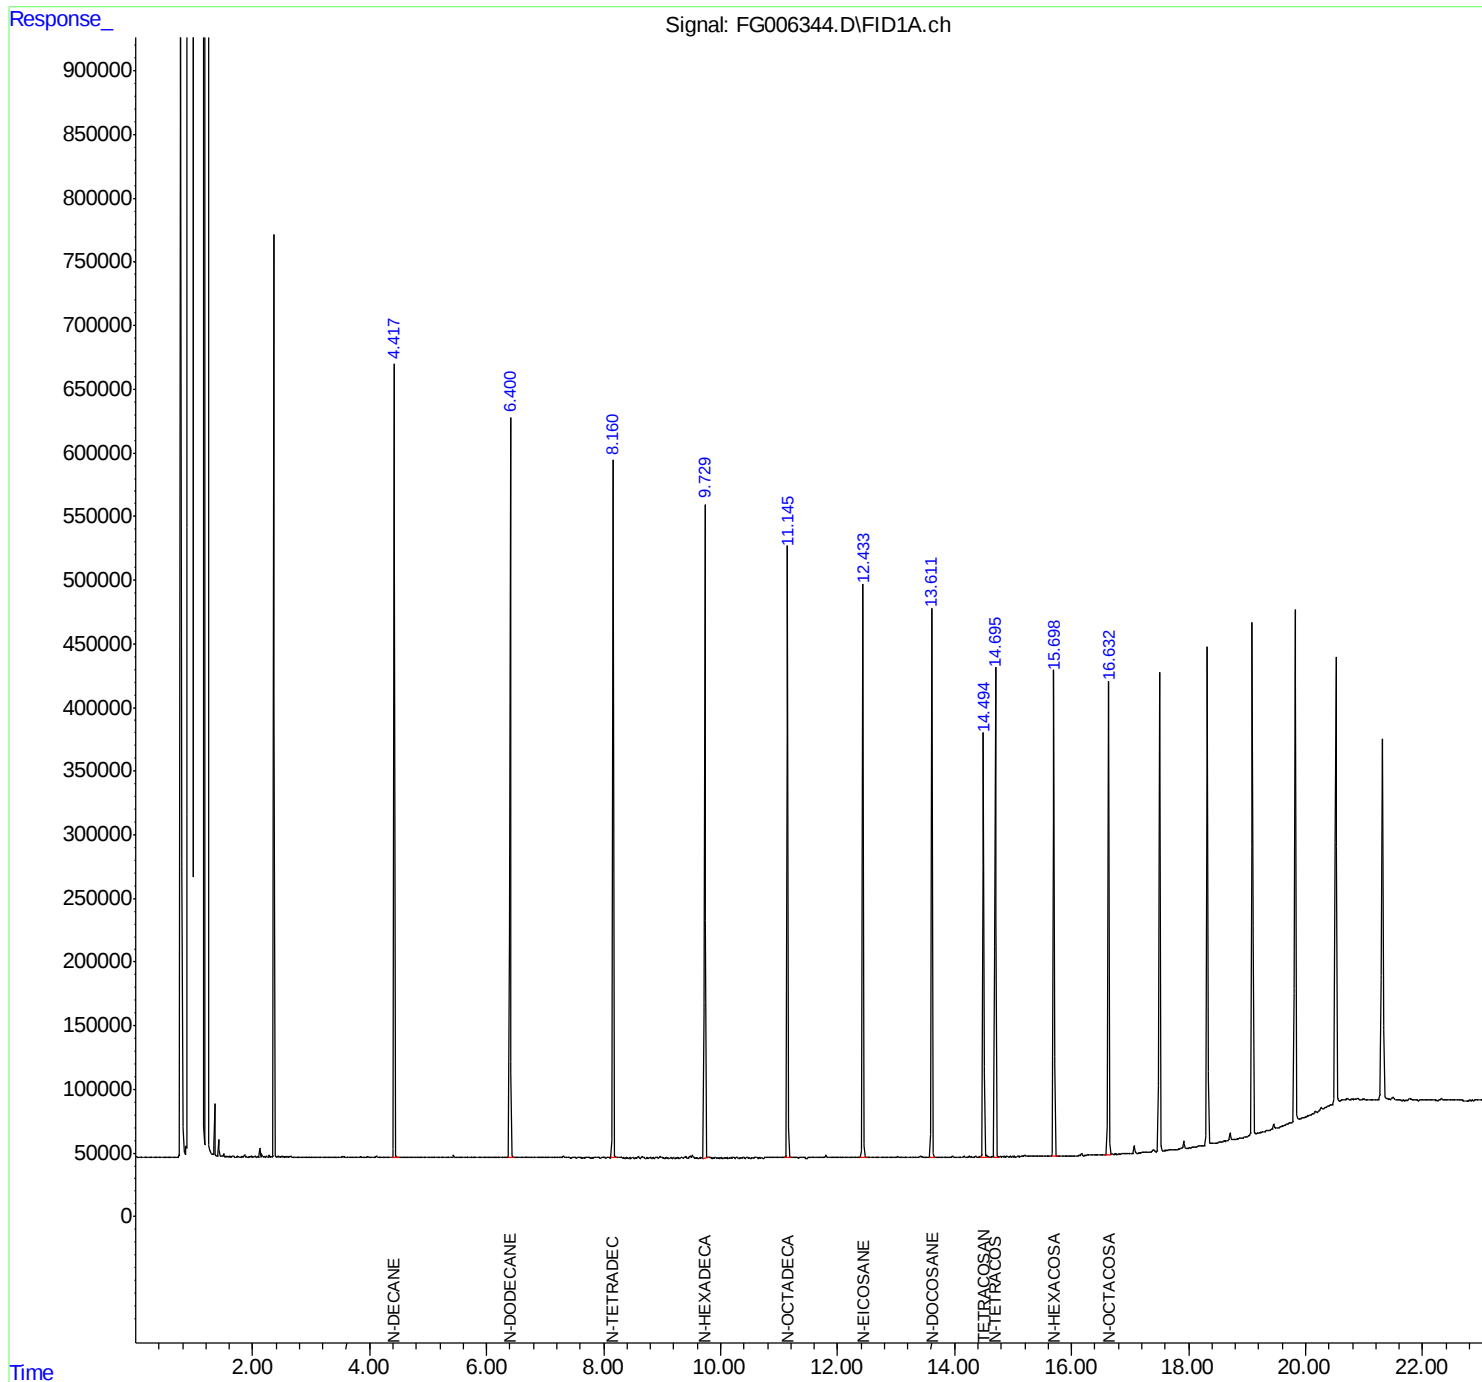

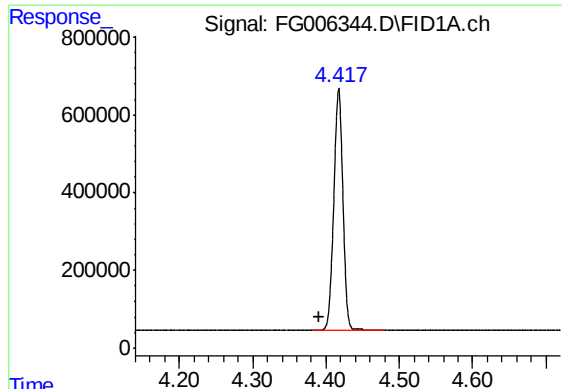


#2 N-DECANE

R.T.: 4.417 min
Delta R.T.: 0.028 min
Response: 5331283
Conc: 55.24 ug/ml

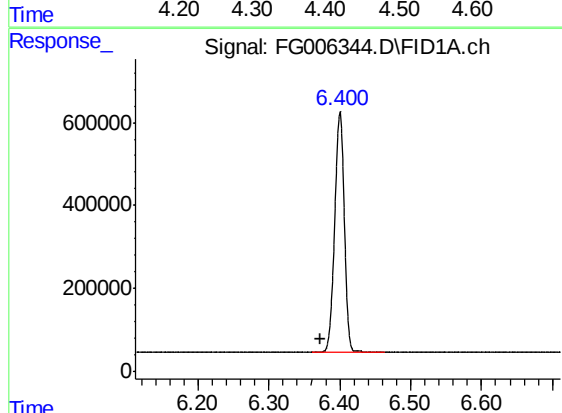


#3 N-DODECANE

R.T.: 6.400 min
Delta R.T.: 0.027 min
Response: 5441985
Conc: 55.81 ug/ml

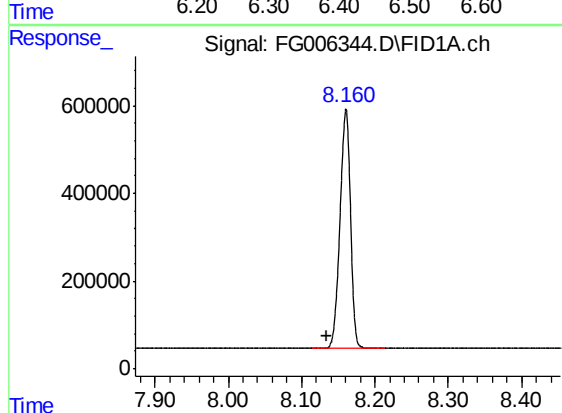


#4 N-TETRADECANE

R.T.: 8.160 min
Delta R.T.: 0.026 min
Response: 5421881
Conc: 55.70 ug/ml

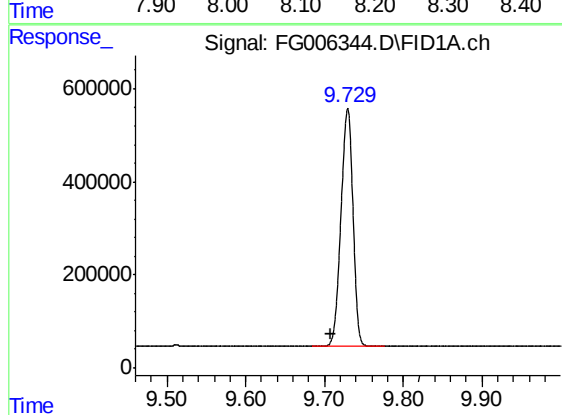


#5 N-HEXADECANE

R.T.: 9.729 min
Delta R.T.: 0.022 min
Response: 5426010
Conc: 55.49 ug/ml

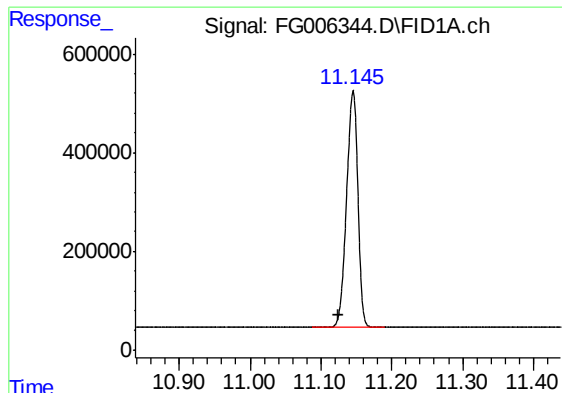


#6 N-OCTADECANE

R.T.: 11.145 min
Delta R.T.: 0.021 min
Response: 5299767
Conc: 55.26 ug/ml

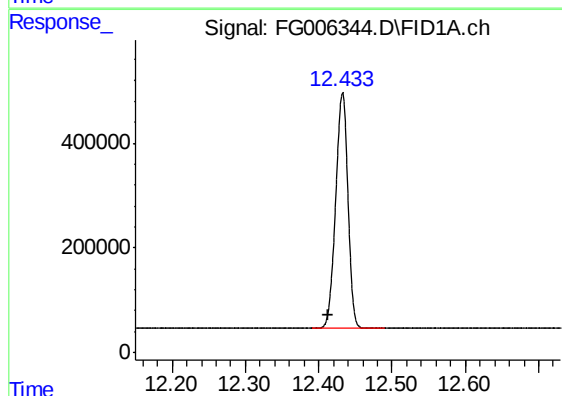


#7 N-EICOSANE

R.T.: 12.432 min
Delta R.T.: 0.019 min
Response: 5212718
Conc: 54.72 ug/ml

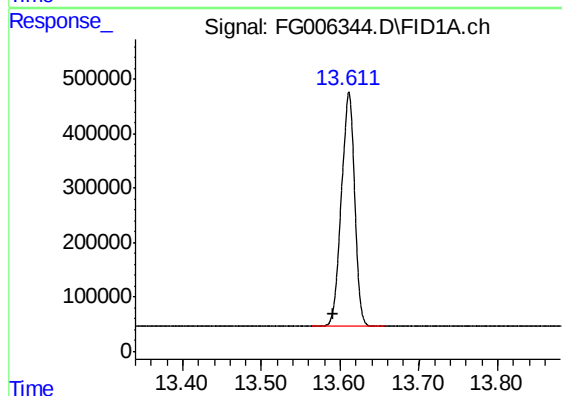


#8 N-DOCOSANE

R.T.: 13.611 min
Delta R.T.: 0.019 min
Response: 5027492
Conc: 54.14 ug/ml

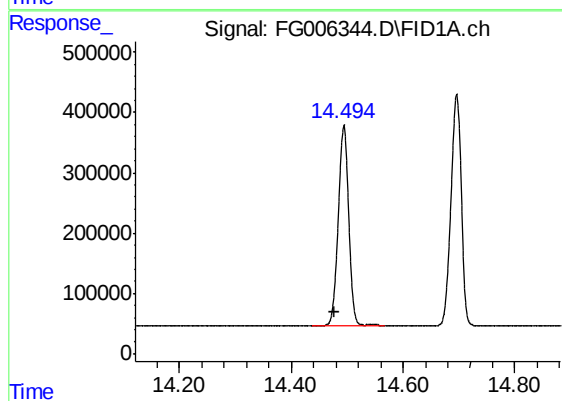


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.494 min
Delta R.T.: 0.018 min
Response: 4282534
Conc: 54.56 ug/ml

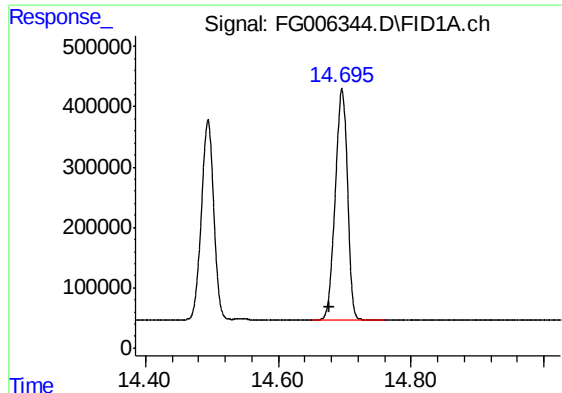


#10 N-TETRACOSANE

R.T.: 14.696 min
Delta R.T.: 0.019 min
Response: 4903130
Conc: 53.86 ug/ml

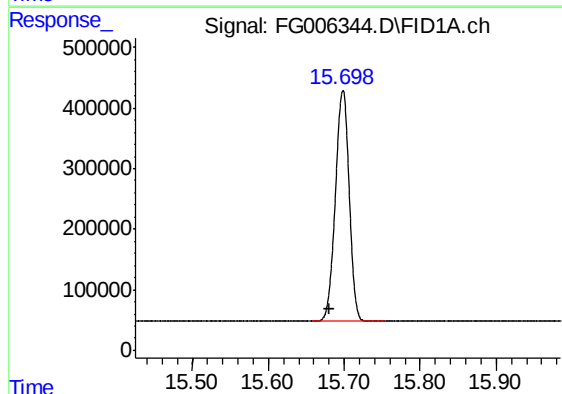

#11 N-HEXACOSANE

R.T.: 15.698 min
Delta R.T.: 0.018 min
Response: 4832079
Conc: 53.83 ug/ml

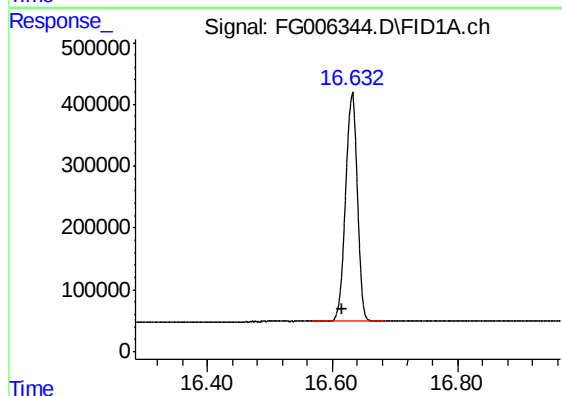

#12 N-OCTACOSANE

R.T.: 16.631 min
Delta R.T.: 0.016 min
Response: 4849637
Conc: 52.75 ug/ml