

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121418\
 Data File : FG003259.D
 Signal(s) : FID1A.ch
 Acq On : 13 Dec 2018 15:51
 Operator : AJ\SJ
 Sample : PB115632BS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 14 00:58:50 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121318.M
 Quant Title :
 QLast Update : Thu Dec 13 00:59:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.702	2637026	21.261 ug/ml
Target Compounds			
2) N-DECANE	4.409	2818788	21.009 ug/ml
3) N-DODECANE	6.435	2867961	21.080 ug/ml
4) N-TETRADECANE	8.234	2940450	21.307 ug/ml
5) N-HEXADECANE	9.838	2985910	21.312 ug/ml
6) N-OCTADECANE	11.283	3017044	21.295 ug/ml
7) N-EICOSANE	12.597	3003093	21.257 ug/ml
8) N-DOCOSANE	13.798	2980270	21.189 ug/ml
10) N-TETRACOSANE	14.906	2951270	21.085 ug/ml
11) N-HEXACOSANE	15.930	2936332	21.067 ug/ml
12) N-OCTACOSANE	16.883	2925125	20.933 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121418\
Data File : FG003259.D
Signal(s) : FID1A.ch
Acq On : 13 Dec 2018 15:51
Operator : AJ\SJ
Sample : PB115632BS
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 14 00:58:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121318.M
Quant Title :
QLast Update : Thu Dec 13 00:59:54 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

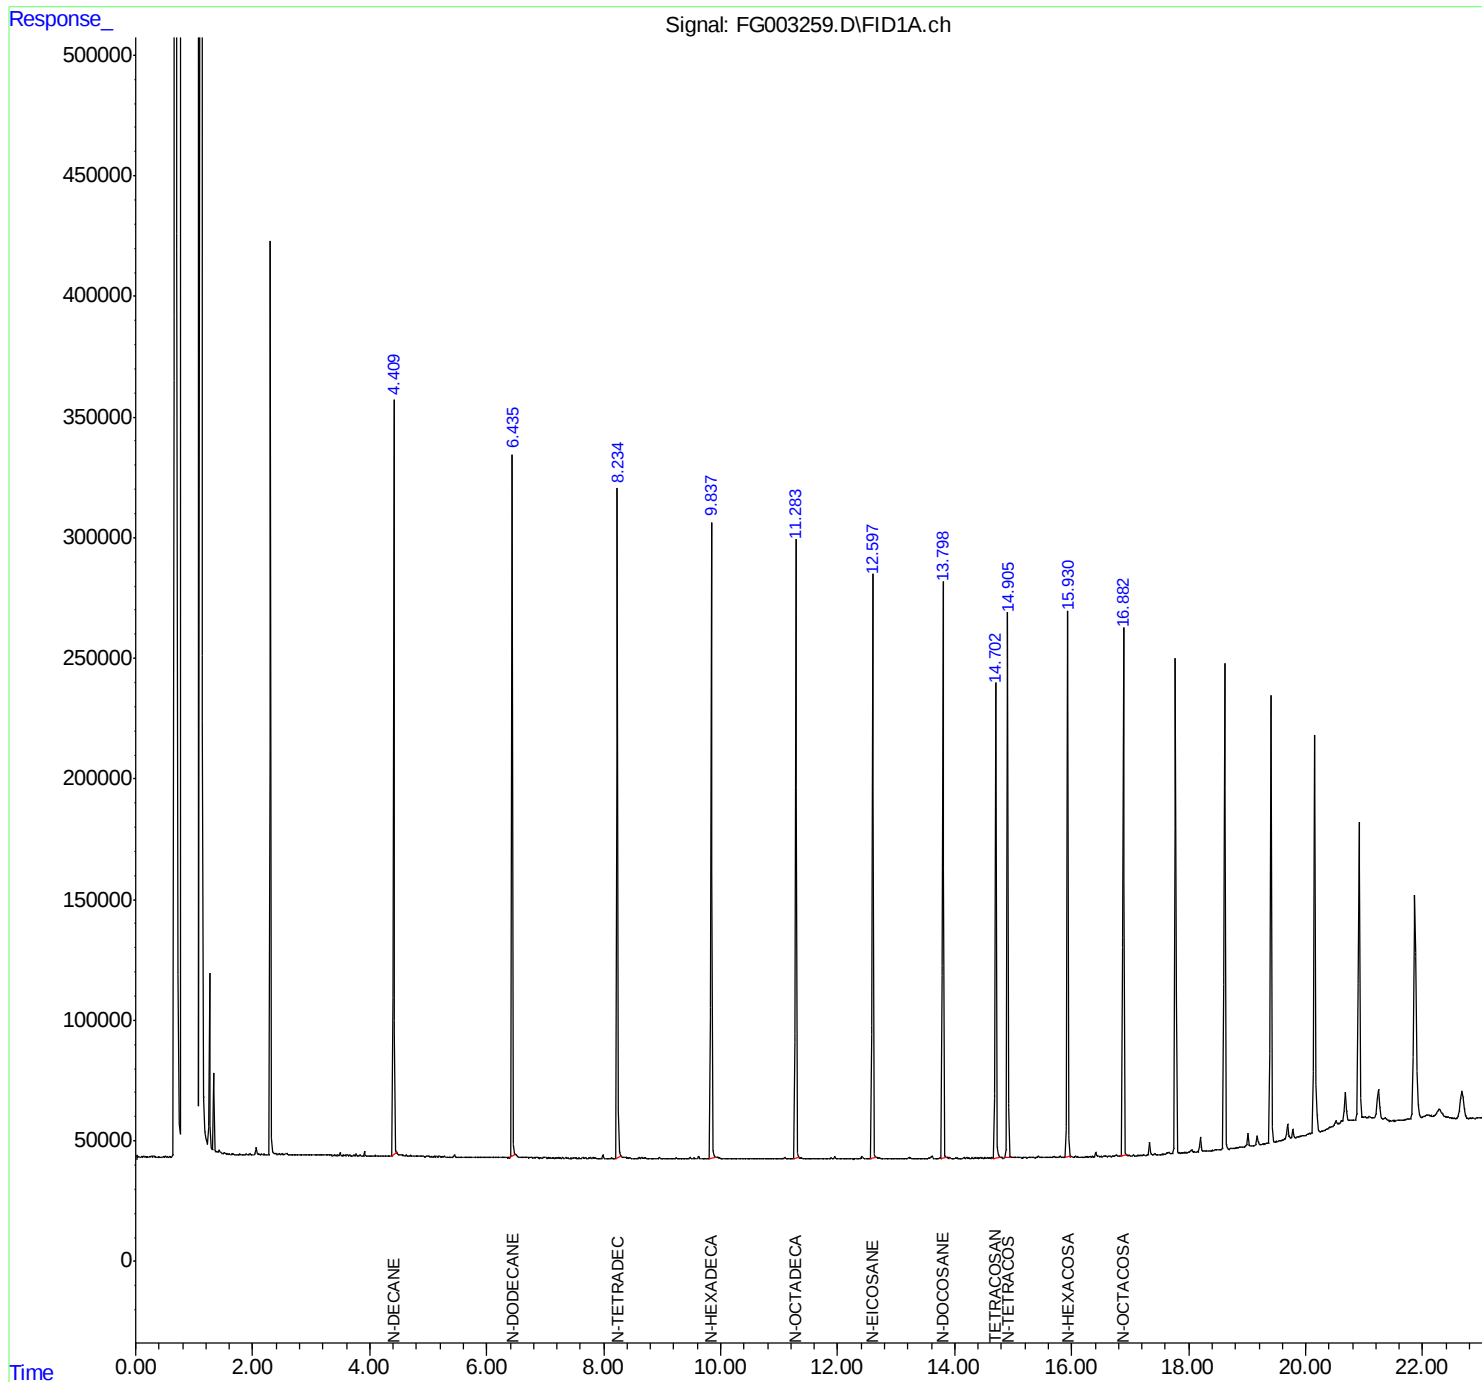

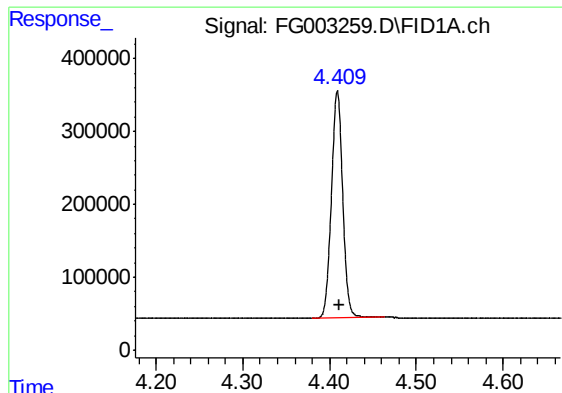


#2 N-DECANE

R.T.: 4.409 min
Delta R.T.: -0.002 min
Response: 2818788
Conc: 21.01 ug/ml

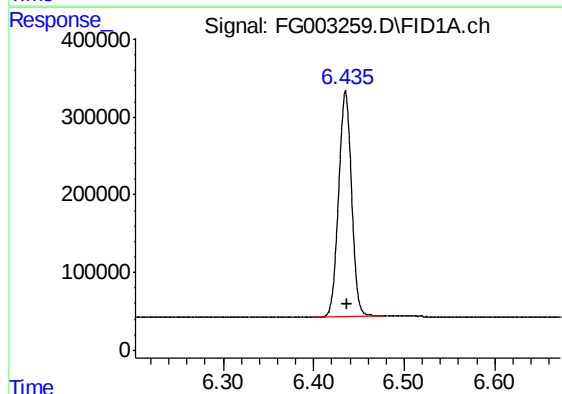


#3 N-DODECANE

R.T.: 6.435 min
Delta R.T.: -0.001 min
Response: 2867961
Conc: 21.08 ug/ml

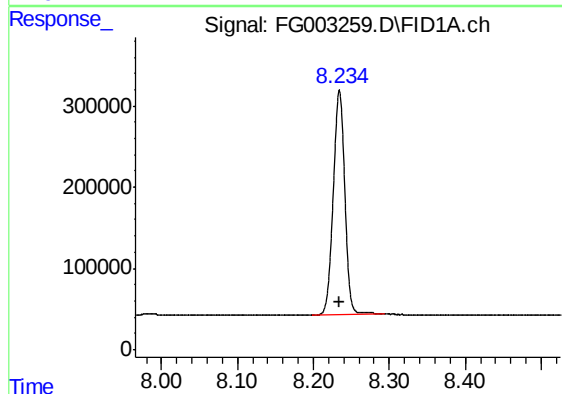


#4 N-TETRADECANE

R.T.: 8.234 min
Delta R.T.: 0.000 min
Response: 2940450
Conc: 21.31 ug/ml

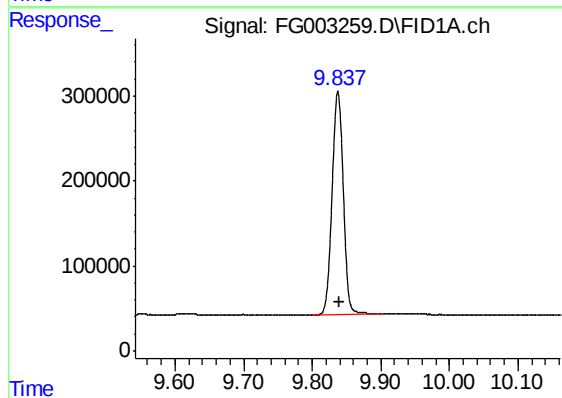


#5 N-HEXADECANE

R.T.: 9.838 min
Delta R.T.: -0.002 min
Response: 2985910
Conc: 21.31 ug/ml

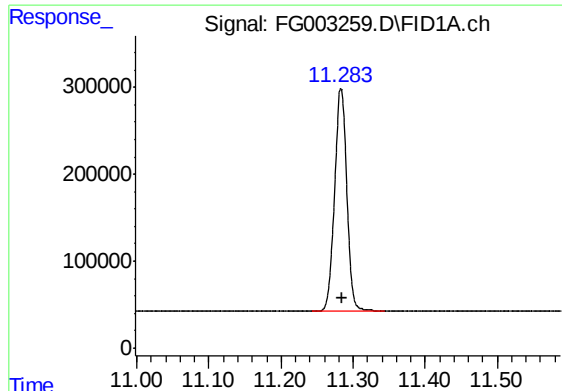


#6 N-OCTADECANE

R.T.: 11.283 min
Delta R.T.: -0.002 min
Response: 3017044
Conc: 21.30 ug/ml

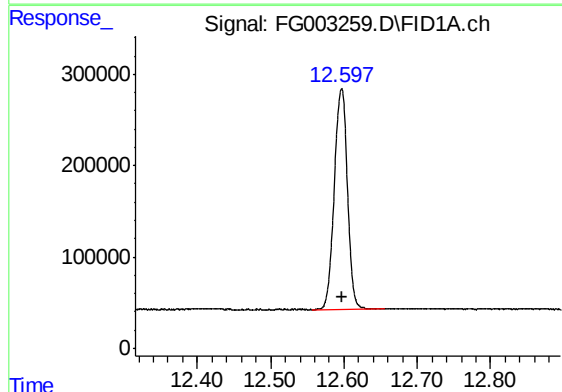


#7 N-EICOSANE

R.T.: 12.597 min
Delta R.T.: -0.001 min
Response: 3003093
Conc: 21.26 ug/ml

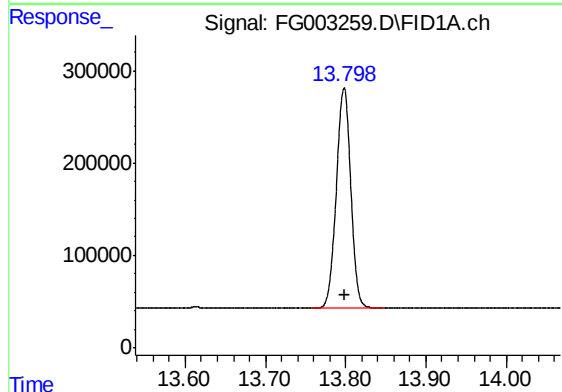


#8 N-DOCOSANE

R.T.: 13.798 min
Delta R.T.: -0.001 min
Response: 2980270
Conc: 21.19 ug/ml

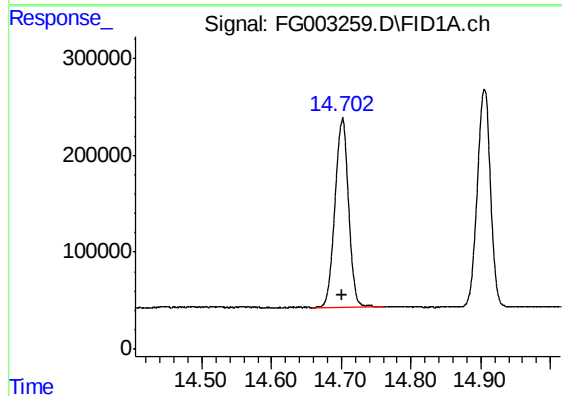


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.702 min
Delta R.T.: 0.000 min
Response: 2637026
Conc: 21.26 ug/ml

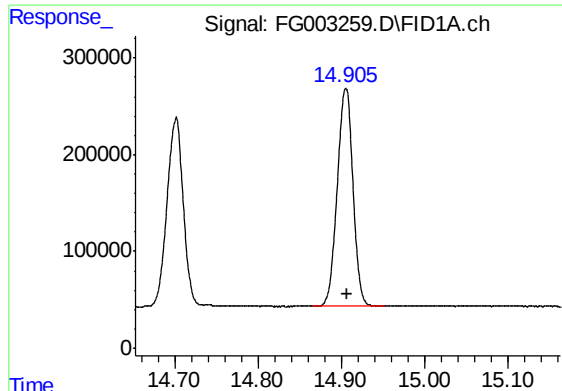


#10 N-TETRACOSANE

R.T.: 14.906 min
Delta R.T.: -0.001 min
Response: 2951270
Conc: 21.08 ug/ml

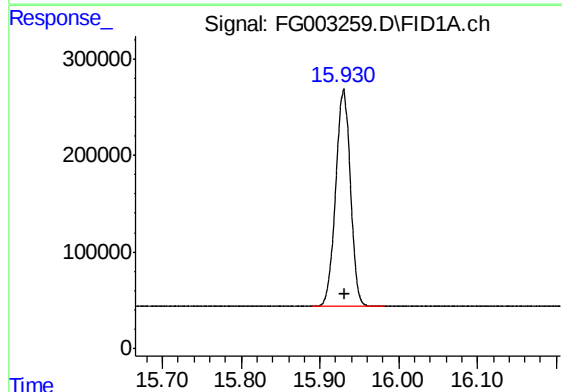

#11 N-HEXACOSANE

R.T.: 15.930 min
Delta R.T.: -0.001 min
Response: 2936332
Conc: 21.07 ug/ml

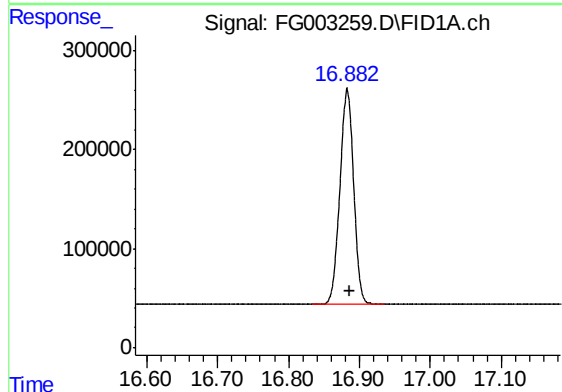

#12 N-OCTACOSANE

R.T.: 16.883 min
Delta R.T.: -0.003 min
Response: 2925125
Conc: 20.93 ug/ml