

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121420\
Data File : FG007463.D
Signal(s) : FID1A.ch
Acq On : 14 Dec 2020 11:12
Operator : DD\AJ
Sample : L5043-06RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
KENS-SS2-121020-0-7RE

Integration File: autoint1.e
Quant Time: Dec 15 00:19:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG120220.M
Quant Title :
QLast Update : Thu Dec 03 08:50:10 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.730	4178202	32.585 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121420\
Data File : FG007463.D
Signal(s) : FID1A.ch
Acq On : 14 Dec 2020 11:12
Operator : DD\AJ
Sample : L5043-06RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
KENS-SS2-121020-0-7RE

Integration File: autoint1.e
Quant Time: Dec 15 00:19:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG120220.M
Quant Title :
QLast Update : Thu Dec 03 08:50:10 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

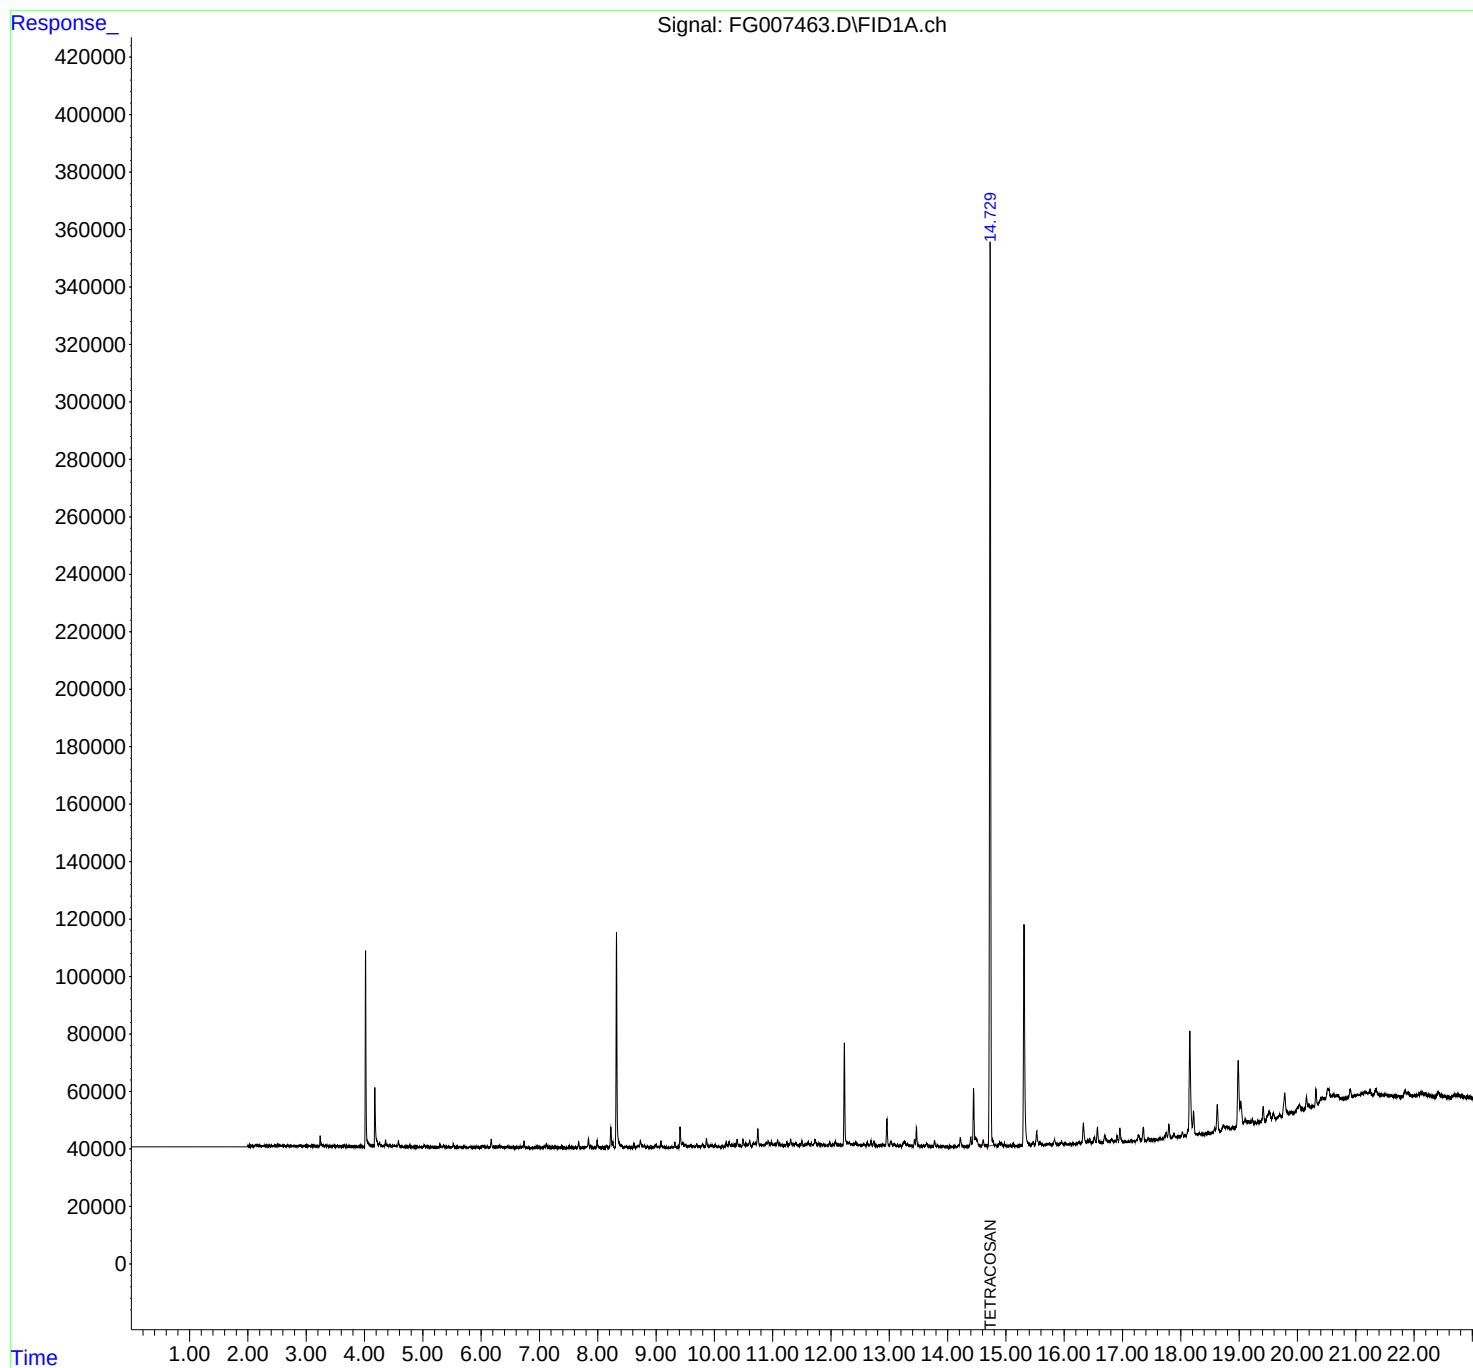

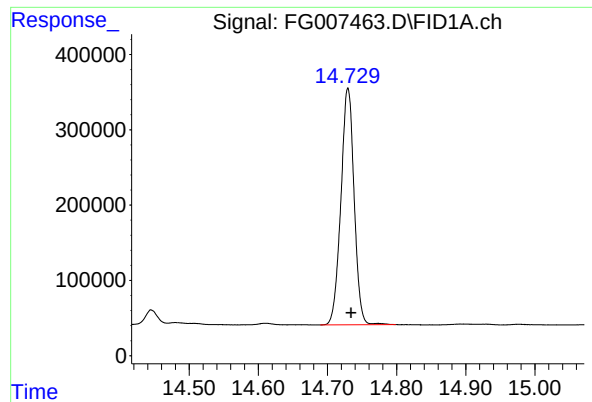

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.730 min
Delta R.T.: -0.004 min
Response: 4178202
Conc: 32.58 ug/ml

Instrument :
FID_G
ClientSampleId :
KENS-SS2-121020-0-7RE