

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121521\
Data File : FG009287.D
Signal(s) : FID1A.ch
Acq On : 15 Dec 2021 20:25
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 16 05:05:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121521.M
Quant Title :
QLast Update : Thu Dec 16 05:01:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.518	2619425	18.965 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.412	45961	0.343 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121521\
Data File : FG009287.D
Signal(s) : FID1A.ch
Acq On : 15 Dec 2021 20:25
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 16 05:05:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121521.M
Quant Title :
QLast Update : Thu Dec 16 05:01:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

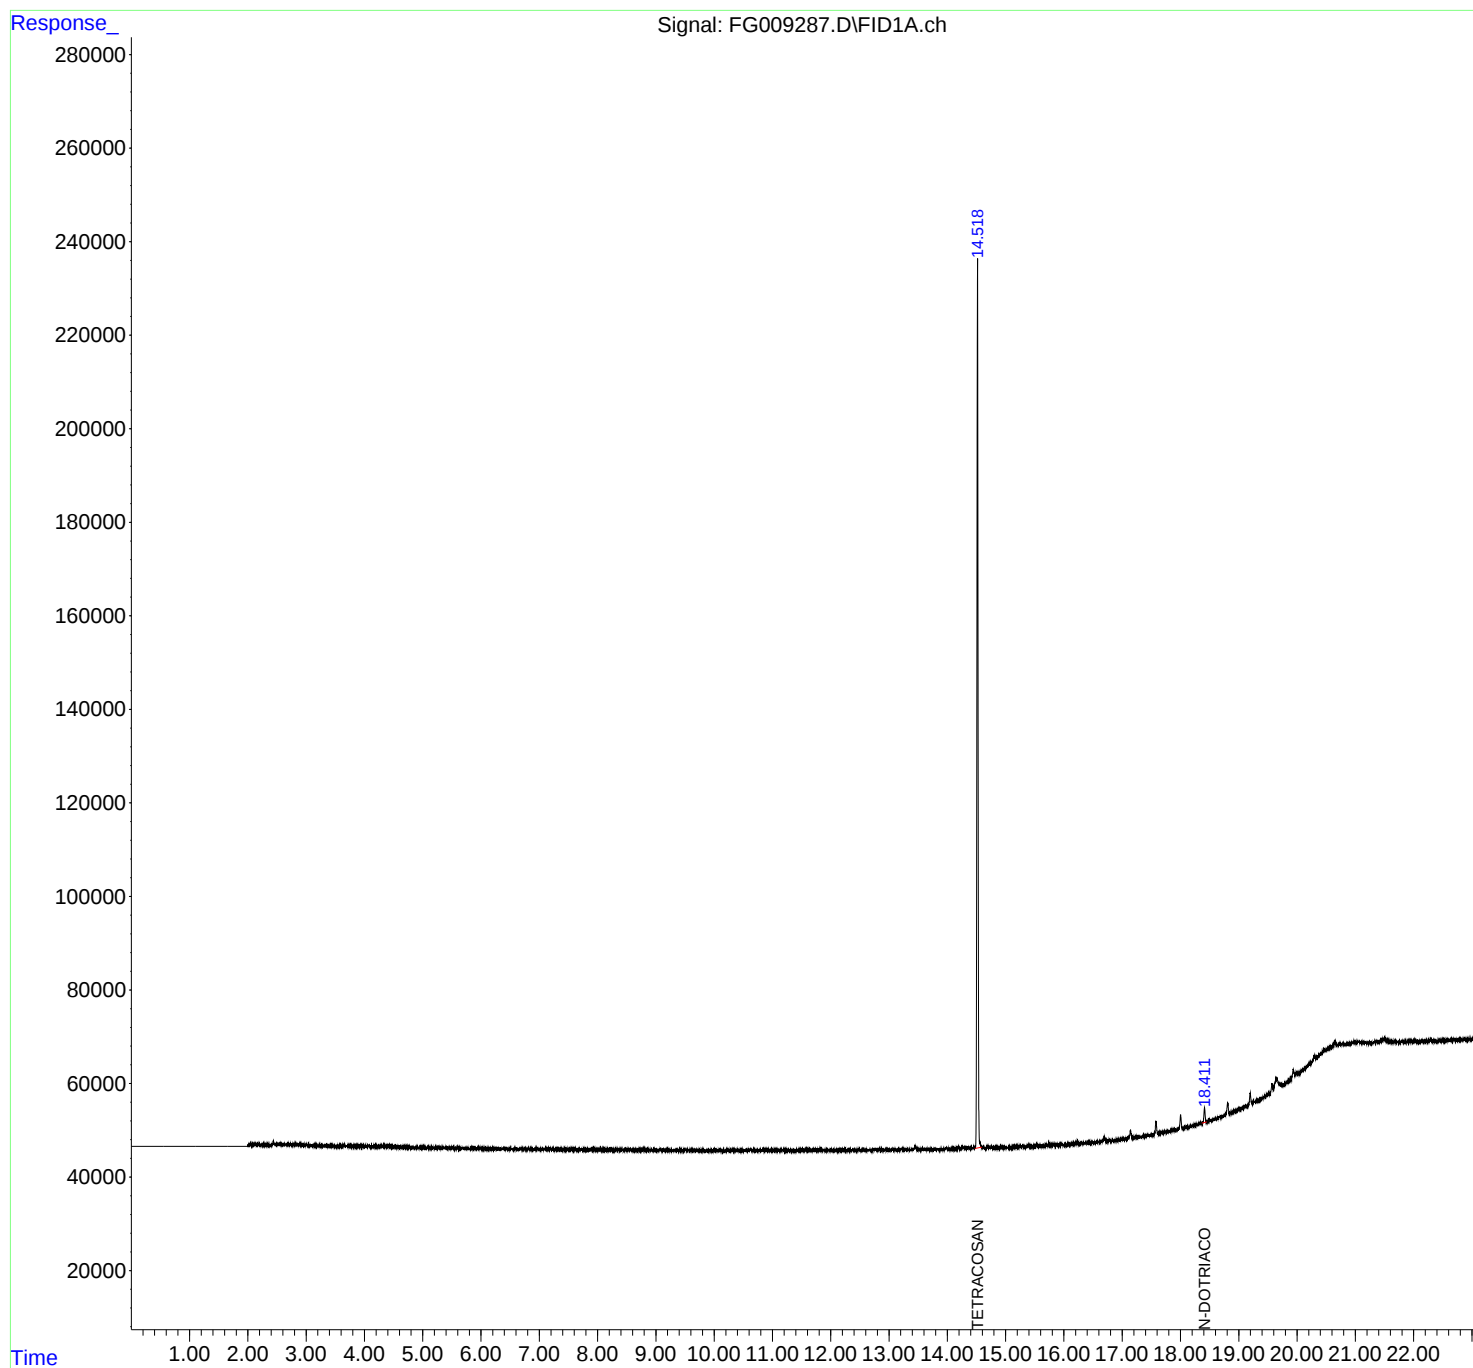


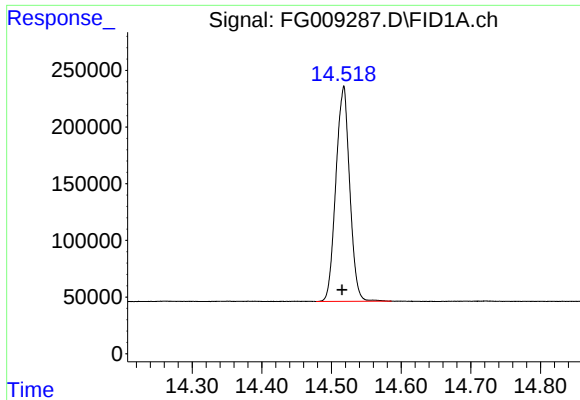

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.518 min
Delta R.T.: 0.002 min
Response: 2619425
Conc: 18.96 ug/ml

Instrument :
FID_G
ClientSampleId :

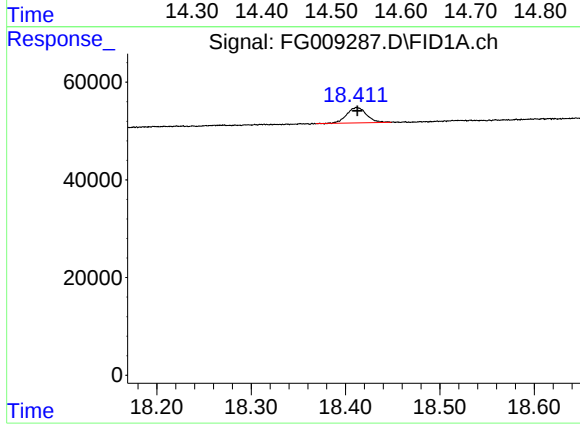

#14 N-DOTRIACONTANE

R.T.: 18.412 min
Delta R.T.: 0.000 min
Response: 45961
Conc: 0.34 ug/ml