

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121521\
Data File : FG009289.D
Signal(s) : FID1A.ch
Acq On : 15 Dec 2021 21:26
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 16 05:06:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121521.M
Quant Title :
QLast Update : Thu Dec 16 05:01:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.263	1392841	8.849 ug/ml
12)	N-OCTACOSANE	16.692	1372982	9.175 ug/ml
13)	N-TRIACONTANE	17.579	65498	0.457 ug/ml
14)	N-DOTRIACONTANE	18.412	80150	0.598 ug/ml
15)	N-TETRATRIACONTANE	19.195	68479	0.546 ug/ml
16)	N-HEXATRIACONTANE	19.935	41614	0.360 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121521\
Data File : FG009289.D
Signal(s) : FID1A.ch
Acq On : 15 Dec 2021 21:26
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 16 05:06:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121521.M
Quant Title :
QLast Update : Thu Dec 16 05:01:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

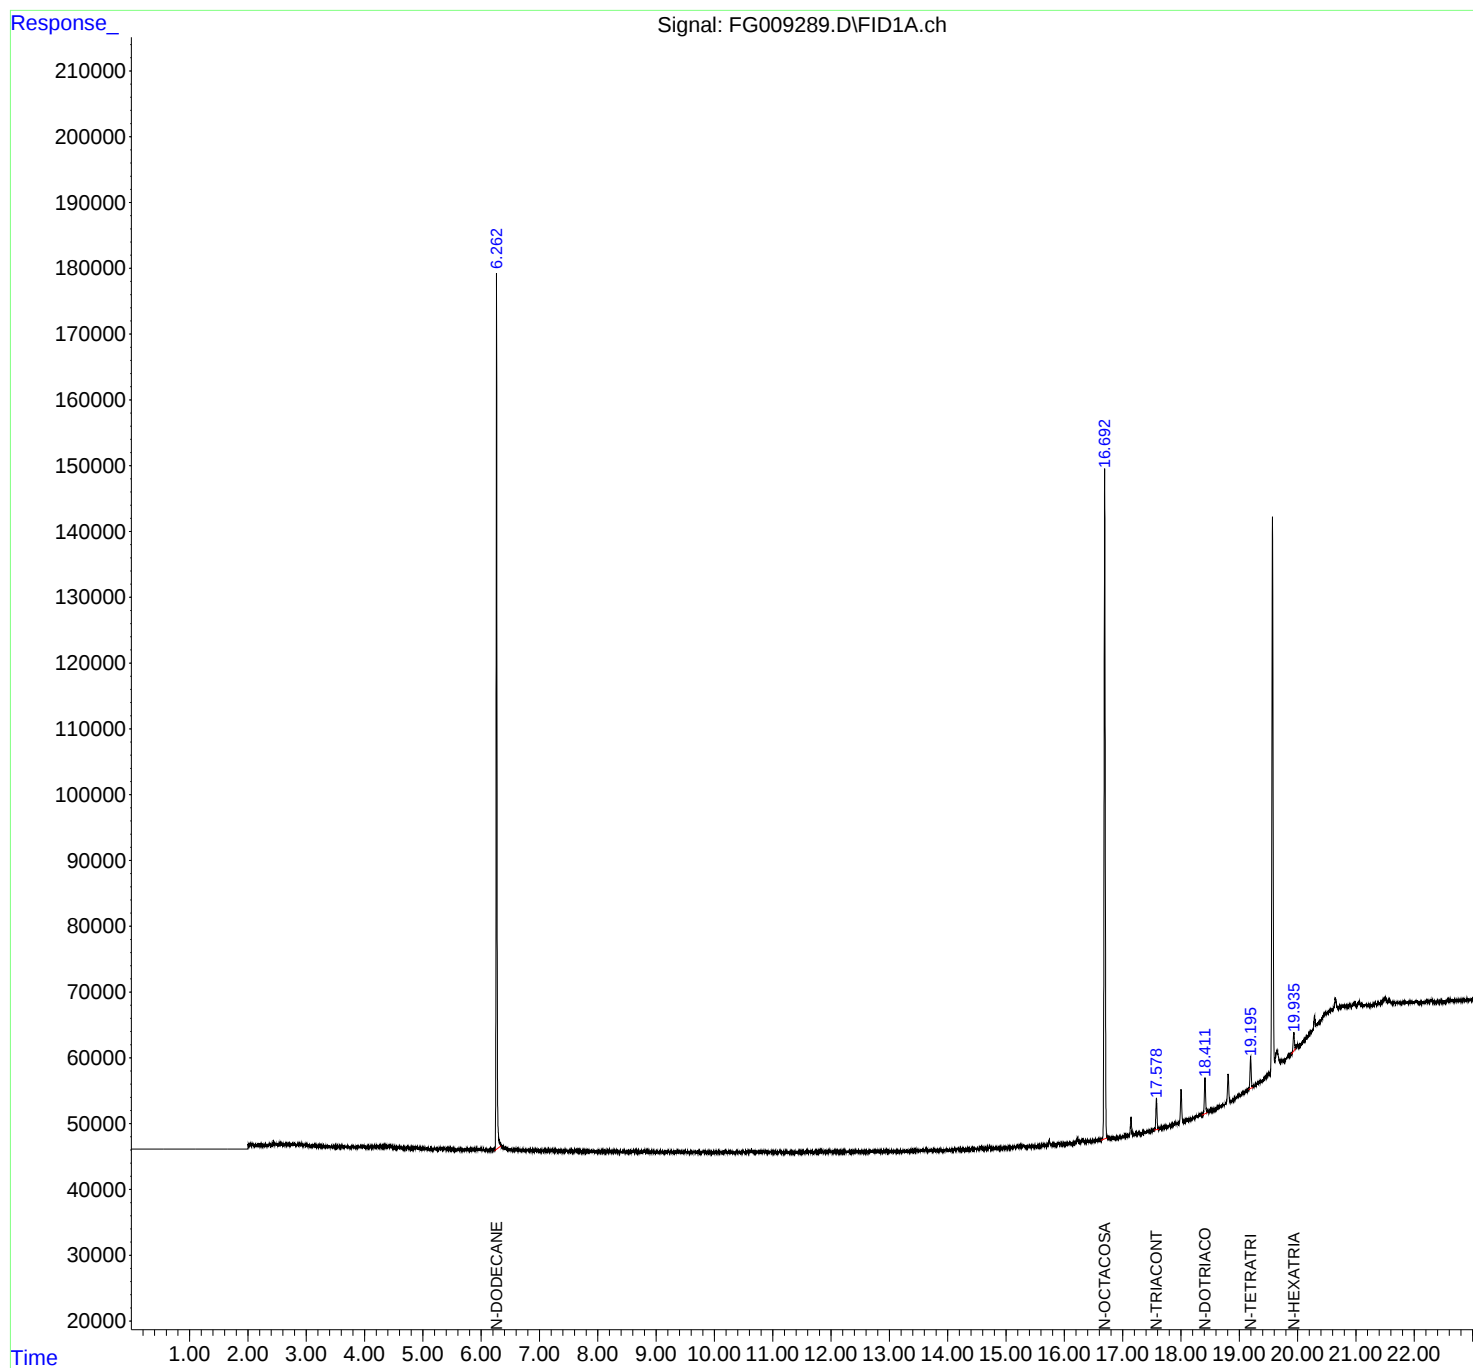


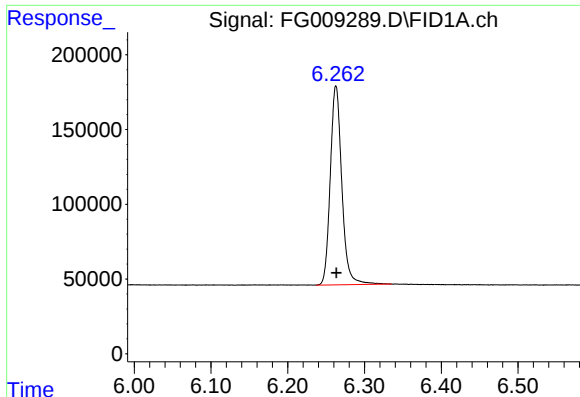

#3 N-DODECANE


R.T.: 6.263 min
Delta R.T.: 0.000 min
Response: 1392841
Conc: 8.85 ug/ml

Instrument :
FID_G
ClientSampleId :

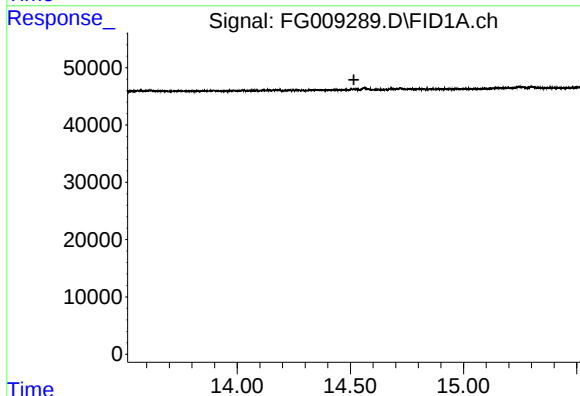


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.515 min
Response: 0
Conc: N.D.

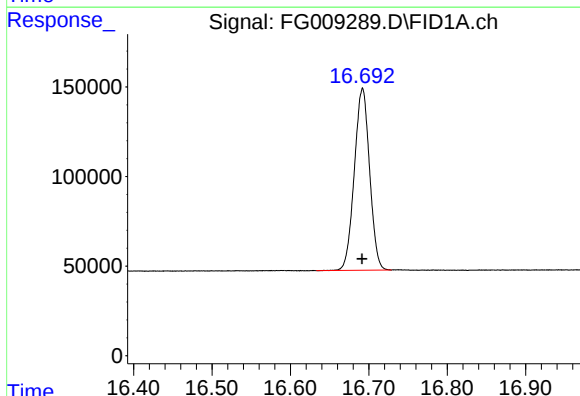


#12 N-OCTACOSANE

R.T.: 16.692 min
Delta R.T.: 0.000 min
Response: 1372982
Conc: 9.18 ug/ml

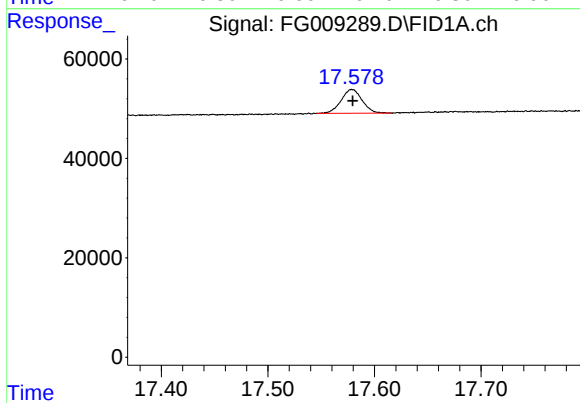

#13 N-TRIACONTANE


R.T.: 17.579 min
Delta R.T.: 0.000 min
Response: 65498
Conc: 0.46 ug/ml

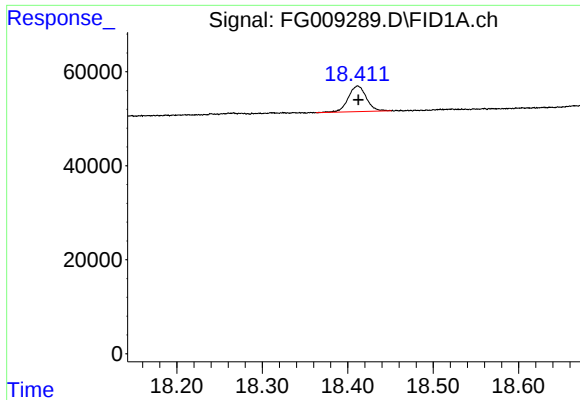

#14 N-DOTRIACONTANE


R.T.: 18.412 min
Delta R.T.: 0.000 min
Response: 80150
Conc: 0.60 ug/ml

Instrument :
FID_G
ClientSampleId :

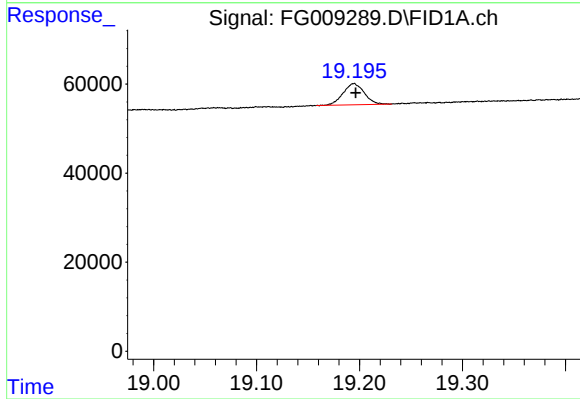

#15 N-TETRATRIACONTANE

R.T.: 19.195 min
Delta R.T.: -0.001 min
Response: 68479
Conc: 0.55 ug/ml

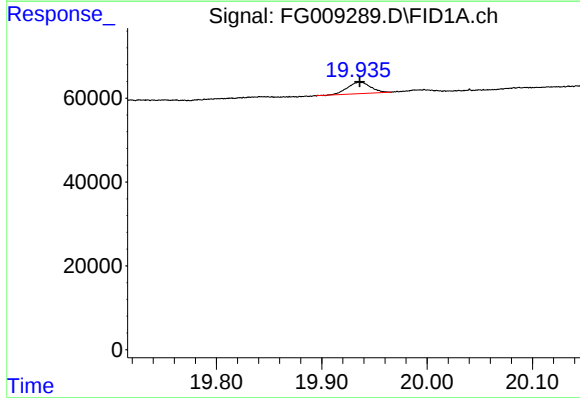

#16 N-HEXATRIACONTANE

R.T.: 19.935 min
Delta R.T.: 0.000 min
Response: 41614
Conc: 0.36 ug/ml