

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121521\
 Data File : FG009292.D
 Signal(s) : FID1A.ch
 Acq On : 15 Dec 2021 22:58
 Operator : AJ\MA
 Sample : M5064-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 16 05:07:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121521.M
 Quant Title :
 QLast Update : Thu Dec 16 05:01:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.516	2088630	15.122 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.736	79295	0.530 ug/ml
13) N-TRIACONTANE	17.579	63550	0.443 ug/ml
14) N-DOTRIACONTANE	18.410	79046	0.590 ug/ml
15) N-TETRATRIACONTANE	19.197	53902	0.430 ug/ml
16) N-HEXATRIACONTANE	19.937	51035	0.442 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121521\
Data File : FG009292.D
Signal(s) : FID1A.ch
Acq On : 15 Dec 2021 22:58
Operator : AJ\MA
Sample : M5064-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 16 05:07:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121521.M
Quant Title :
QLast Update : Thu Dec 16 05:01:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

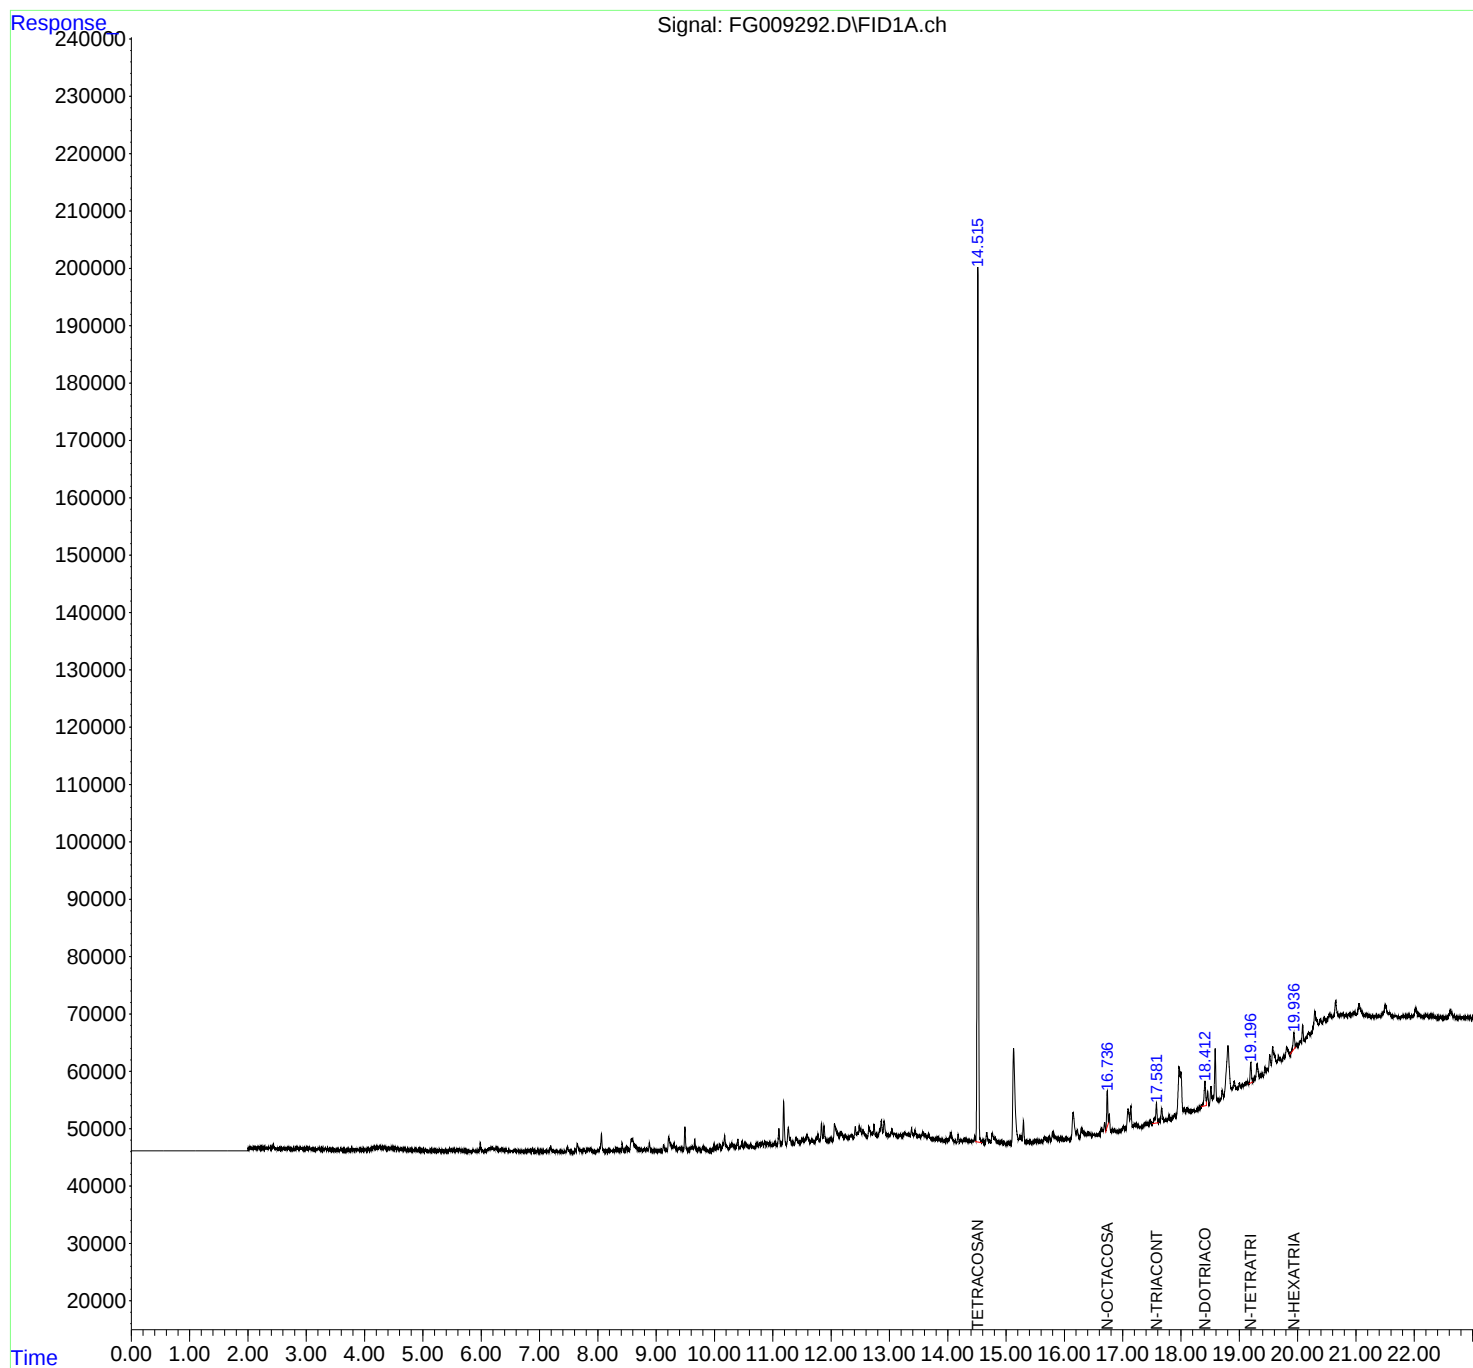


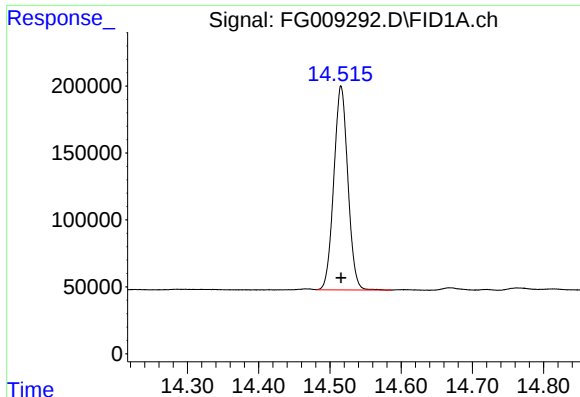

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.516 min
Delta R.T.: 0.000 min
Response: 2088630
Conc: 15.12 ug/ml

Instrument :
FID_G
ClientSampleId :

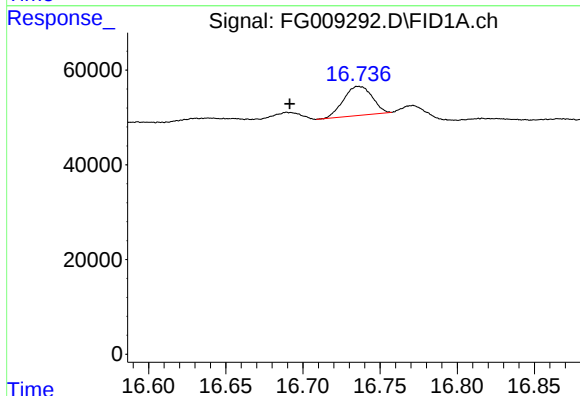


#12 N-OCTACOSANE

R.T.: 16.736 min
Delta R.T.: 0.044 min
Response: 79295
Conc: 0.53 ug/ml

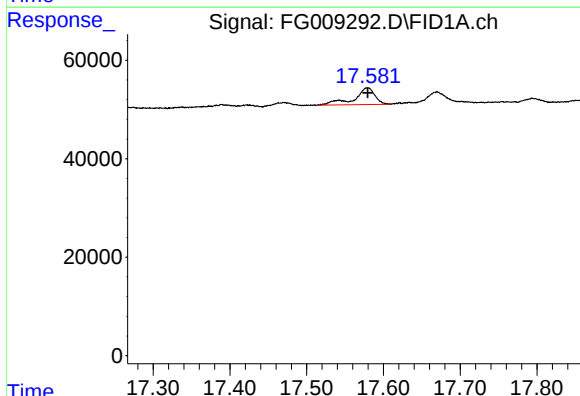


#13 N-TRIACONTANE

R.T.: 17.579 min
Delta R.T.: 0.000 min
Response: 63550
Conc: 0.44 ug/ml

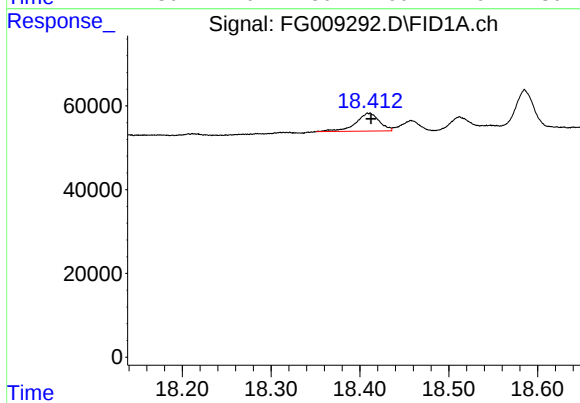

#14 N-DOTRIACONTANE


R.T.: 18.410 min
Delta R.T.: -0.002 min
Response: 79046
Conc: 0.59 ug/ml

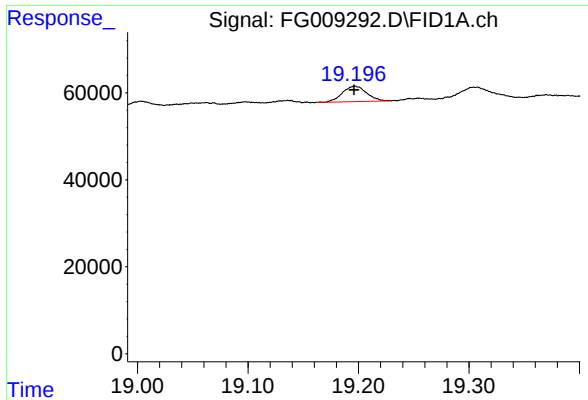

#15 N-TETRATRIACONTANE

R.T.: 19.197 min
Delta R.T.: 0.000 min
Response: 53902
Conc: 0.43 ug/ml

Instrument :
FID_G
ClientSampleId :

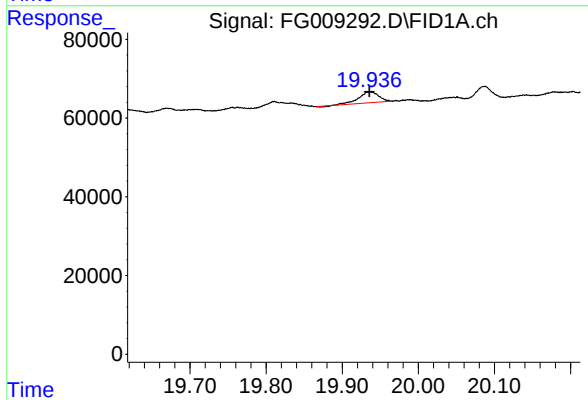

#16 N-HEXATRIACONTANE

R.T.: 19.937 min
Delta R.T.: 0.000 min
Response: 51035
Conc: 0.44 ug/ml