

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121521\
 Data File : FG009293.D
 Signal(s) : FID1A.ch
 Acq On : 15 Dec 2021 23:29
 Operator : AJ\MA
 Sample : M5064-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 16 05:07:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121521.M
 Quant Title :
 QLast Update : Thu Dec 16 05:01:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.517	2052325	14.859 ug/ml
Target Compounds			
4) N-TETRADECANE	8.060	66437	0.413 ug/ml
6) N-OCTADECANE	11.104	56558	0.348 ug/ml
11) N-HEXACOSANE	15.741	53852	0.349 ug/ml
12) N-OCTACOSANE	16.691	50596	0.338 ug/ml
13) N-TRIACONTANE	17.579	99812	0.696 ug/ml
14) N-DOTRIACONTANE	18.411	103728	0.774 ug/ml
15) N-TETRATRIACONTANE	19.197	59628	0.476 ug/ml
16) N-HEXATRIACONTANE	19.938	47333	0.410 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121521\
Data File : FG009293.D
Signal(s) : FID1A.ch
Acq On : 15 Dec 2021 23:29
Operator : AJ\MA
Sample : M5064-02
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 16 05:07:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121521.M
Quant Title :
QLast Update : Thu Dec 16 05:01:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

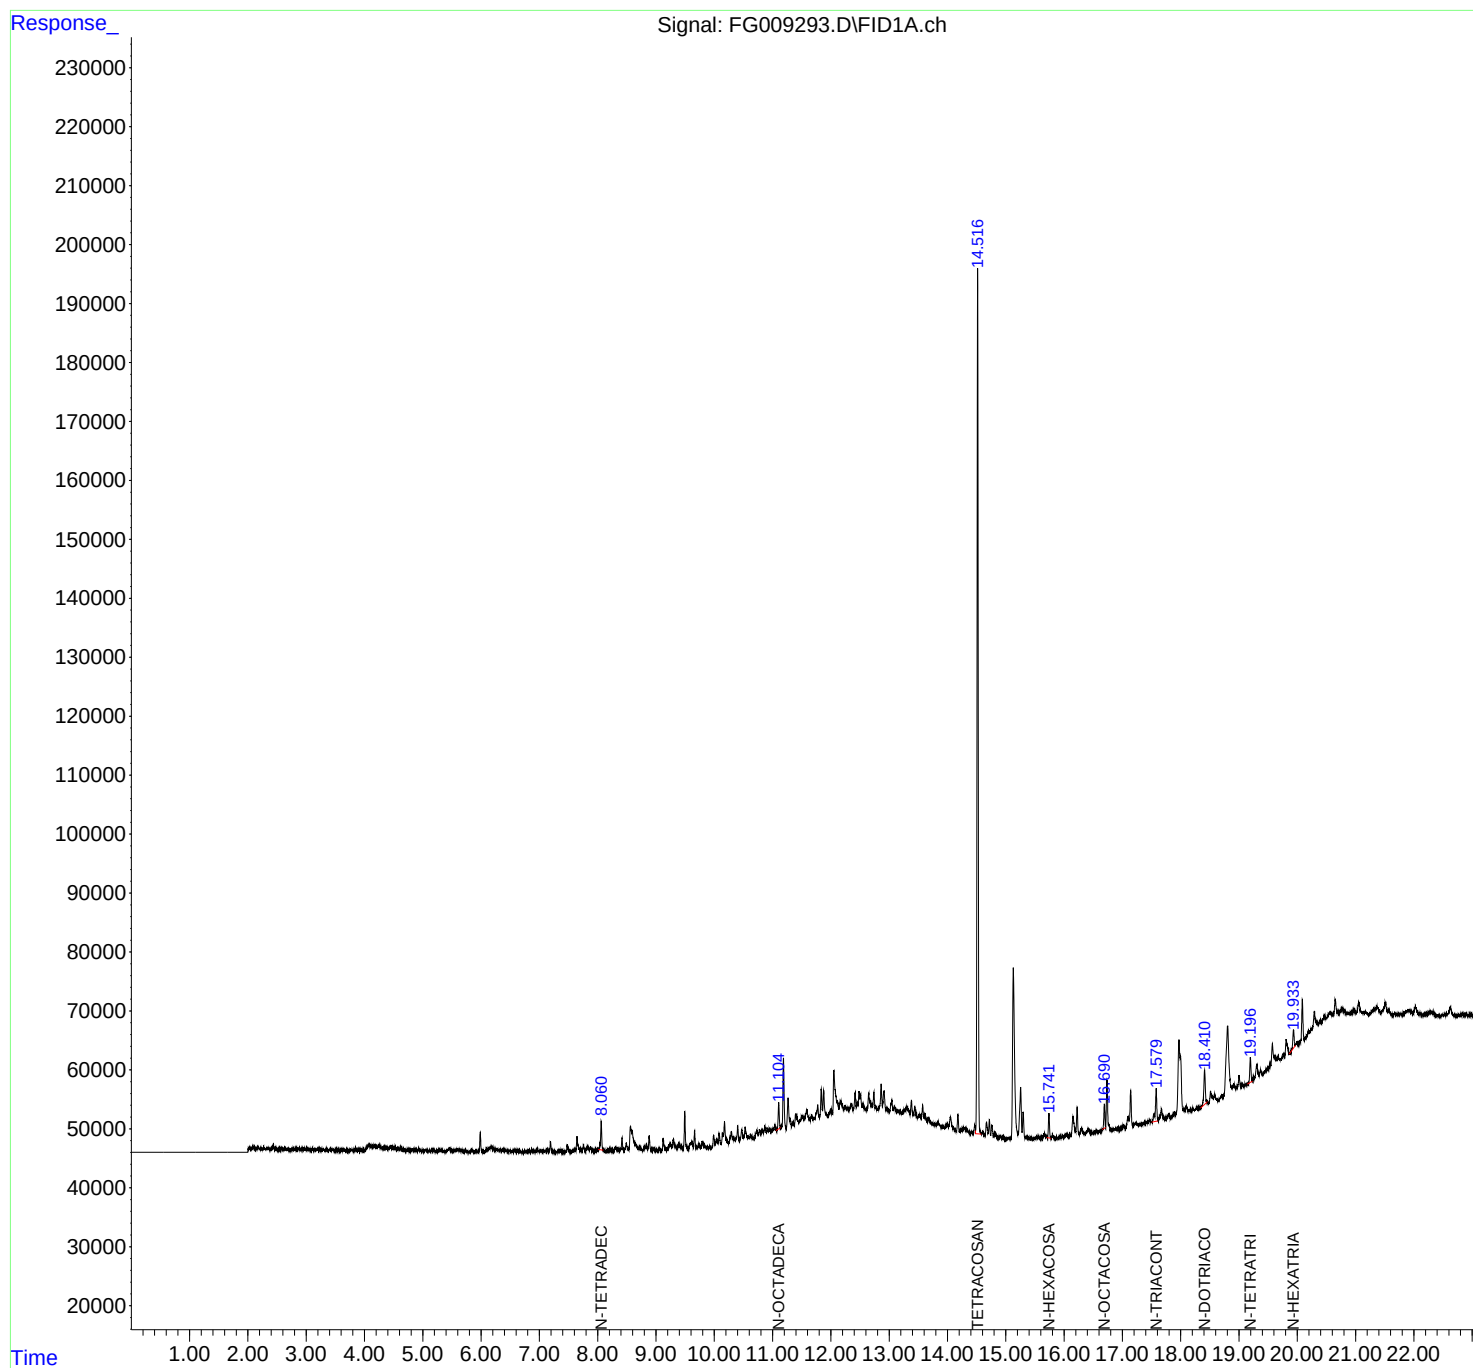


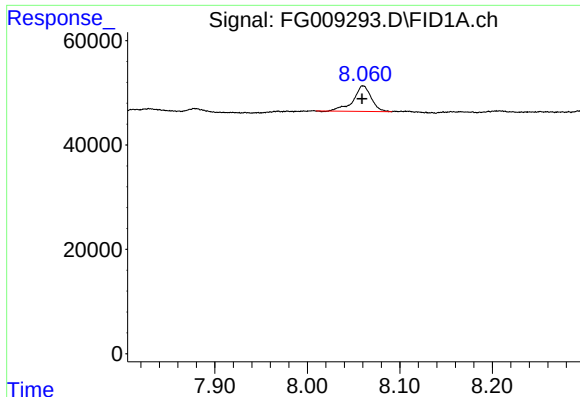

#4 N-TETRADECANE


R.T.: 8.060 min
Delta R.T.: 0.000 min
Response: 66437
Conc: 0.41 ug/ml

Instrument :
FID_G
ClientSampleId :

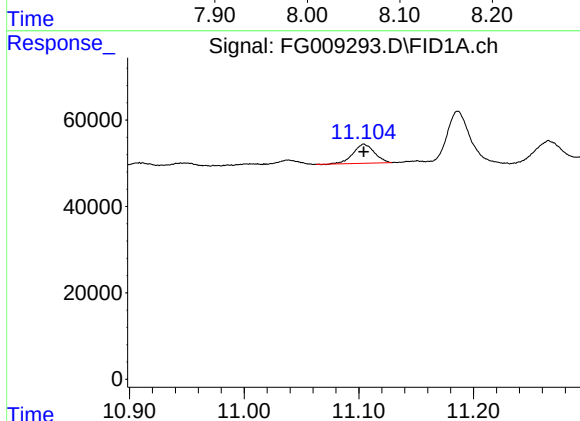


#6 N-OCTADECANE

R.T.: 11.104 min
Delta R.T.: 0.000 min
Response: 56558
Conc: 0.35 ug/ml

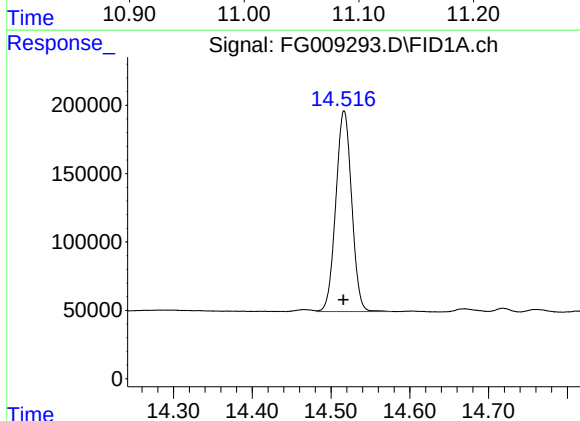


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.517 min
Delta R.T.: 0.001 min
Response: 2052325
Conc: 14.86 ug/ml

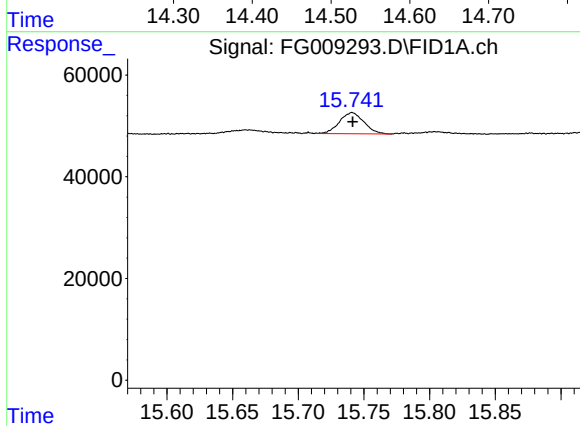

#11 N-HEXACOSANE


R.T.: 15.741 min
Delta R.T.: 0.000 min
Response: 53852
Conc: 0.35 ug/ml

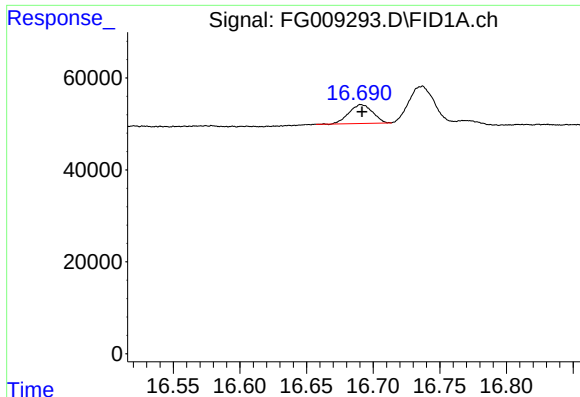

#12 N-OCTACOSANE


R.T.: 16.691 min
Delta R.T.: 0.000 min
Response: 50596
Conc: 0.34 ug/ml

Instrument :
FID_G
ClientSampleId :

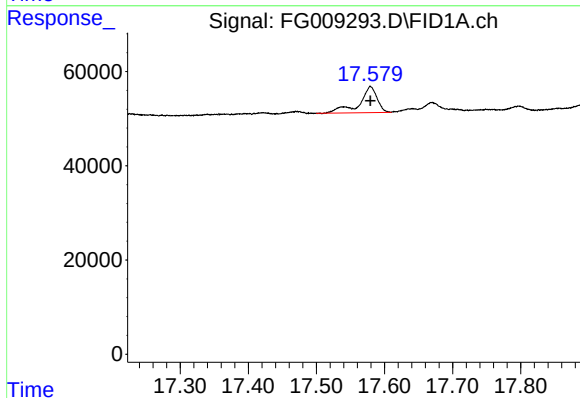


#13 N-TRIACONTANE

R.T.: 17.579 min
Delta R.T.: 0.000 min
Response: 99812
Conc: 0.70 ug/ml

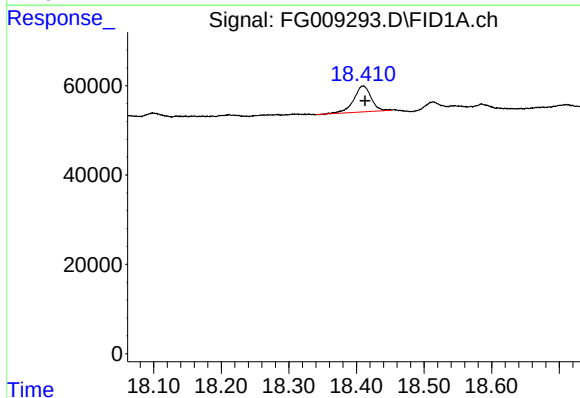


#14 N-DOTRIACONTANE

R.T.: 18.411 min
Delta R.T.: -0.002 min
Response: 103728
Conc: 0.77 ug/ml

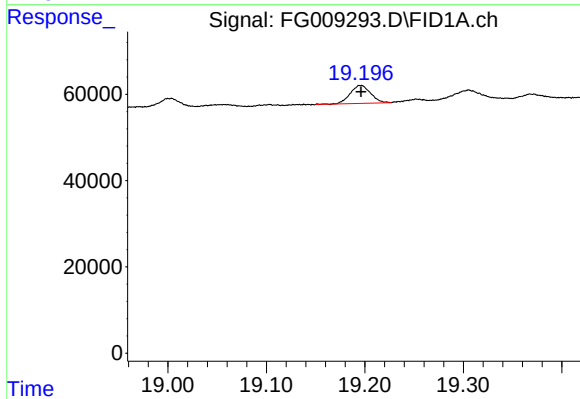

#15 N-TETRATRIACONTANE

R.T.: 19.197 min
Delta R.T.: 0.000 min
Response: 59628
Conc: 0.48 ug/ml

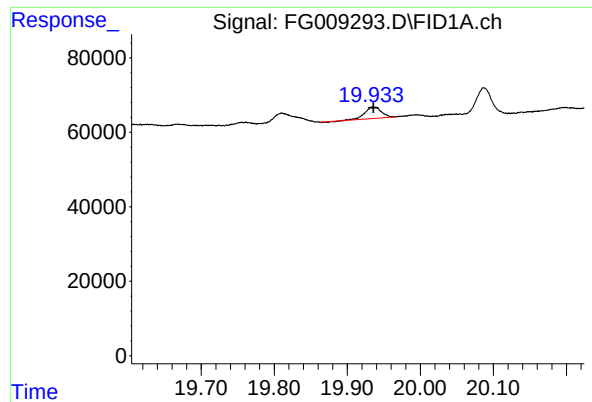

#16 N-HEXATRIACONTANE

R.T.: 19.938 min
Delta R.T.: 0.002 min
Response: 47333
Conc: 0.41 ug/ml

Instrument :

FID_G

ClientSampleId :