

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121521\
Data File : FG009292.D
Signal(s) : FID1A.ch
Acq On : 15 Dec 2021 22:58
Operator : AJ\MA
Sample : M5064-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SASP2-121-1-(0-5)

Integration File: autoint1.e
Quant Time: Dec 16 05:07:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121521.M
Quant Title :
QLast Update : Thu Dec 16 05:01:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.516	2088630	15.122 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121521\
Data File : FG009292.D
Signal(s) : FID1A.ch
Acq On : 15 Dec 2021 22:58
Operator : AJ\MA
Sample : M5064-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SASP2-121-1-(0-5)

Integration File: autoint1.e
Quant Time: Dec 16 05:07:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121521.M
Quant Title :
QLast Update : Thu Dec 16 05:01:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

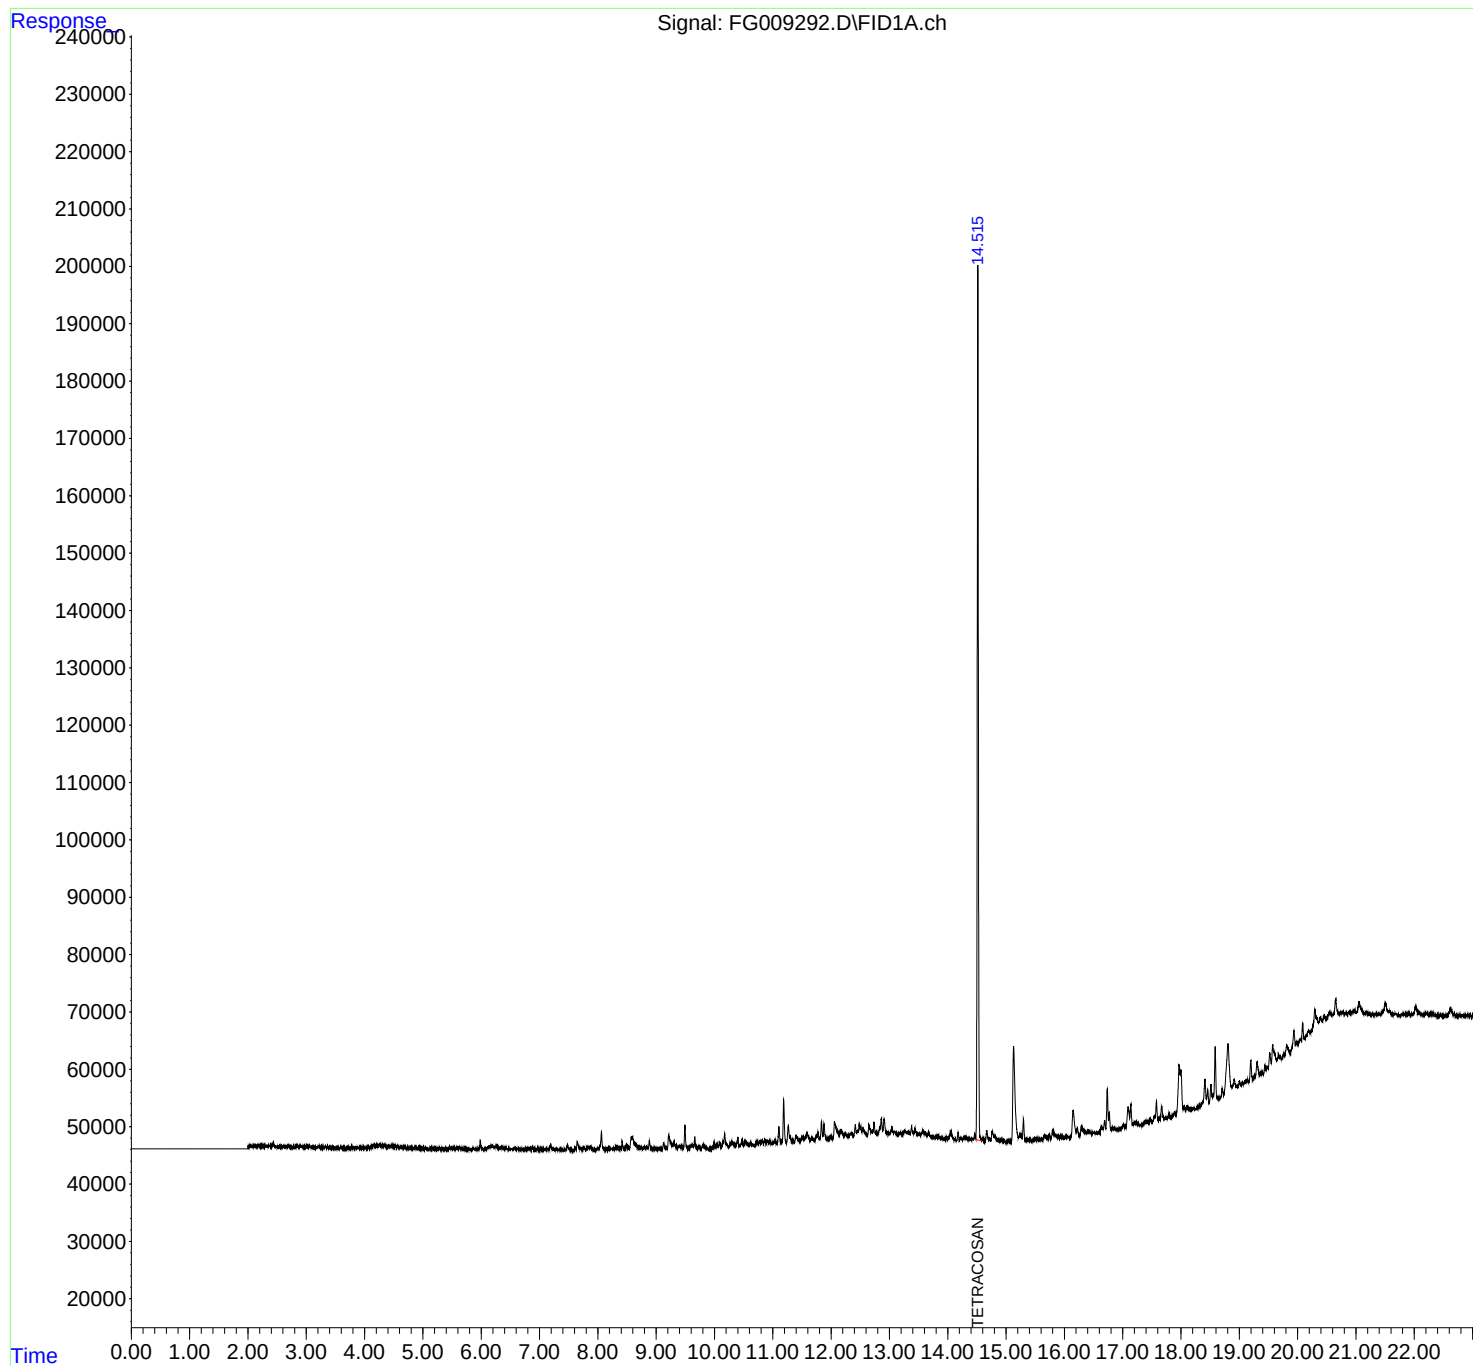

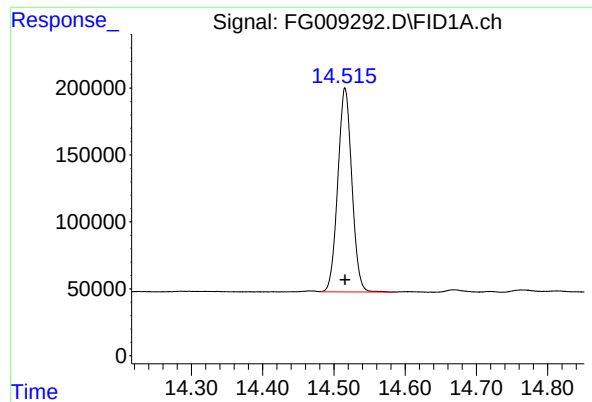

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.516 min
Delta R.T.: 0.000 min
Response: 2088630
Conc: 15.12 ug/ml

Instrument :
FID_G
ClientSampleId :
SASP2-121-1-(0-5)