

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG121523\  
 Data File : FG013298.D  
 Signal(s) : FID1A.ch  
 Acq On : 15 Dec 2023 19:58  
 Operator : YP\AJ  
 Sample : 05862-07 20X  
 Misc :  
 ALS Vial : 21 Sample Multiplier: 1

Instrument :  
 FID\_G  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Dec 15 22:37:58 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG120423.M  
 Quant Title :  
 QLast Update : Mon Dec 04 11:42:34 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.    | Response | Conc Units  |
|-------------------------------|---------|----------|-------------|
| -----                         |         |          |             |
| System Monitoring Compounds   |         |          |             |
| 9) S TETRACOSANE-d50 (SURR... | 15.078  | 88051    | 0.820 ug/ml |
| Target Compounds              |         |          |             |
| 7) N-EICOSANE                 | 13.044f | 78470    | 0.664 ug/ml |
| 10) N-TETRACOSANE             | 15.270  | 169933   | 1.459 ug/ml |
| 17) N-OCTATRIACONTANE         | 21.323  | 81716    | 1.182 ug/ml |
| -----                         |         |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG121523\  
Data File : FG013298.D  
Signal(s) : FID1A.ch  
Acq On : 15 Dec 2023 19:58  
Operator : YP\AJ  
Sample : 05862-07 20X  
Misc :  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Dec 15 22:37:58 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG120423.M  
Quant Title :  
QLast Update : Mon Dec 04 11:42:34 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

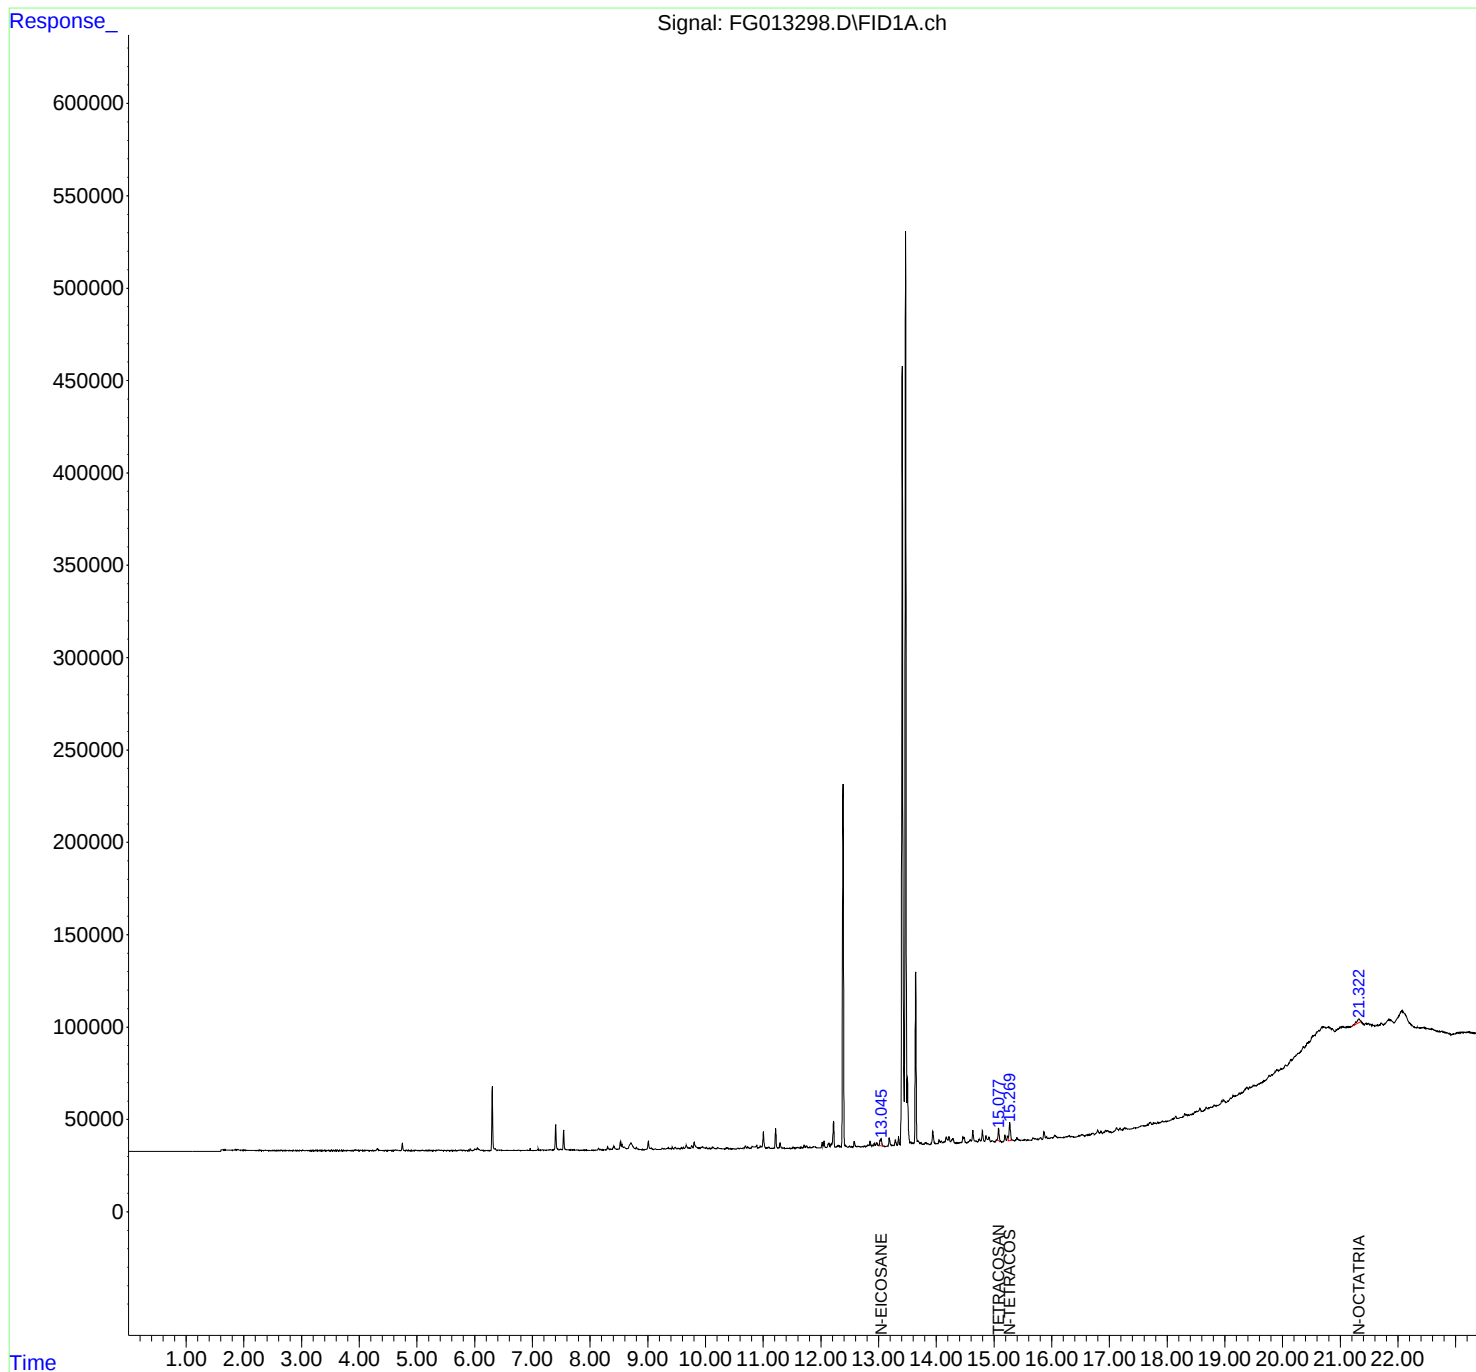


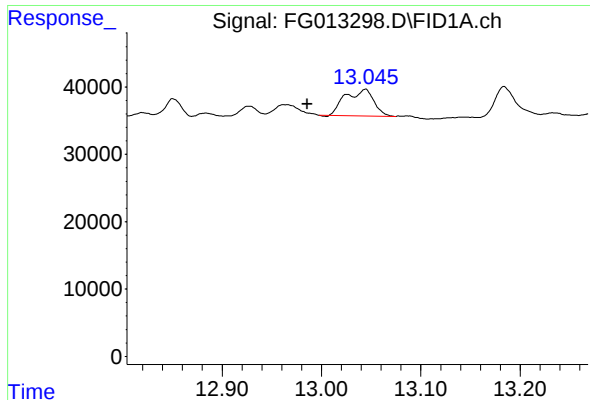

#7 N-EICOSANE


R.T.: 13.044 min  
Delta R.T.: 0.059 min  
Response: 78470  
Conc: 0.66 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

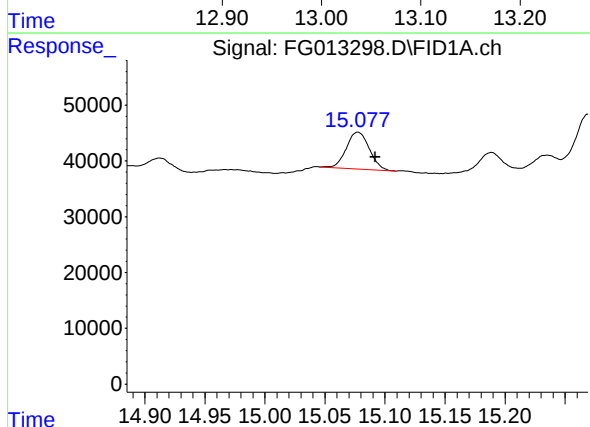


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.078 min  
Delta R.T.: -0.015 min  
Response: 88051  
Conc: 0.82 ug/ml

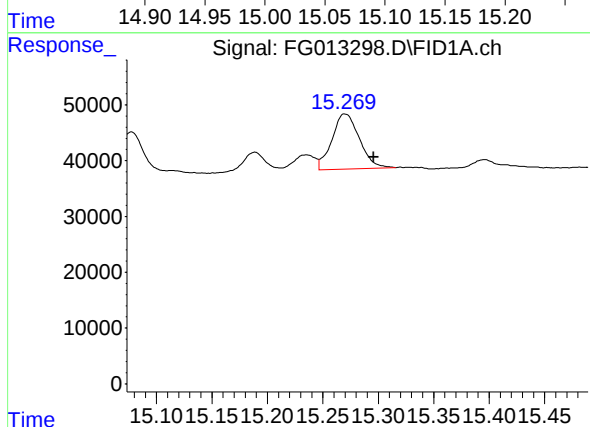

#10 N-TETRACOSANE

R.T.: 15.270 min  
Delta R.T.: -0.026 min  
Response: 169933  
Conc: 1.46 ug/ml

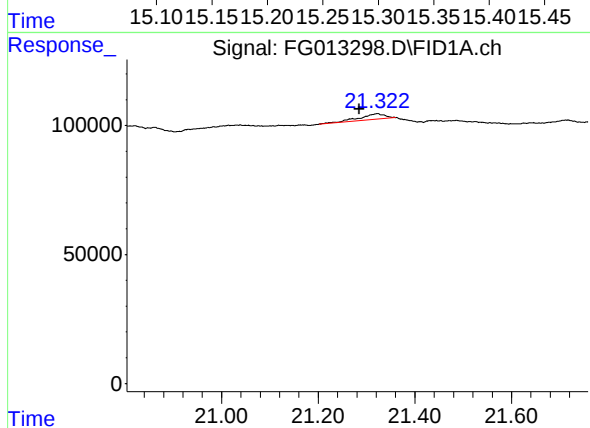

#17 N-OCTATRIACONTANE

R.T.: 21.323 min  
Delta R.T.: 0.037 min  
Response: 81716  
Conc: 1.18 ug/ml