

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG121525\  
Data File : FG017174.D  
Signal(s) : FID1A.ch  
Acq On : 15 Dec 2025 18:07  
Operator : YP\AJ  
Sample : Q3846-01 50X  
Misc :  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :  
BU-02-12112025

Manual Integrations  
APPROVED

Reviewed By :Rahul Chavli 12/16/2025  
Supervised By :Yogesh Patel 12/16/2025

Integration File: autoint1.e  
Quant Time: Dec 16 01:13:06 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG120125.M  
Quant Title :  
QLast Update : Mon Dec 01 15:19:01 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 15.141 | 33433    | 0.321 ug/mlm |
| Target Compounds              |        |          |              |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG121525\  
Data File : FG017174.D  
Signal(s) : FID1A.ch  
Acq On : 15 Dec 2025 18:07  
Operator : YP\AJ  
Sample : Q3846-01 50X  
Misc :  
ALS Vial : 27 Sample Multiplier: 1


Instrument :  
FID\_G  
ClientSampleId :  
BU-02-12112025


Manual Integrations  
APPROVED

Reviewed By :Rahul Chavli 12/16/2025  
Supervised By :Yogesh Patel 12/16/2025

Integration File: autoint1.e  
Quant Time: Dec 16 01:13:06 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG120125.M  
Quant Title :  
QLast Update : Mon Dec 01 15:19:01 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

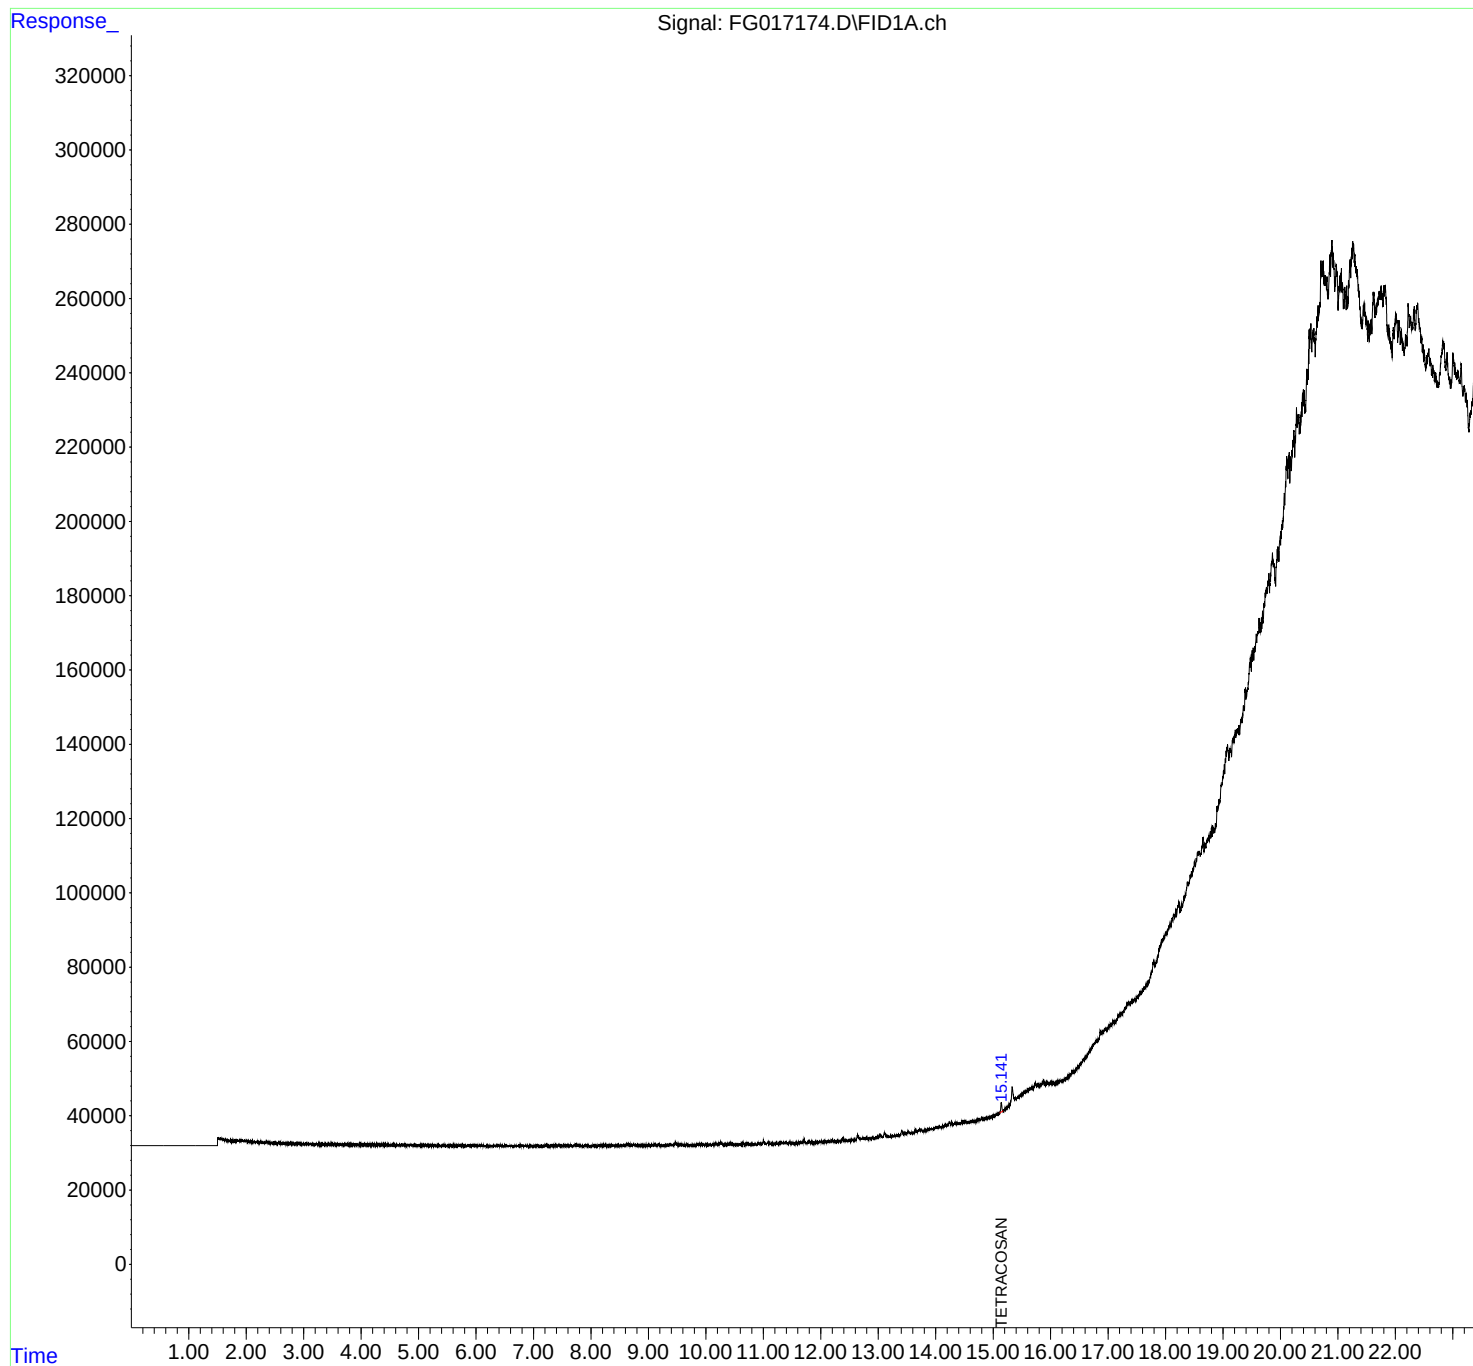

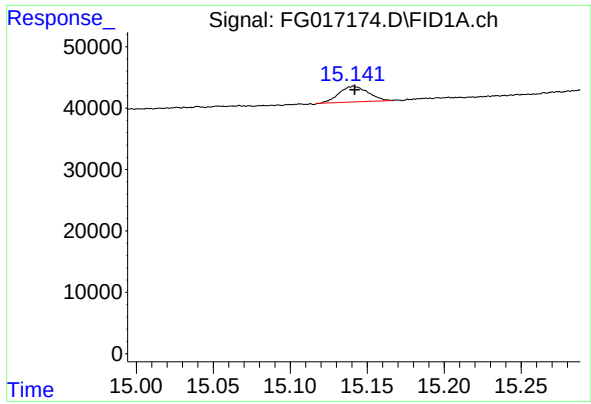

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.141 min  
Delta R.T.: -0.001 min  
Response: 33433  
Conc: 0.32 ug/ml

Instrument :  
FID\_G  
ClientSampleId :  
BU-02-12112025

Manual Integrations  
APPROVED

Reviewed By :Rahul Chavli 12/16/2025  
Supervised By :Yogesh Patel 12/16/2025