

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE121525AL\  
Data File : FE057331.D  
Signal(s) : FID1B.ch  
Acq On : 15 Dec 2025 09:48  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Dec 16 03:35:23 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 112725.M  
Quant Title : GC Extractables  
QLast Update : Mon Dec 01 08:04:59 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

| Compound | R.T. | Response | Conc Units |
|----------|------|----------|------------|
|----------|------|----------|------------|

-----  
System Monitoring Compounds

Target Compounds

|       |                          |        |        |             |
|-------|--------------------------|--------|--------|-------------|
| 17) T | n-Tricontane (C30)       | 18.087 | 95911  | 0.427 ug/ml |
| 18) T | n-Dotriacontane (C32)    | 18.921 | 159837 | 0.685 ug/ml |
| 19) T | n-Tetratriacontane (C34) | 19.706 | 170680 | 0.799 ug/ml |
| 20) T | n-Hexatriacontane (C36)  | 20.448 | 84533  | 0.454 ug/ml |

-----  
(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE121525AL\  
Data File : FE057331.D  
Signal(s) : FID1B.ch  
Acq On : 15 Dec 2025 09:48  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Dec 16 03:35:23 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 112725.M  
Quant Title : GC Extractables  
QLast Update : Mon Dec 01 08:04:59 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

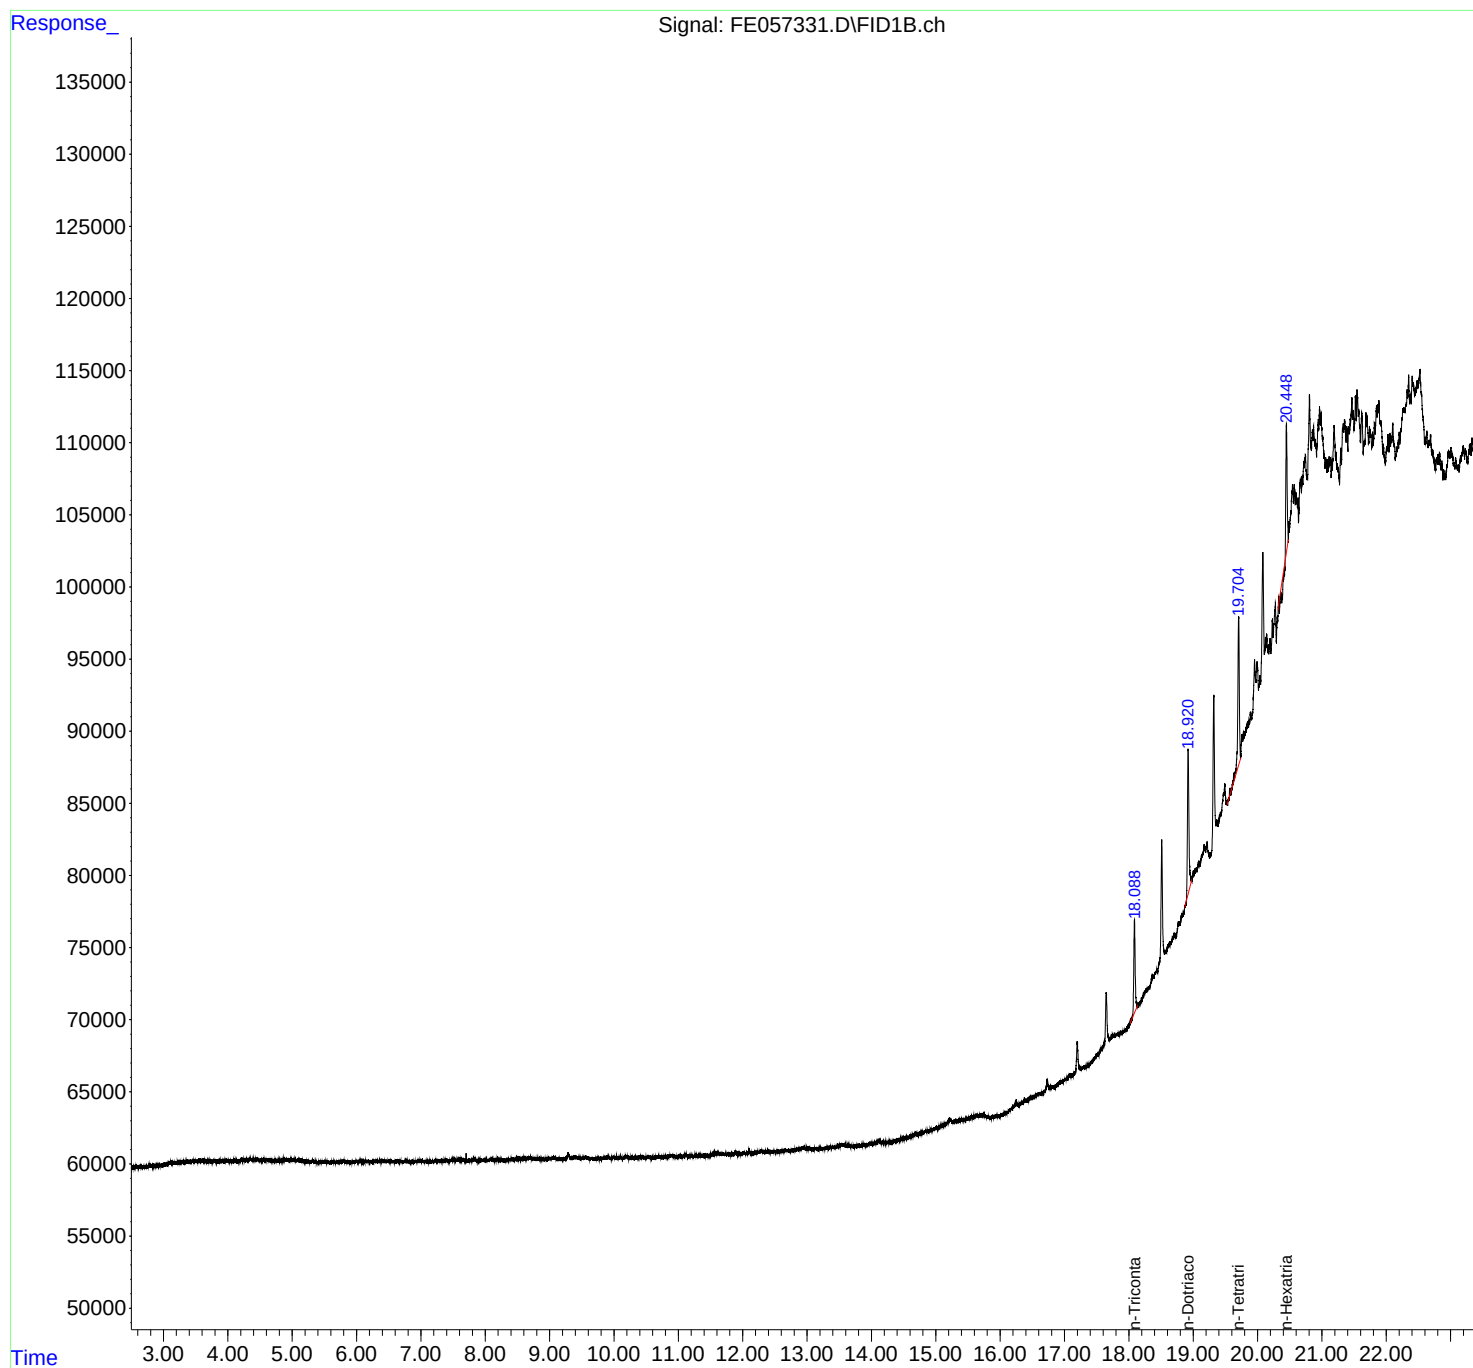


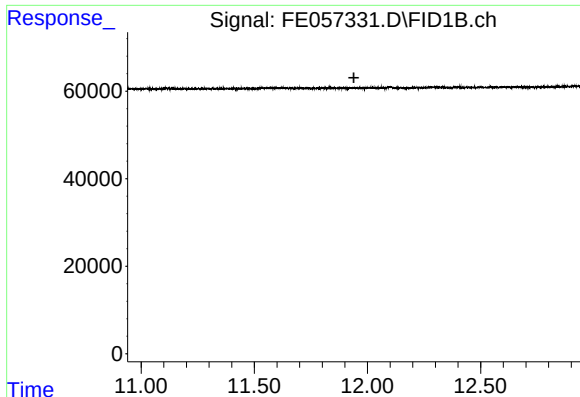

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min  
Exp R.T. : 11.940 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_G  
ClientSampleId :

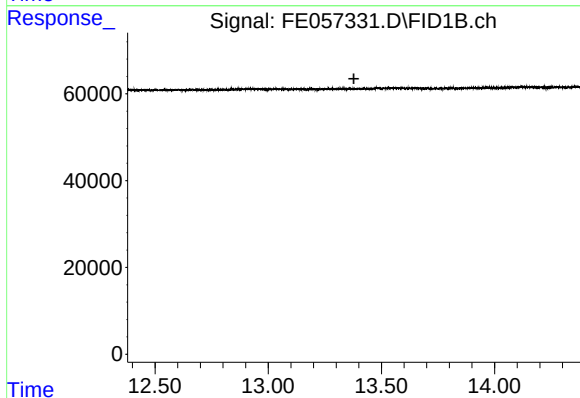


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min  
Exp R.T. : 13.378 min  
Response: 0  
Conc: N.D.

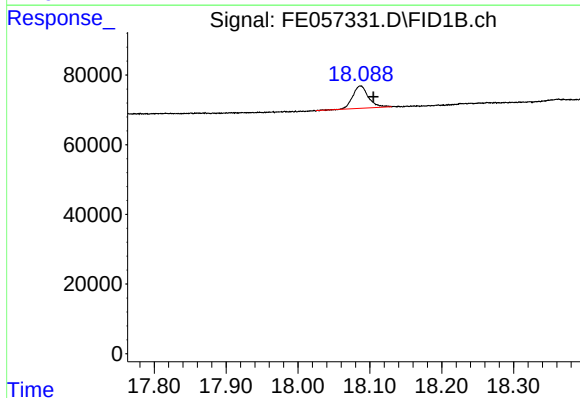


#17 n-Tricontane (C30)

R.T.: 18.087 min  
Delta R.T.: -0.018 min  
Response: 95911  
Conc: 0.43 ug/ml

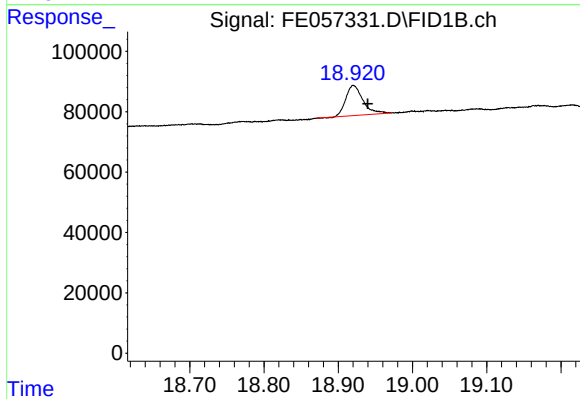

#18 n-Dotriacontane (C32)


R.T.: 18.921 min  
Delta R.T.: -0.019 min  
Response: 159837  
Conc: 0.68 ug/ml

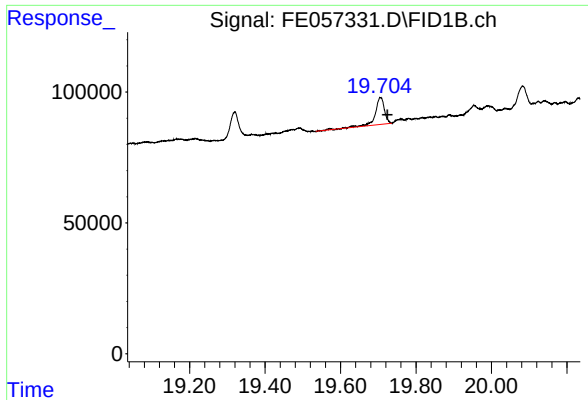

#19 n-Tetratriacontane (C34)

R.T.: 19.706 min  
Delta R.T.: -0.019 min  
Response: 170680  
Conc: 0.80 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

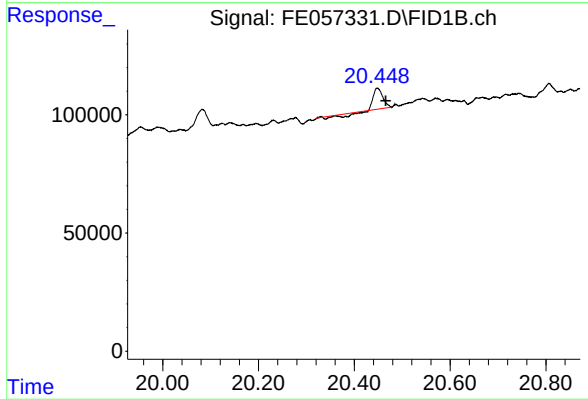

#20 n-Hexatriacontane (C36)

R.T.: 20.448 min  
Delta R.T.: -0.017 min  
Response: 84533  
Conc: 0.45 ug/ml