

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121622\
Data File : FG011209.D
Signal(s) : FID1A.ch
Acq On : 16 Dec 2022 12:02
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 16 17:56:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG120522.M
Quant Title :
QLast Update : Tue Dec 06 04:53:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.762	3615514	26.530 ug/ml
12)	N-OCTACOSANE	17.248	3374851	27.365 ug/ml
13)	N-TRIACONTANE	18.134	381910	3.219 ug/ml
14)	N-DOTRIACONTANE	18.968	491884	4.288 ug/ml
15)	N-TETRATRIACONTANE	19.753	391953	3.524 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121622\
Data File : FG011209.D
Signal(s) : FID1A.ch
Acq On : 16 Dec 2022 12:02
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 16 17:56:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG120522.M
Quant Title :
QLast Update : Tue Dec 06 04:53:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

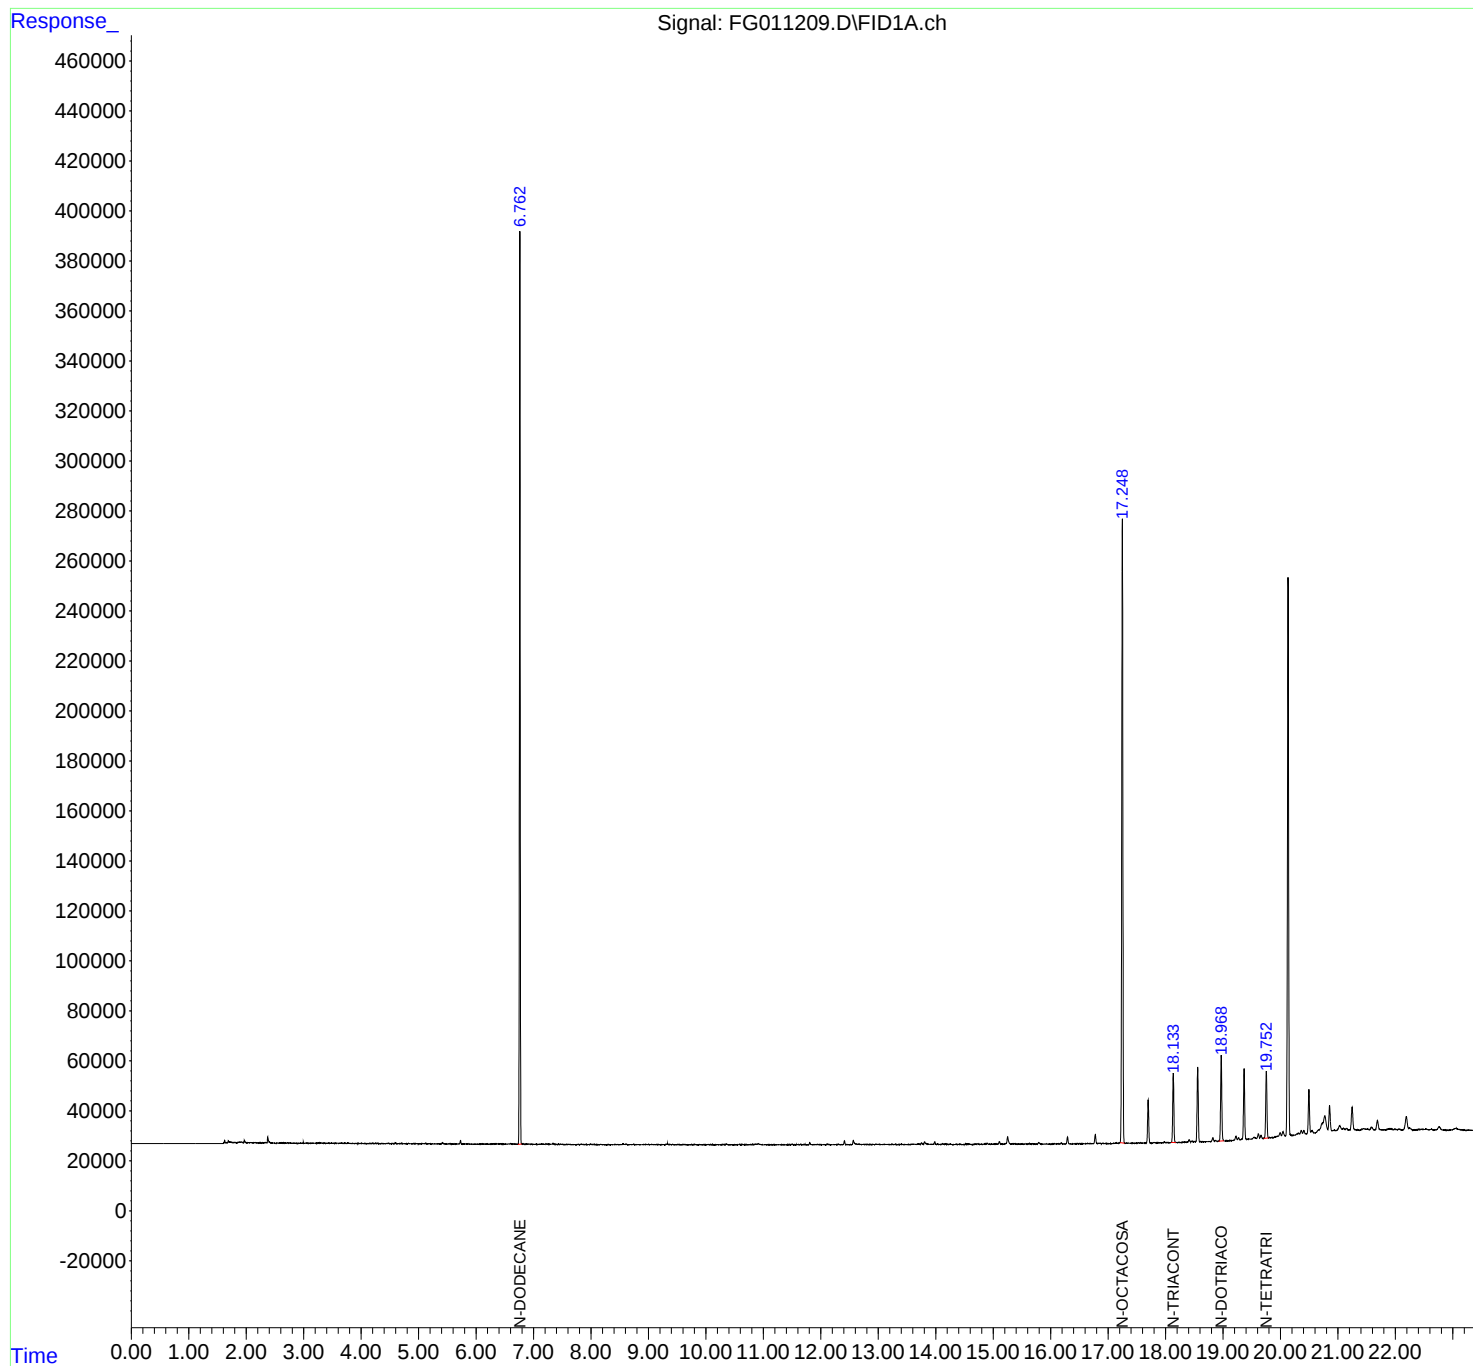


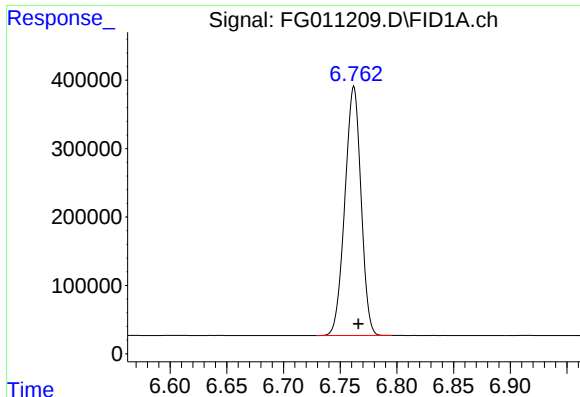

#3 N-DODECANE


R.T.: 6.762 min
Delta R.T.: -0.004 min
Response: 3615514
Conc: 26.53 ug/ml

Instrument :
FID_G
ClientSampleId :

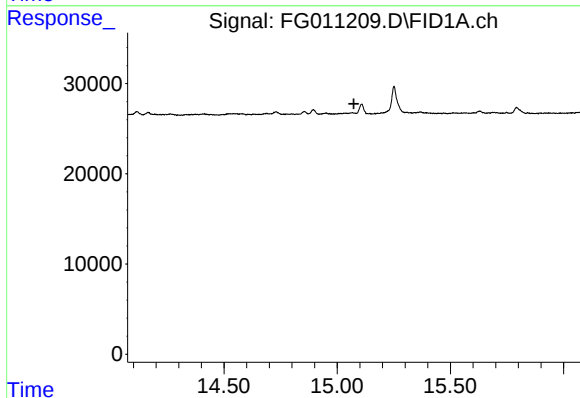


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.074 min
Response: 0
Conc: N.D.

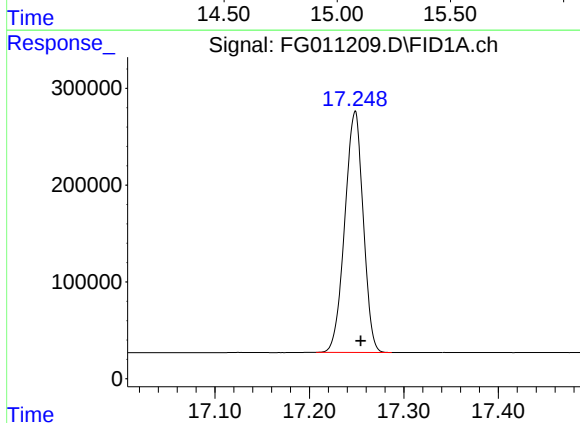


#12 N-OCTACOSANE

R.T.: 17.248 min
Delta R.T.: -0.006 min
Response: 3374851
Conc: 27.36 ug/ml

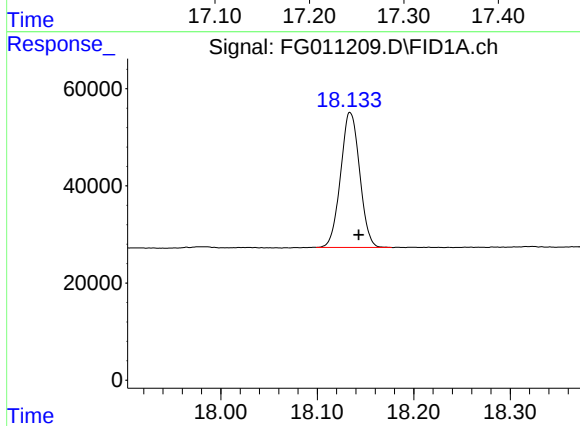

#13 N-TRIACONTANE


R.T.: 18.134 min
Delta R.T.: -0.009 min
Response: 381910
Conc: 3.22 ug/ml

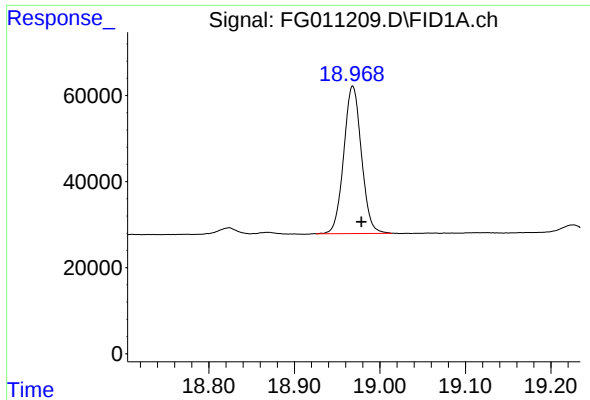

#14 N-DOTRIACONTANE

R.T.: 18.968 min
Delta R.T.: -0.010 min
Response: 491884
Conc: 4.29 ug/ml

Instrument :
FID_G
ClientSampleId :

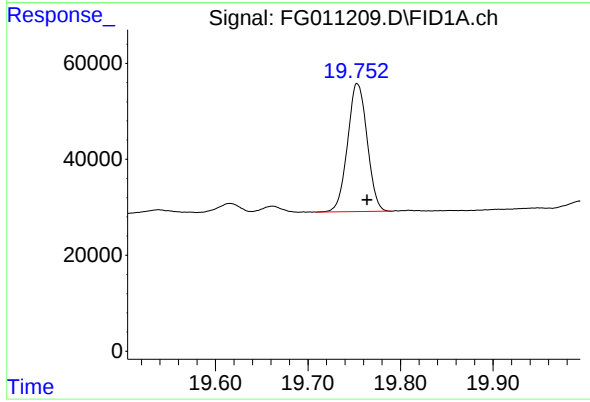

#15 N-TETRATRIACONTANE

R.T.: 19.753 min
Delta R.T.: -0.011 min
Response: 391953
Conc: 3.52 ug/ml