

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG122022\
Data File : FG011232.D
Signal(s) : FID1A.ch
Acq On : 20 Dec 2022 12:19
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Dec 20 17:27:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG120522.M
Quant Title :
QLast Update : Tue Dec 06 04:53:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.762	2783290	20.424 ug/ml
12) N-OCTACOSANE	17.246	2550247	20.678 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG122022\
Data File : FG011232.D
Signal(s) : FID1A.ch
Acq On : 20 Dec 2022 12:19
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Dec 20 17:27:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG120522.M
Quant Title :
QLast Update : Tue Dec 06 04:53:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

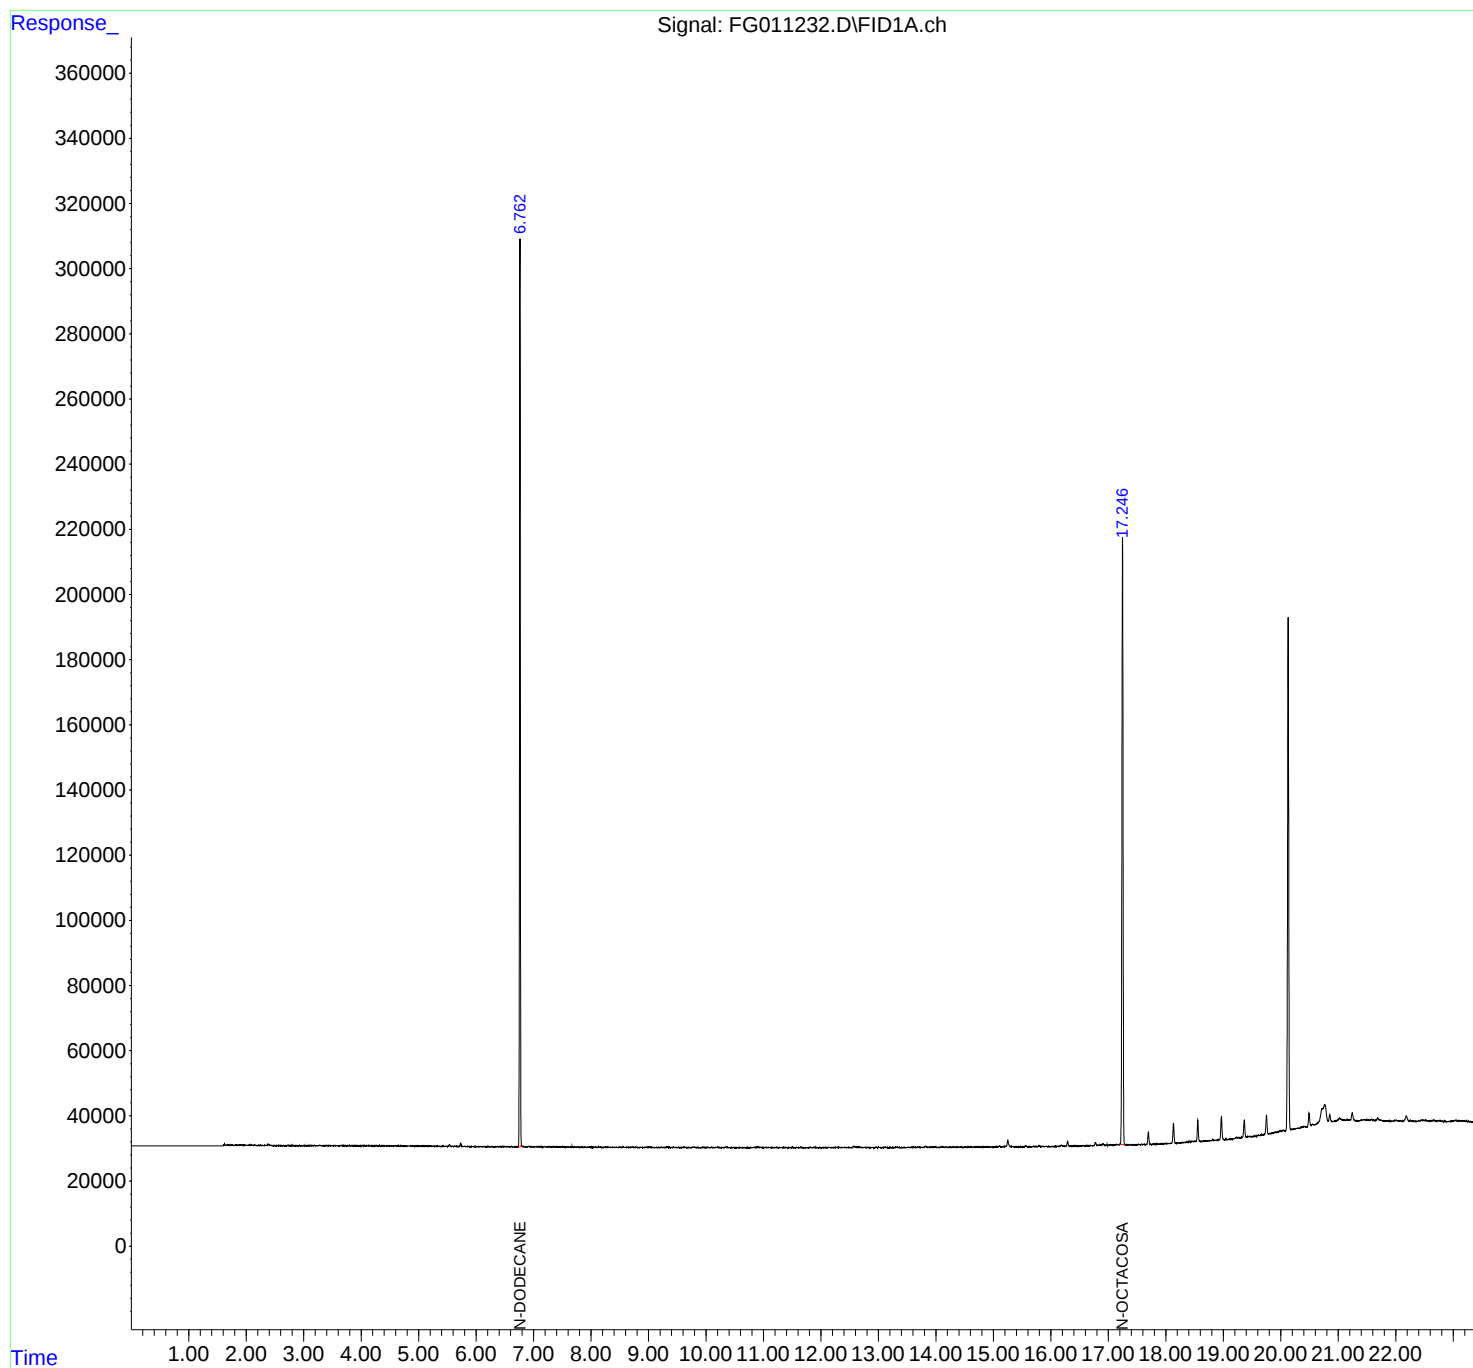


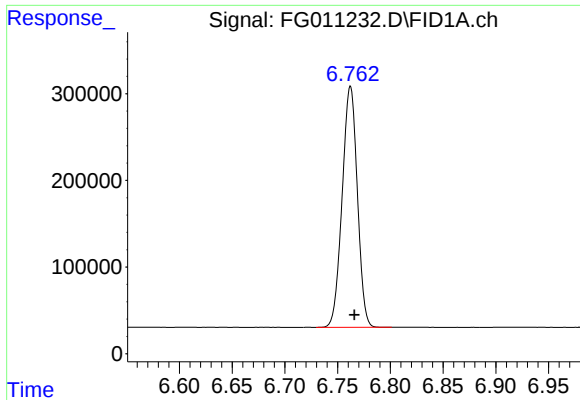

#3 N-DODECANE


R.T.: 6.762 min
Delta R.T.: -0.004 min
Response: 2783290
Conc: 20.42 ug/ml

Instrument :
FID_G
ClientSampleId :
RT MARKER

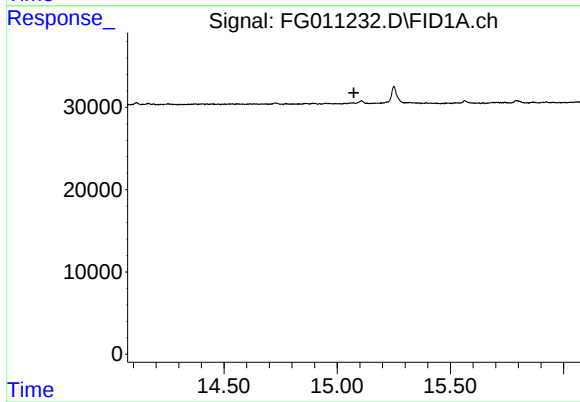

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 15.074 min
Response: 0
Conc: N.D.

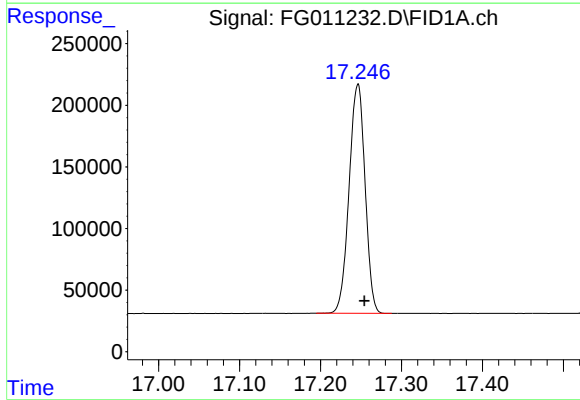

#12 N-OCTACOSANE

R.T.: 17.246 min
Delta R.T.: -0.008 min
Response: 2550247
Conc: 20.68 ug/ml