

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG122022\
Data File : FG011236.D
Signal(s) : FID1A.ch
Acq On : 20 Dec 2022 15:51
Operator : YP\AJ
Sample : N6067-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
WC-LIQUID-20221214

Integration File: autoint1.e
Quant Time: Dec 20 17:28:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG120522.M
Quant Title :
QLast Update : Tue Dec 06 04:53:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.066	1530213	13.136 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG122022\
Data File : FG011236.D
Signal(s) : FID1A.ch
Acq On : 20 Dec 2022 15:51
Operator : YP\AJ
Sample : N6067-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
WC-LIQUID-20221214

Integration File: autoint1.e
Quant Time: Dec 20 17:28:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG120522.M
Quant Title :
QLast Update : Tue Dec 06 04:53:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

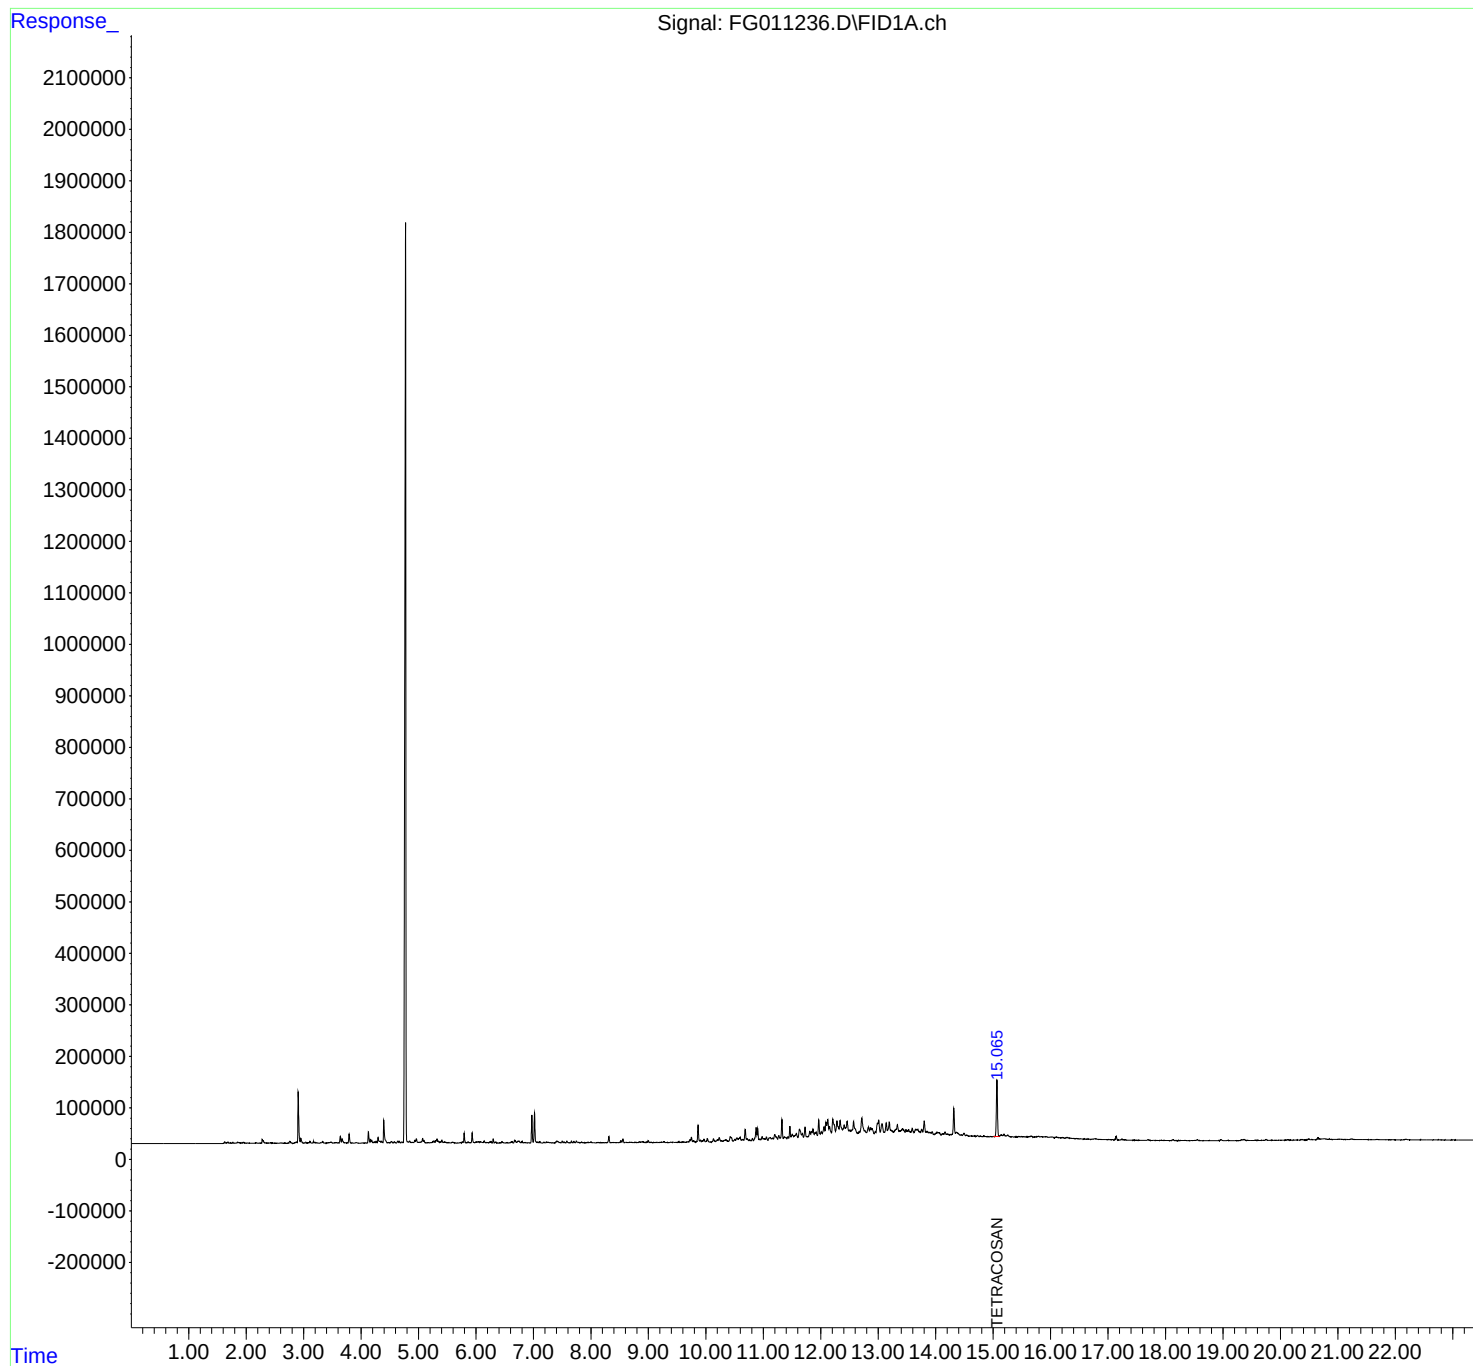

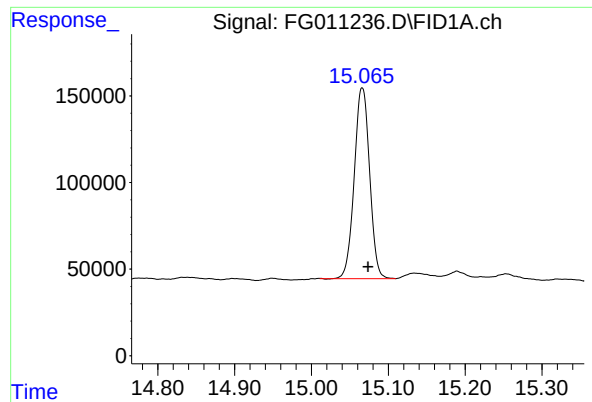

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.066 min
Delta R.T.: -0.008 min
Response: 1530213
Conc: 13.14 ug/ml

Instrument :
FID_G
ClientSampleId :
WC-LIQUID-20221214