

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG122221\
Data File : FG009331.D
Signal(s) : FID1A.ch
Acq On : 22 Dec 2021 15:38
Operator : AJ\MA
Sample : M5187-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SASP2-119-1-0-5

Integration File: autoint1.e
Quant Time: Dec 22 23:54:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121521.M
Quant Title :
QLast Update : Thu Dec 16 05:01:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.516	2096968	15.182 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG122221\
Data File : FG009331.D
Signal(s) : FID1A.ch
Acq On : 22 Dec 2021 15:38
Operator : AJ\MA
Sample : M5187-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
SASP2-119-1-0-5

Integration File: autoint1.e
Quant Time: Dec 22 23:54:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121521.M
Quant Title :
QLast Update : Thu Dec 16 05:01:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

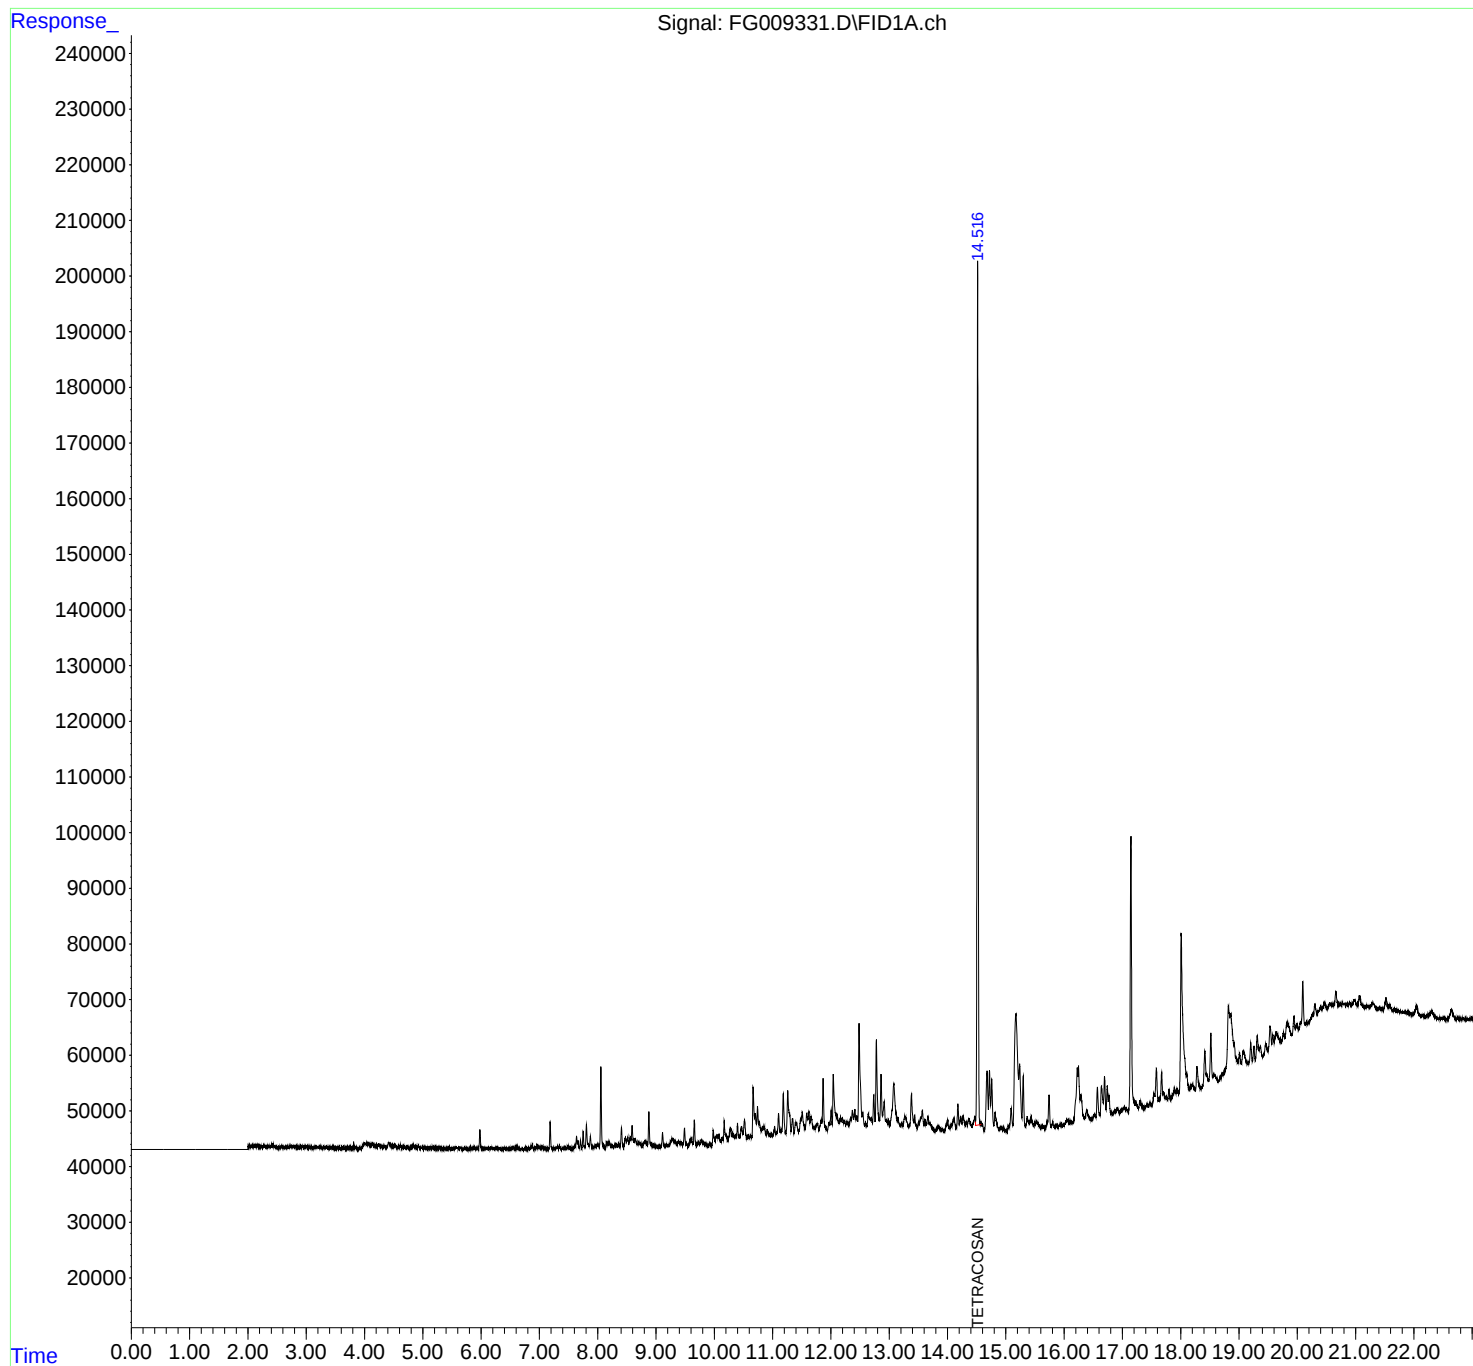

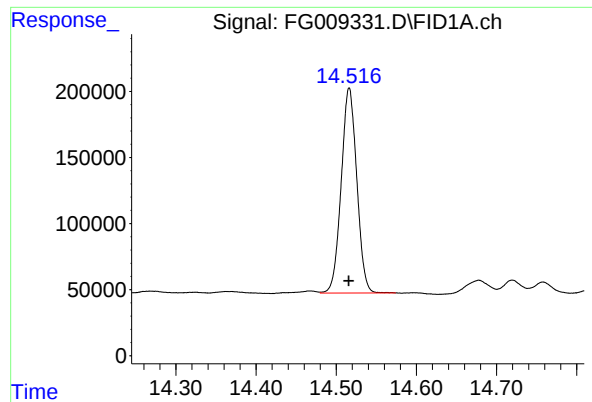

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.516 min
Delta R.T.: 0.000 min
Response: 2096968
Conc: 15.18 ug/ml

Instrument :
FID_G
ClientSampleId :
SASP2-119-1-0-5