

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG122221\
 Data File : FG009338.D
 Signal(s) : FID1A.ch
 Acq On : 22 Dec 2021 19:12
 Operator : AJ\MA
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Dec 22 23:56:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121521.M
 Quant Title :
 QLast Update : Thu Dec 16 05:01:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.520	6587134	47.691 ug/ml
Target Compounds			
2) N-DECANE	4.238	8030059	52.245 ug/ml
3) N-DODECANE	6.259	8129572	51.647 ug/ml
4) N-TETRADECANE	8.057	8170357	50.828 ug/ml
5) N-HEXADECANE	9.661	8071437	50.363 ug/ml
6) N-OCTADECANE	11.106	8103362	49.793 ug/ml
7) N-EICOSANE	12.418	7959764	49.027 ug/ml
8) N-DOCOSANE	13.618	7674101	48.196 ug/ml
10) N-TETRACOSANE	14.724	7498349	47.506 ug/ml
11) N-HEXACOSANE	15.747	7210172	46.766 ug/ml
12) N-OCTACOSANE	16.697	6915281	46.214 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG122221\
Data File : FG009338.D
Signal(s) : FID1A.ch
Acq On : 22 Dec 2021 19:12
Operator : AJ\MA
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Dec 22 23:56:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121521.M
Quant Title :
QLast Update : Thu Dec 16 05:01:34 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

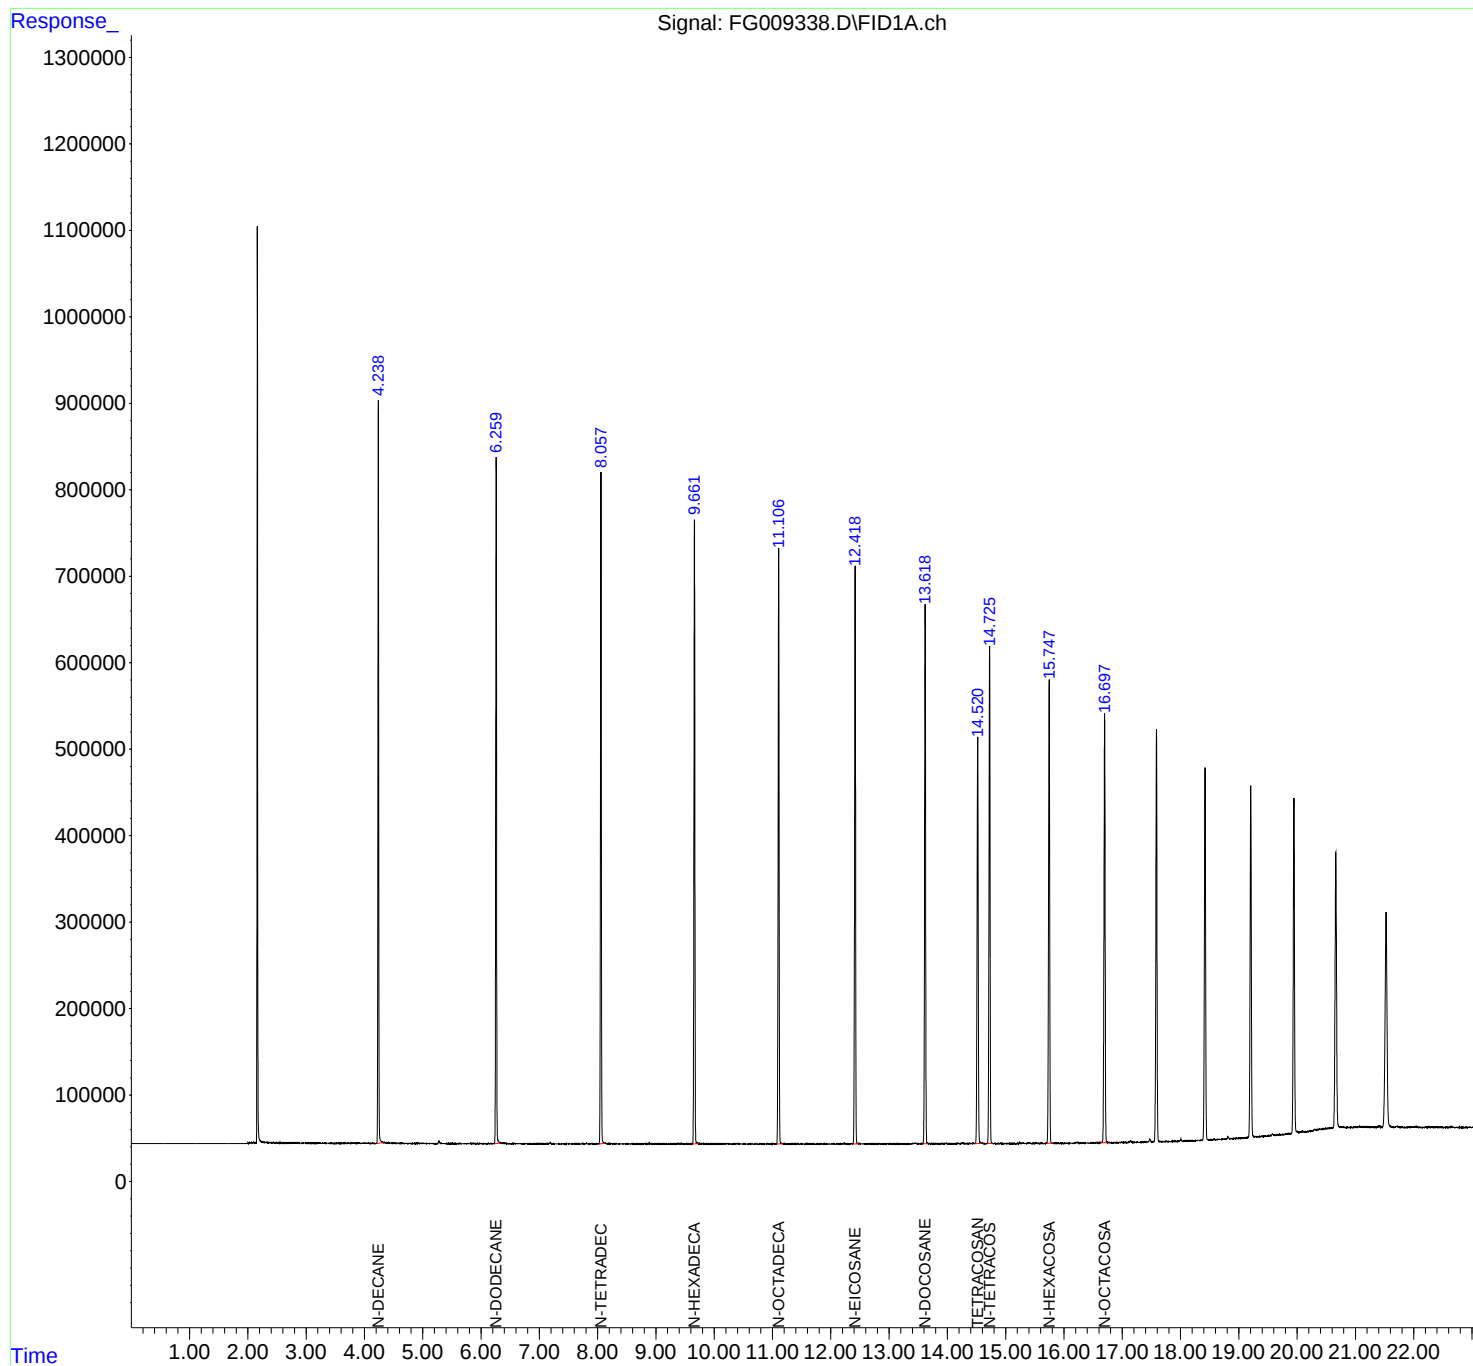


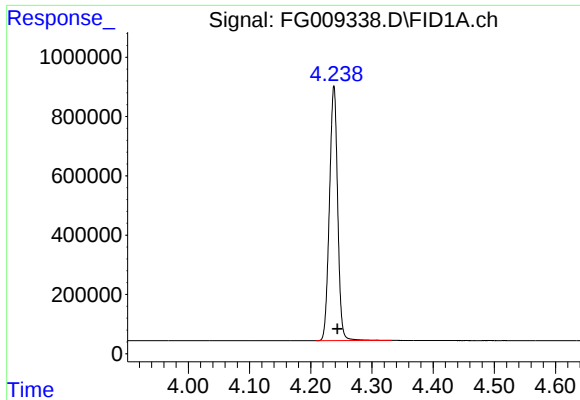

#2 N-DECANE


R.T.: 4.238 min
Delta R.T.: -0.005 min
Response: 8030059
Conc: 52.25 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

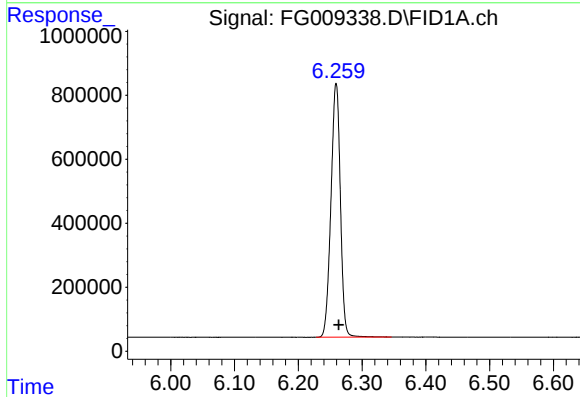


#3 N-DODECANE

R.T.: 6.259 min
Delta R.T.: -0.004 min
Response: 8129572
Conc: 51.65 ug/ml

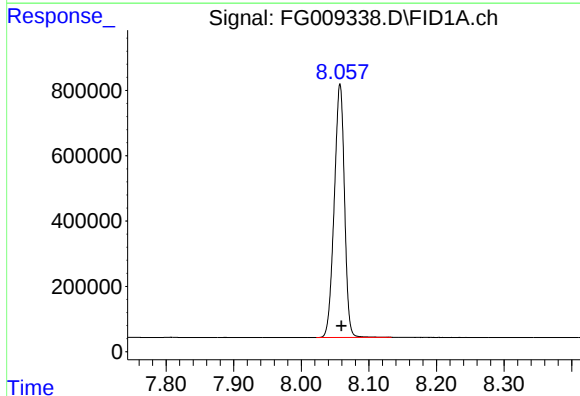


#4 N-TETRADECANE

R.T.: 8.057 min
Delta R.T.: -0.002 min
Response: 8170357
Conc: 50.83 ug/ml

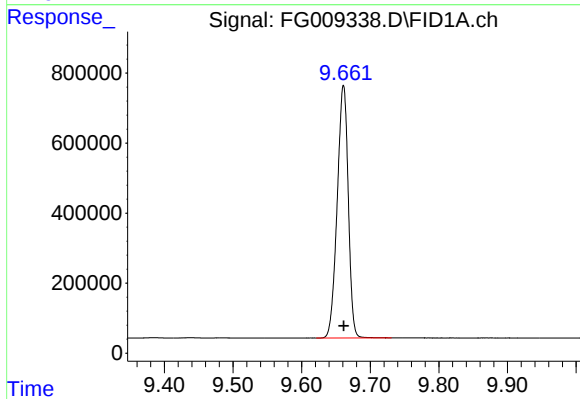

#5 N-HEXADECANE


R.T.: 9.661 min
Delta R.T.: 0.000 min
Response: 8071437
Conc: 50.36 ug/ml

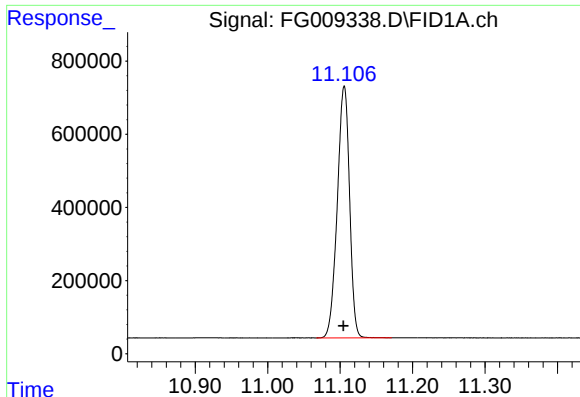

#6 N-OCTADECANE


R.T.: 11.106 min
Delta R.T.: 0.001 min
Response: 8103362
Conc: 49.79 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

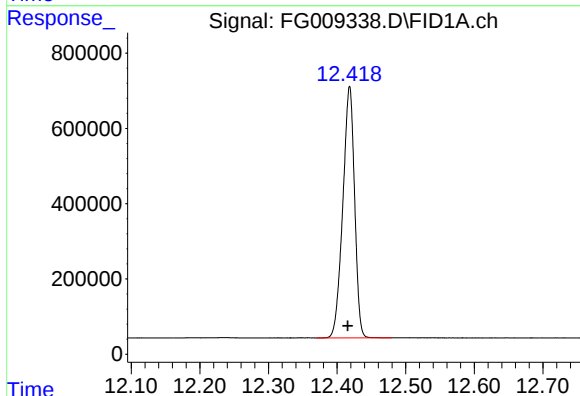


#7 N-EICOSANE

R.T.: 12.418 min
Delta R.T.: 0.003 min
Response: 7959764
Conc: 49.03 ug/ml

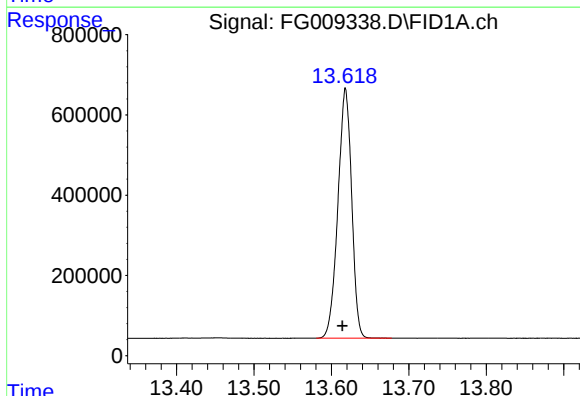


#8 N-DOCOSANE

R.T.: 13.618 min
Delta R.T.: 0.004 min
Response: 7674101
Conc: 48.20 ug/ml

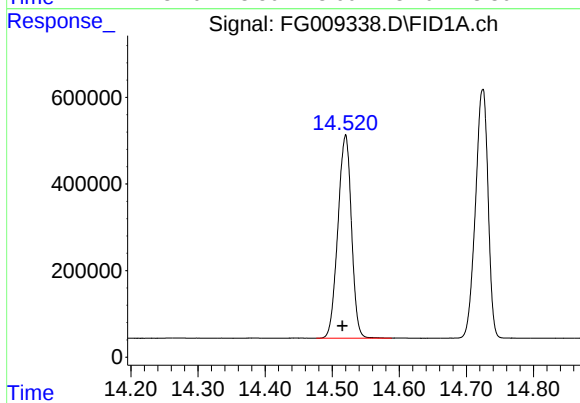

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.520 min
Delta R.T.: 0.005 min
Response: 6587134
Conc: 47.69 ug/ml

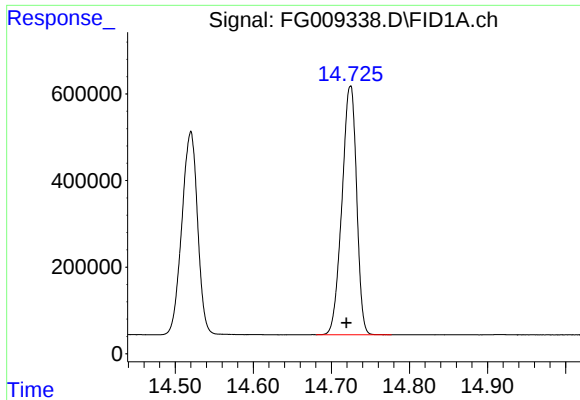

#10 N-TETRACOSANE


R.T.: 14.724 min
Delta R.T.: 0.005 min
Response: 7498349
Conc: 47.51 ug/ml

Instrument :
FID_G
ClientSampleId :
50 PPM TRPH STD

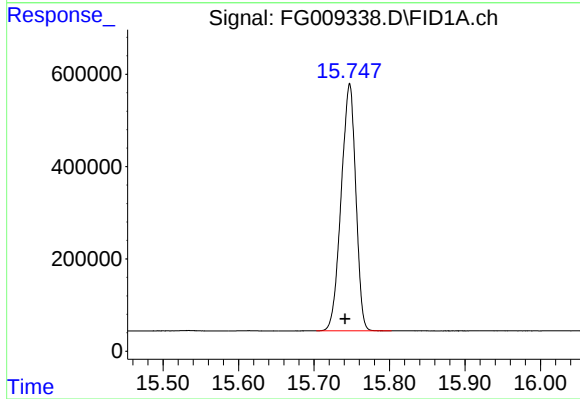

#11 N-HEXACOSANE

R.T.: 15.747 min
Delta R.T.: 0.006 min
Response: 7210172
Conc: 46.77 ug/ml

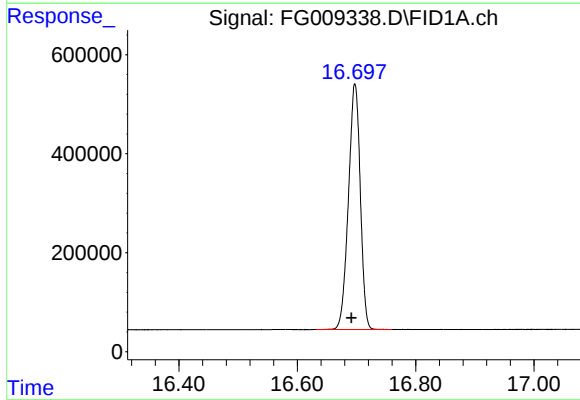

#12 N-OCTACOSANE

R.T.: 16.697 min
Delta R.T.: 0.006 min
Response: 6915281
Conc: 46.21 ug/ml