

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG122324\  
 Data File : FG015018.D  
 Signal(s) : FID1A.ch  
 Acq On : 23 Dec 2024 12:26  
 Operator : YP\AJ  
 Sample : P5361-01  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 FID\_G  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Dec 24 00:27:34 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG121924.M  
 Quant Title :  
 QLast Update : Thu Dec 19 16:42:40 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 15.060 | 1467932  | 10.983 ug/ml |
| Target Compounds              |        |          |              |
| 4) N-TETRADECANE              | 8.546  | 116755   | 0.870 ug/ml  |
| 10) N-TETRACOSANE             | 15.231 | 166531   | 1.125 ug/ml  |
| 14) N-DOTRIACONTANE           | 18.963 | 316476   | 2.193 ug/ml  |
| 16) N-HEXATRIACONTANE         | 20.496 | 191735   | 1.717 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG122324\  
Data File : FG015018.D  
Signal(s) : FID1A.ch  
Acq On : 23 Dec 2024 12:26  
Operator : YP\AJ  
Sample : P5361-01  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Dec 24 00:27:34 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG121924.M  
Quant Title :  
QLast Update : Thu Dec 19 16:42:40 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

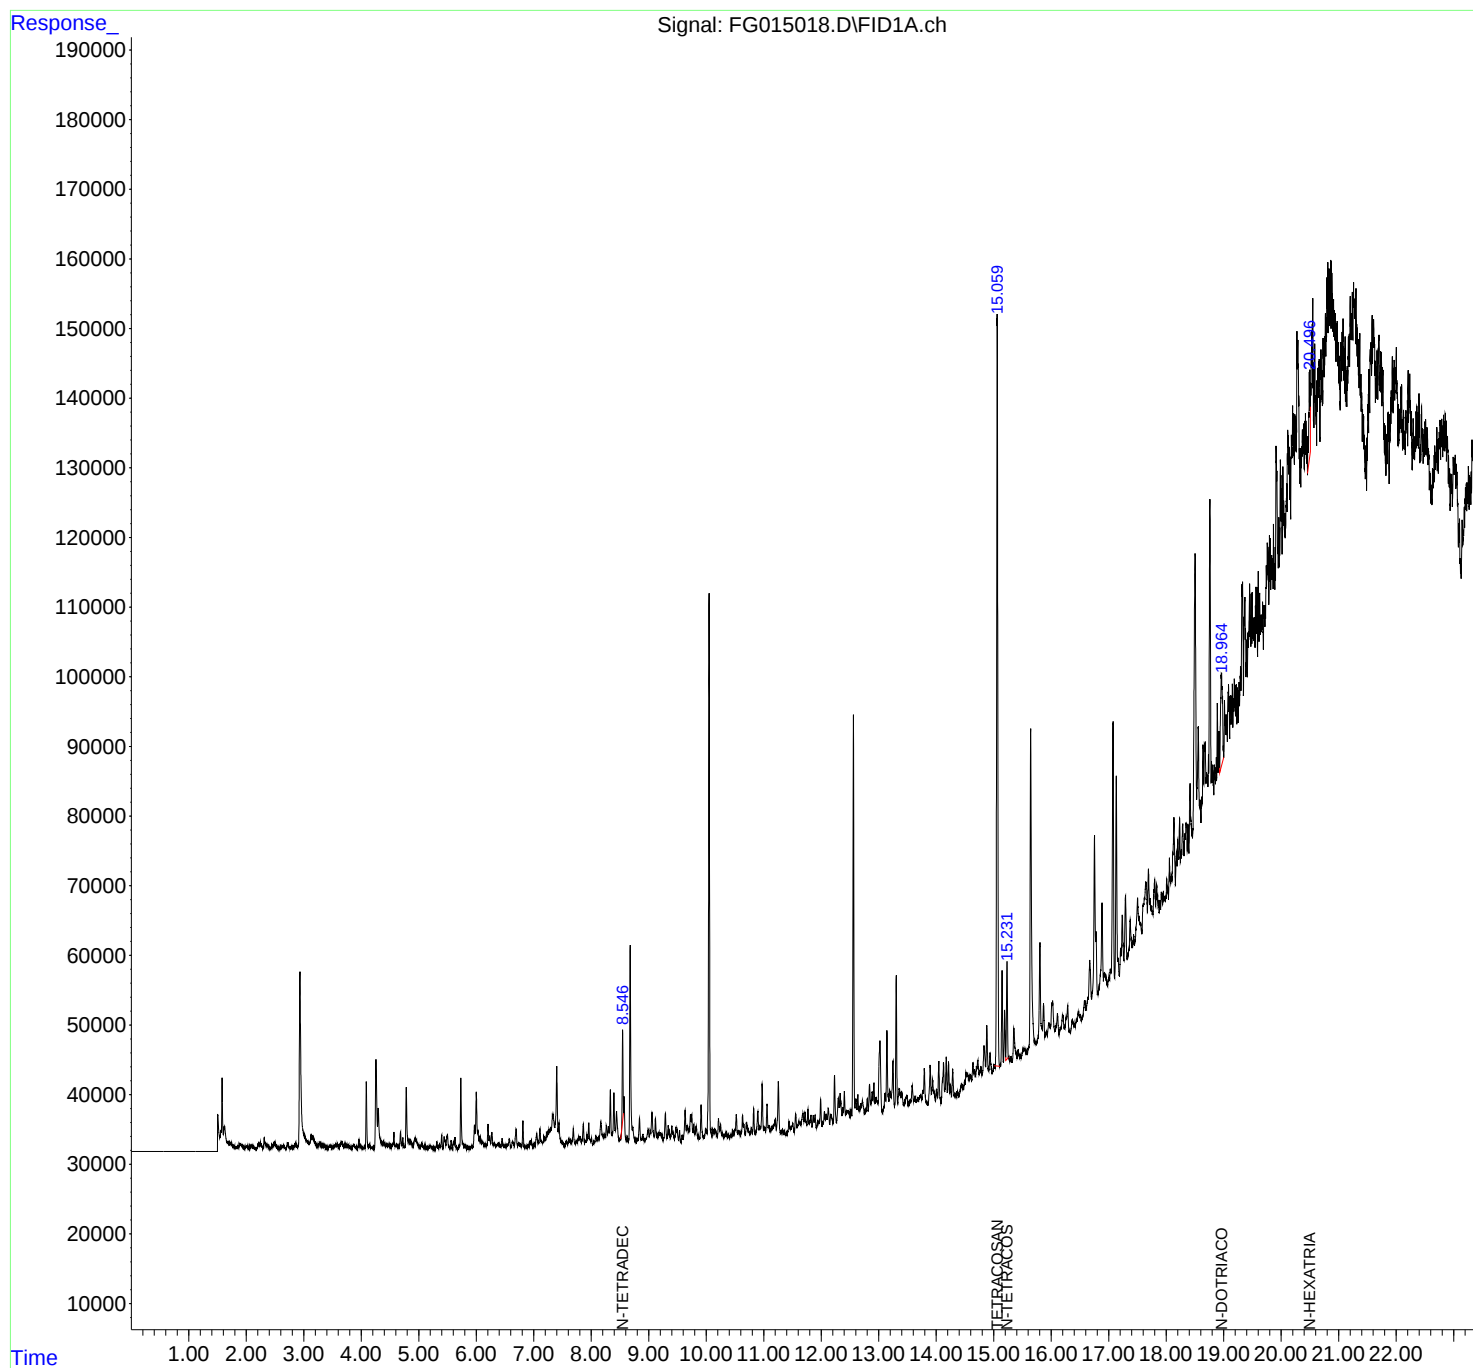


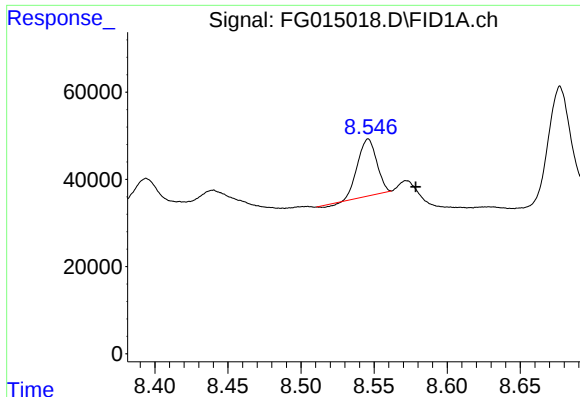

#4 N-TETRADECANE


R.T.: 8.546 min  
Delta R.T.: -0.033 min  
Response: 116755  
Conc: 0.87 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

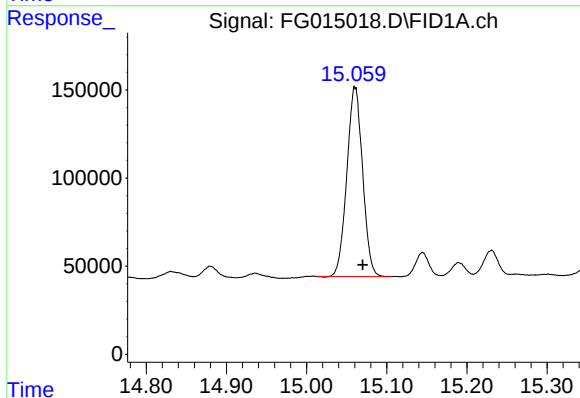


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.060 min  
Delta R.T.: -0.010 min  
Response: 1467932  
Conc: 10.98 ug/ml

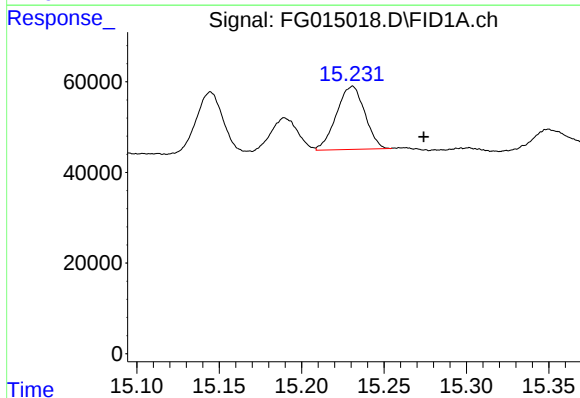


#10 N-TETRACOSANE

R.T.: 15.231 min  
Delta R.T.: -0.043 min  
Response: 166531  
Conc: 1.13 ug/ml

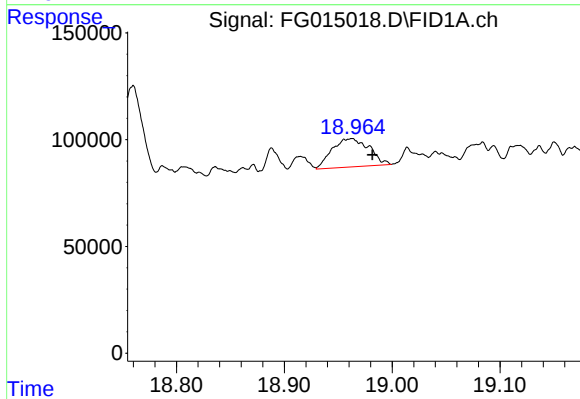

#14 N-DOTRIACONTANE

R.T.: 18.963 min  
Delta R.T.: -0.019 min  
Response: 316476  
Conc: 2.19 ug/ml

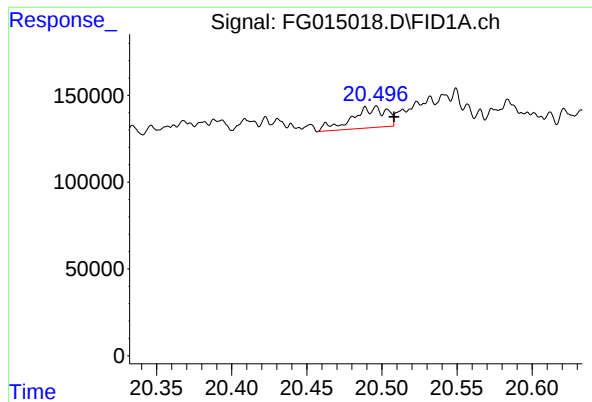

#16 N-HEXATRIACONTANE

R.T.: 20.496 min  
Delta R.T.: -0.012 min  
Response: 191735  
Conc: 1.72 ug/ml

Instrument :

FID\_G

ClientSampleId :