

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG122324\
Data File : FG015017.D
Signal(s) : FID1A.ch
Acq On : 23 Dec 2024 11:58
Operator : YP\AJ
Sample : P5318-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
AU-06-122024

Integration File: autoint1.e
Quant Time: Dec 24 00:27:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121924.M
Quant Title :
QLast Update : Thu Dec 19 16:42:40 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.057	1020760	7.637 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG122324\
Data File : FG015017.D
Signal(s) : FID1A.ch
Acq On : 23 Dec 2024 11:58
Operator : YP\AJ
Sample : P5318-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
AU-06-122024

Integration File: autoint1.e
Quant Time: Dec 24 00:27:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121924.M
Quant Title :
QLast Update : Thu Dec 19 16:42:40 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

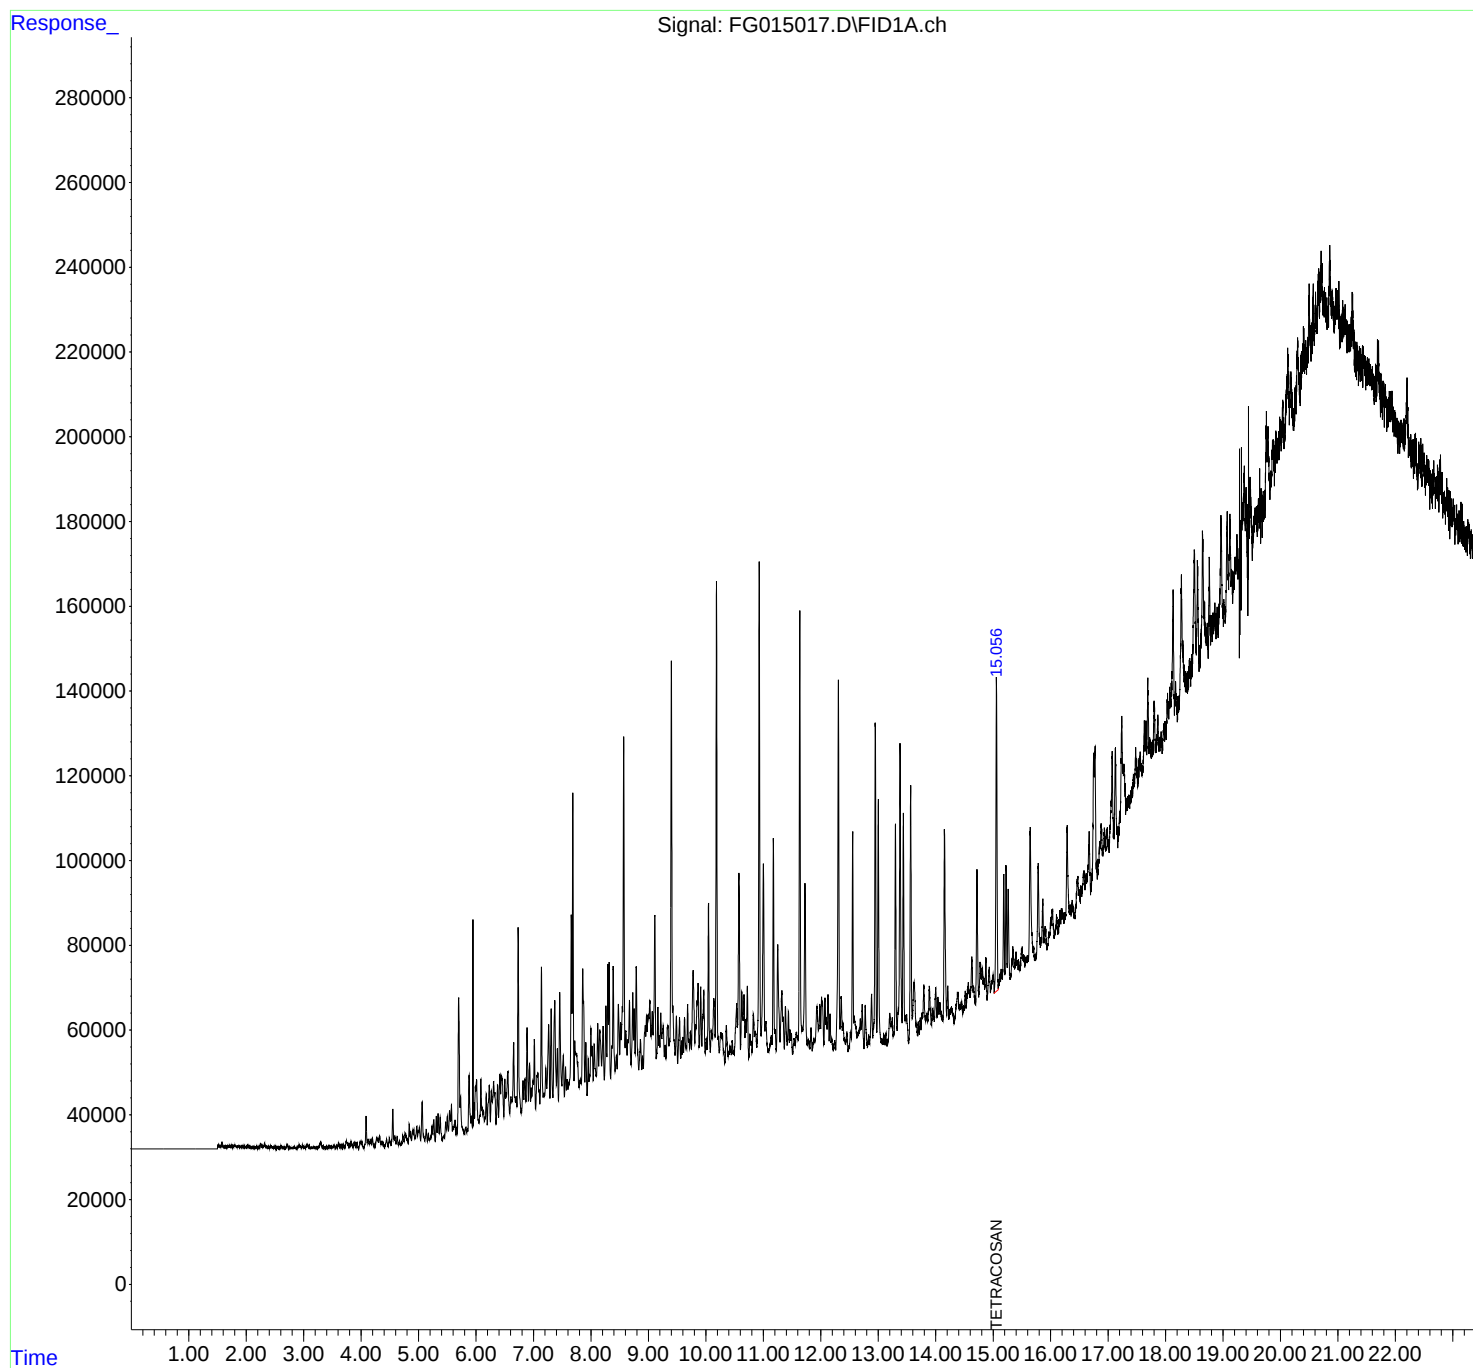

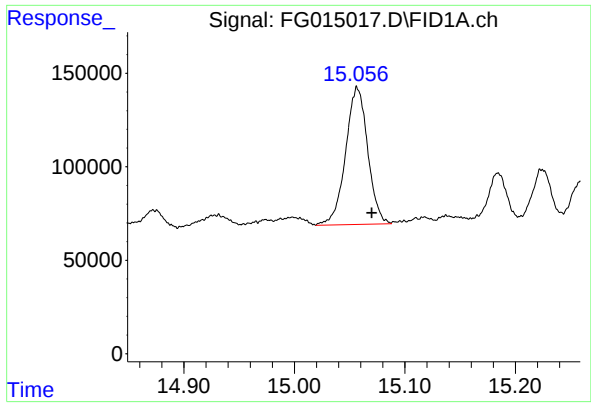

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.057 min
Delta R.T.: -0.013 min
Response: 1020760
Conc: 7.64 ug/ml

Instrument :
FID_G
ClientSampleId :
AU-06-122024