

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG122324\
Data File : FG015028.D
Signal(s) : FID1A.ch
Acq On : 23 Dec 2024 17:37
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Dec 24 00:30:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121924.M
Quant Title :
QLast Update : Thu Dec 19 16:42:40 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.058	2458731	18.396 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG122324\
Data File : FG015028.D
Signal(s) : FID1A.ch
Acq On : 23 Dec 2024 17:37
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Dec 24 00:30:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121924.M
Quant Title :
QLast Update : Thu Dec 19 16:42:40 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

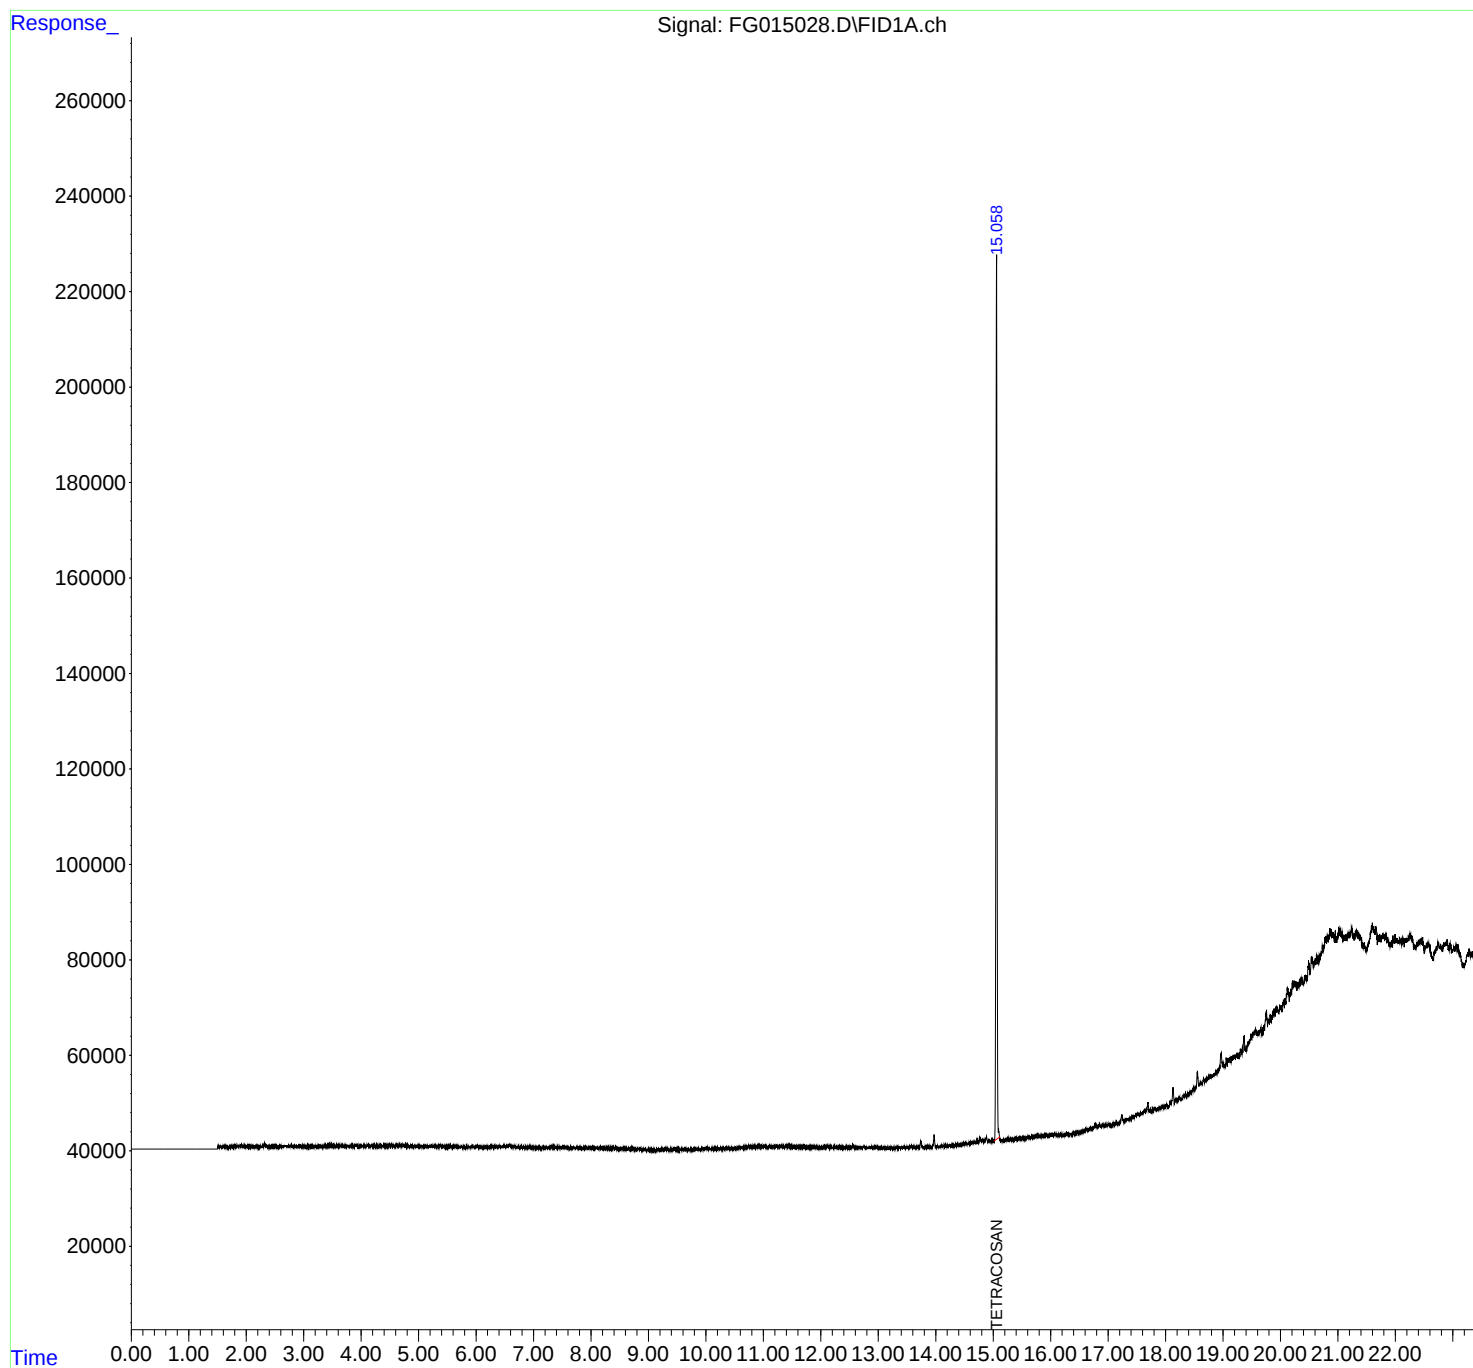

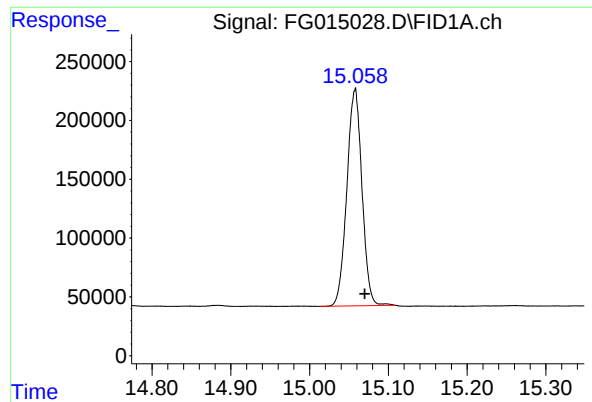

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.058 min
Delta R.T.: -0.012 min
Response: 2458731
Conc: 18.40 ug/ml

Instrument :
FID_G
ClientSampleId :
I.BLK