

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG122623\
Data File : FG013314.D
Signal(s) : FID1A.ch
Acq On : 26 Dec 2023 13:25
Operator : YP\AJ
Sample : PB158056BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB158056BL

Integration File: autoint1.e
Quant Time: Dec 26 22:29:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG120423.M
Quant Title :
QLast Update : Mon Dec 04 11:42:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.075	1650980	15.379 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG122623\
Data File : FG013314.D
Signal(s) : FID1A.ch
Acq On : 26 Dec 2023 13:25
Operator : YP\AJ
Sample : PB158056BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
PB158056BL

Integration File: autoint1.e
Quant Time: Dec 26 22:29:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG120423.M
Quant Title :
QLast Update : Mon Dec 04 11:42:34 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

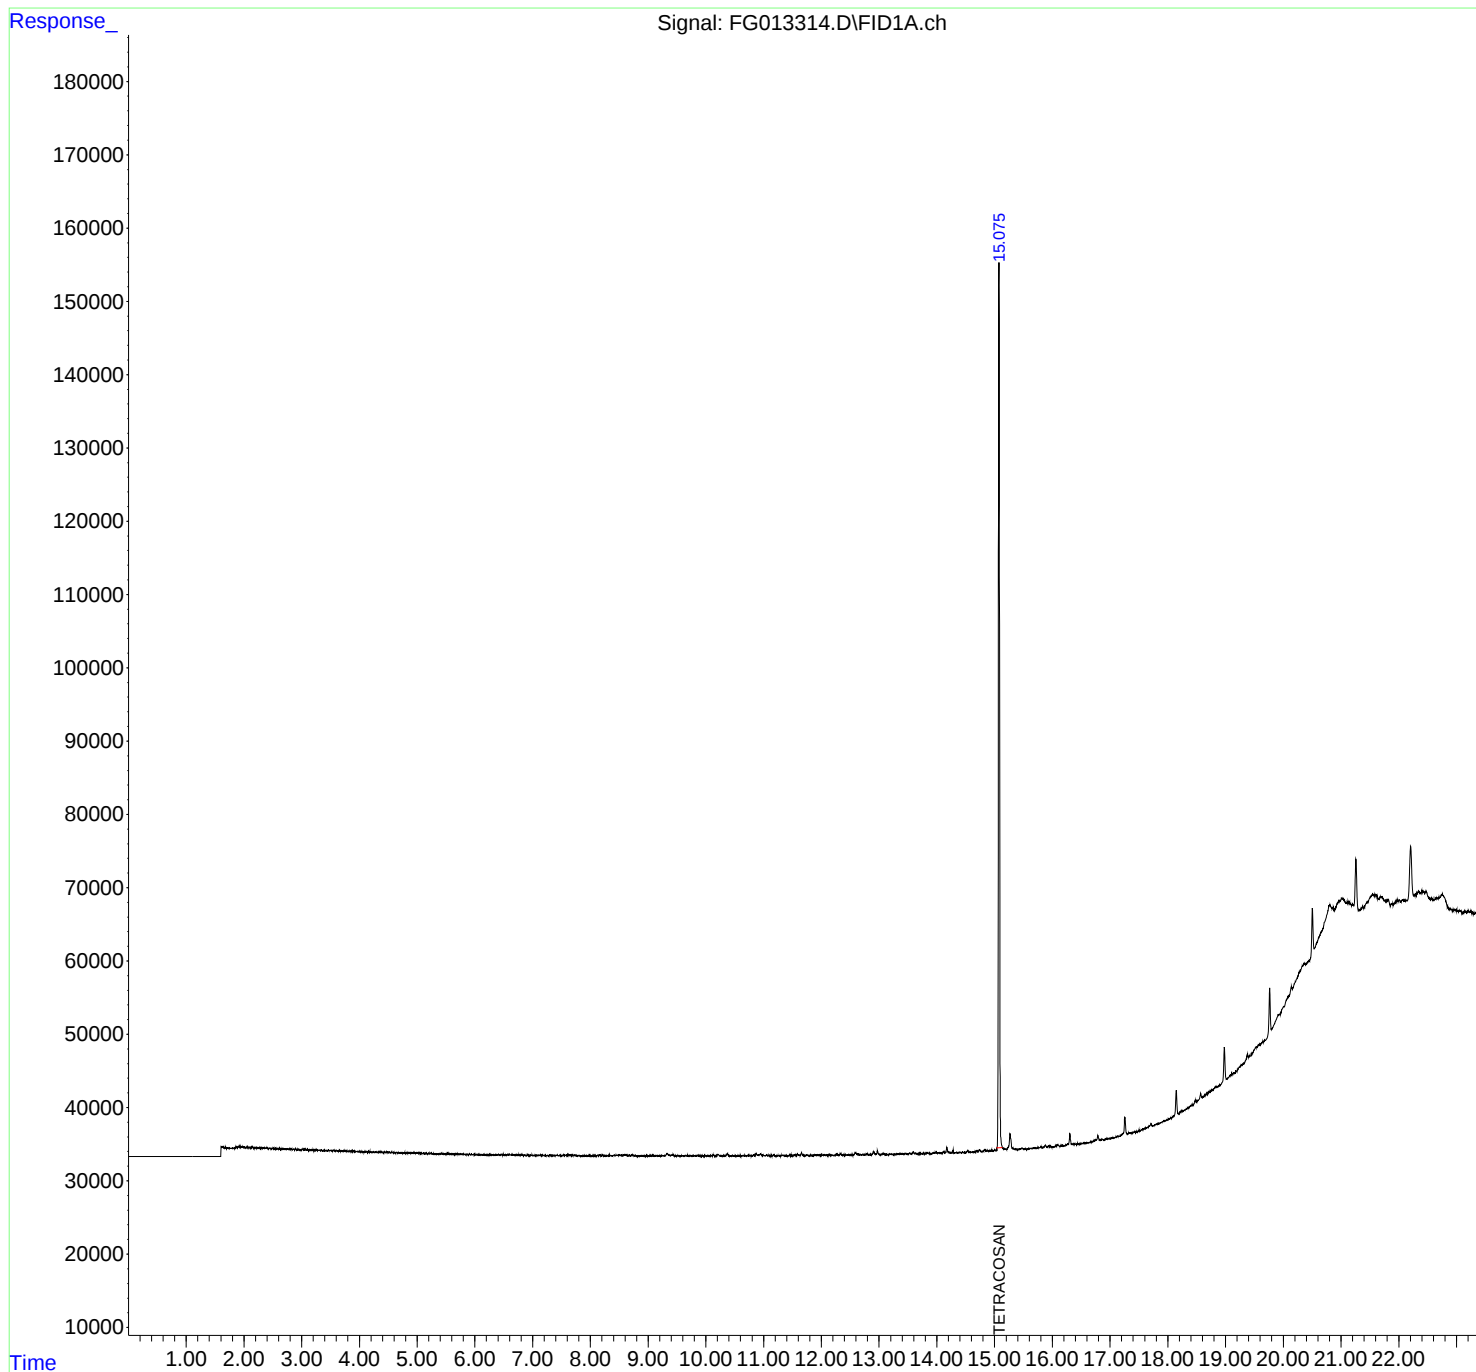

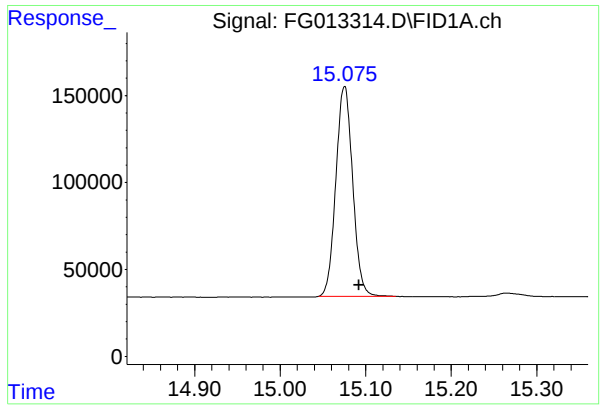

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.075 min
Delta R.T.: -0.017 min
Response: 1650980
Conc: 15.38 ug/ml

Instrument :
FID_G
ClientSampleId :
PB158056BL