

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG122718\
 Data File : FG003351.D
 Signal(s) : FID1A.ch
 Acq On : 27 Dec 2018 16:11
 Operator : AJ\SJ
 Sample : J6195-13 5X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 28 00:38:14 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121318.M
 Quant Title :
 QLast Update : Thu Dec 13 00:59:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.699	363312	2.929 ug/ml
Target Compounds				
3)	N-DODECANE	6.432	521504	3.833 ug/ml
4)	N-TETRADECANE	8.231	984336	7.133 ug/ml
5)	N-HEXADECANE	9.835	1003566	7.163 ug/ml
6)	N-OCTADECANE	11.281	719254	5.077 ug/ml
7)	N-EICOSANE	12.593	636120	4.503 ug/ml
8)	N-DOCOSANE	13.796	305083	2.169 ug/ml
10)	N-TETRACOSANE	14.901	687031	4.908 ug/ml
11)	N-HEXACOSANE	15.929	287122	2.060 ug/ml
12)	N-OCTACOSANE	16.884	165105	1.182 ug/ml
13)	N-TRIACONTANE	17.777	468183	3.301 ug/ml
14)	N-DOTRIACONTANE	18.617	583803	4.231 ug/ml
15)	N-TETRATRIACONTANE	19.403	301460	2.288 ug/ml
16)	N-HEXATRIACONTANE	20.153	260245	2.052 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG122718\
Data File : FG003351.D
Signal(s) : FID1A.ch
Acq On : 27 Dec 2018 16:11
Operator : AJ\SJ
Sample : J6195-13 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 28 00:38:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG121318.M
Quant Title :
QLast Update : Thu Dec 13 00:59:54 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

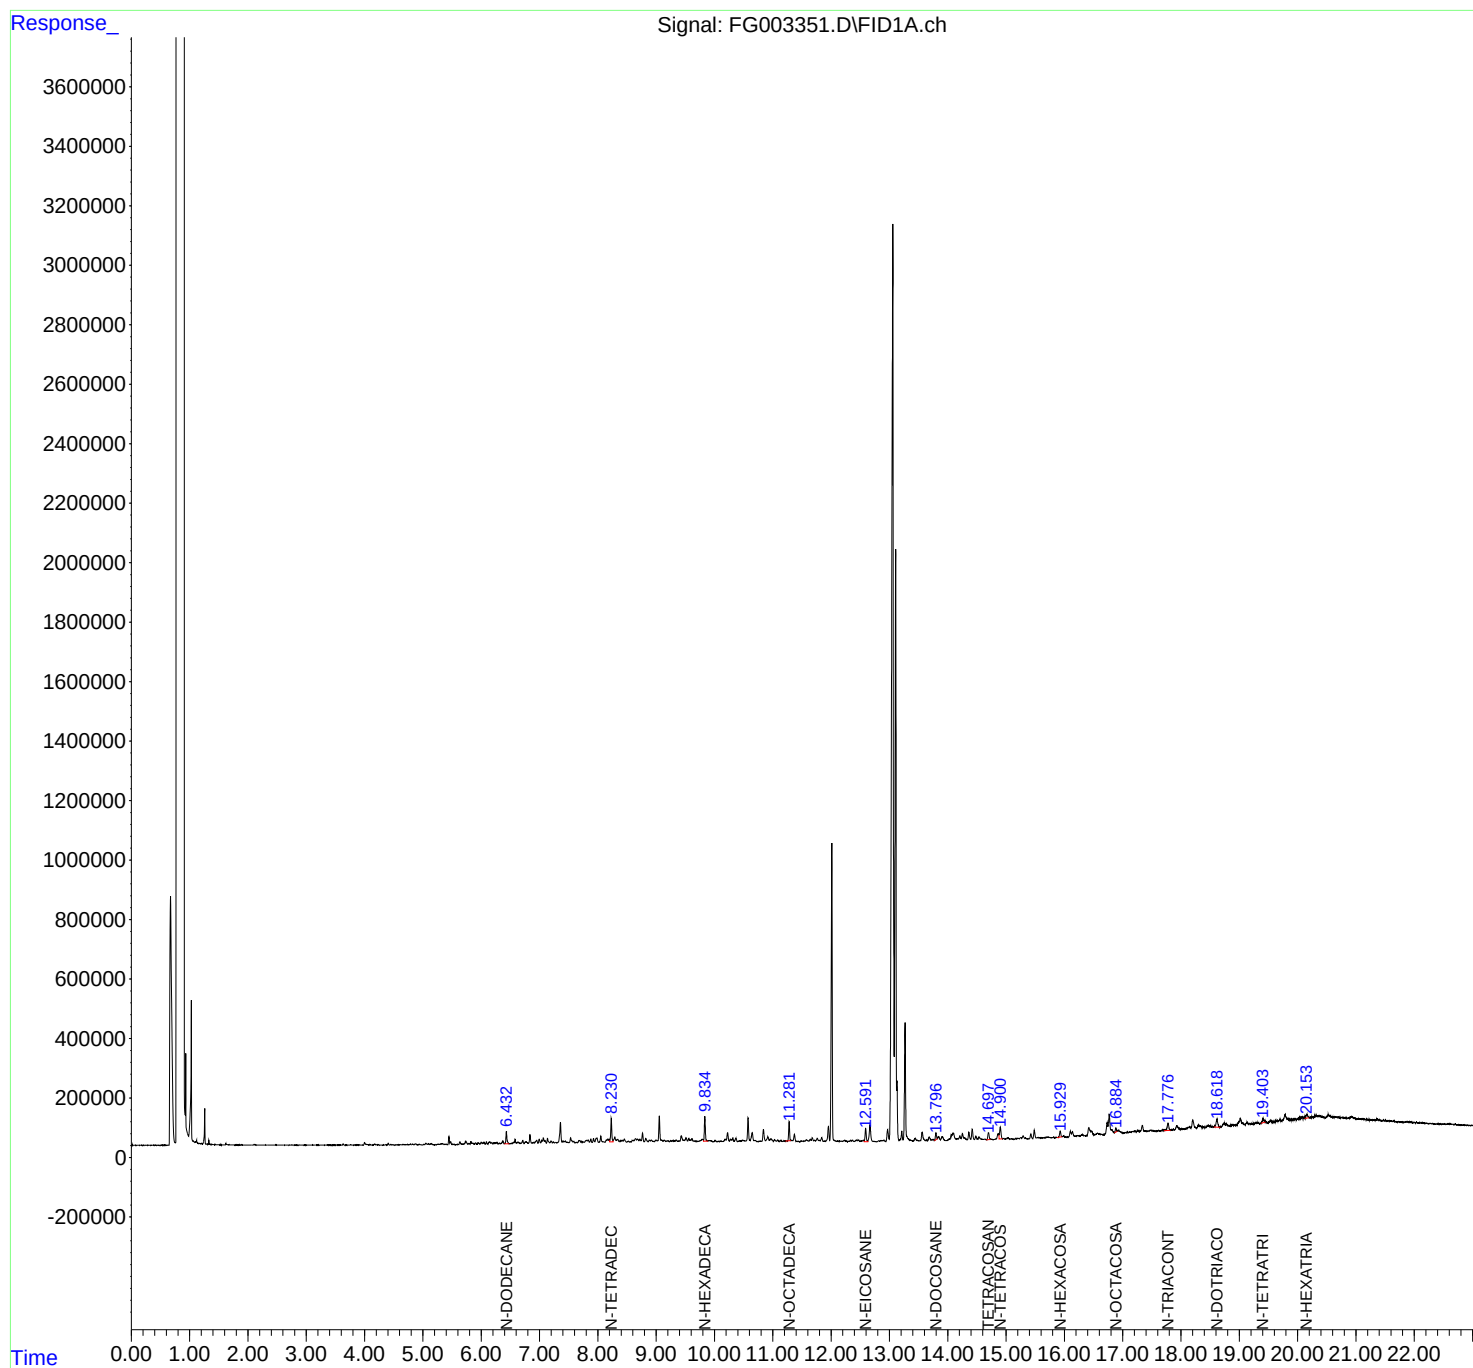

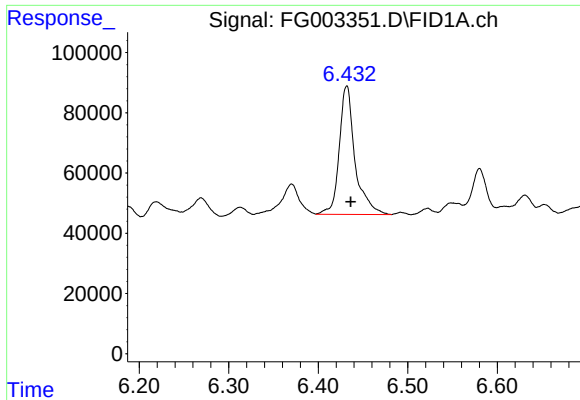


#3 N-DODECANE

R.T.: 6.432 min
Delta R.T.: -0.005 min
Response: 521504
Conc: 3.83 ug/ml

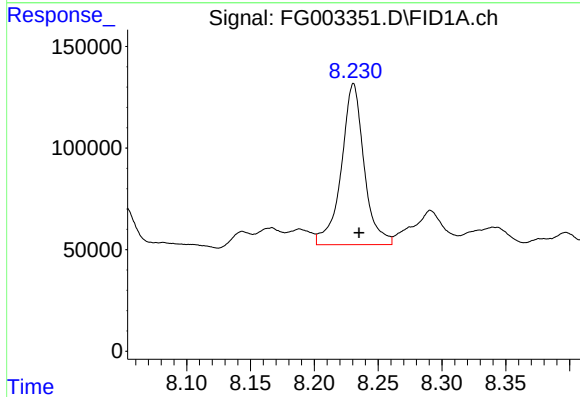


#4 N-TETRADECANE

R.T.: 8.231 min
Delta R.T.: -0.004 min
Response: 984336
Conc: 7.13 ug/ml

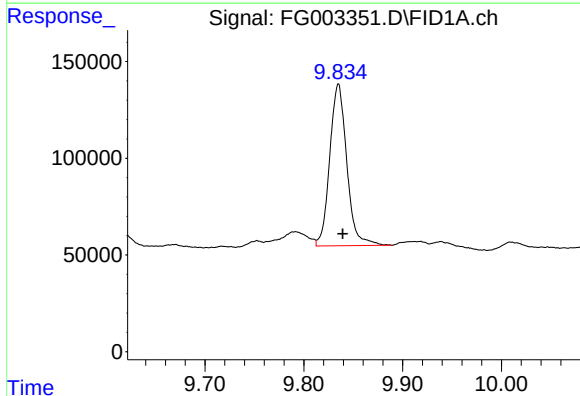


#5 N-HEXADECANE

R.T.: 9.835 min
Delta R.T.: -0.004 min
Response: 1003566
Conc: 7.16 ug/ml

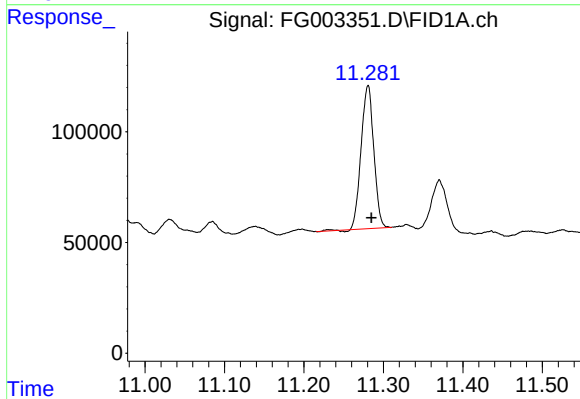


#6 N-OCTADECANE

R.T.: 11.281 min
Delta R.T.: -0.004 min
Response: 719254
Conc: 5.08 ug/ml

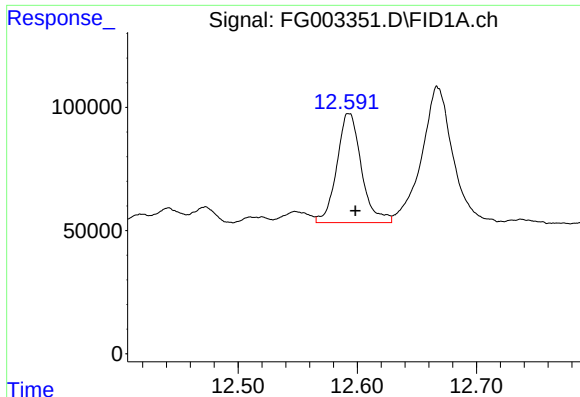


#7 N-EICOSANE

R.T.: 12.593 min
Delta R.T.: -0.006 min
Response: 636120
Conc: 4.50 ug/ml

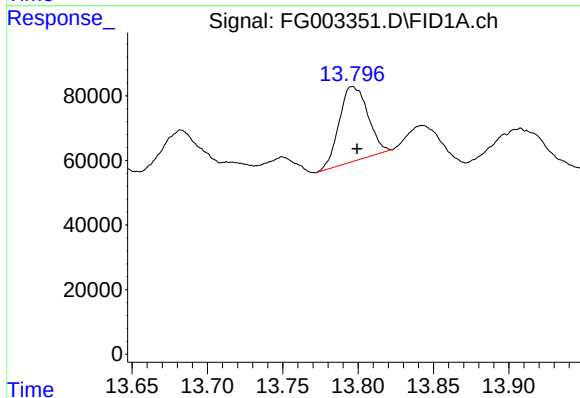


#8 N-DOCOSANE

R.T.: 13.796 min
Delta R.T.: -0.003 min
Response: 305083
Conc: 2.17 ug/ml

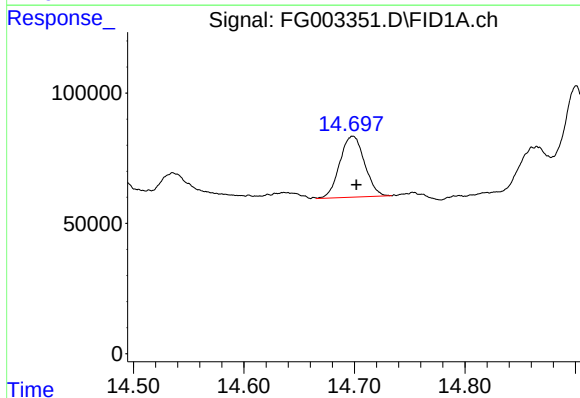


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.699 min
Delta R.T.: -0.003 min
Response: 363312
Conc: 2.93 ug/ml

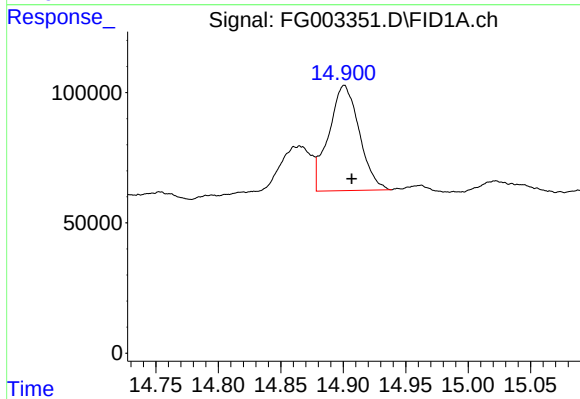


#10 N-TETRACOSANE

R.T.: 14.901 min
Delta R.T.: -0.006 min
Response: 687031
Conc: 4.91 ug/ml

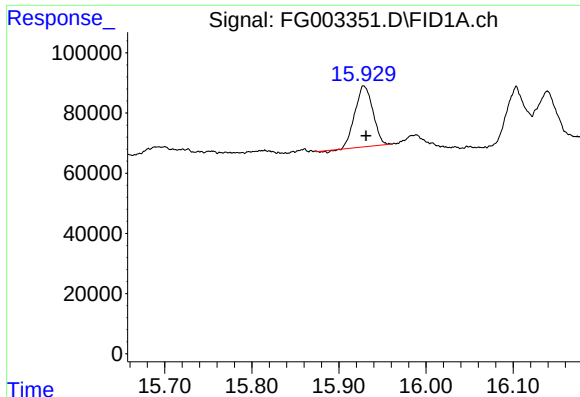


#11 N-HEXACOSANE

R.T.: 15.929 min
Delta R.T.: -0.002 min
Response: 287122
Conc: 2.06 ug/ml

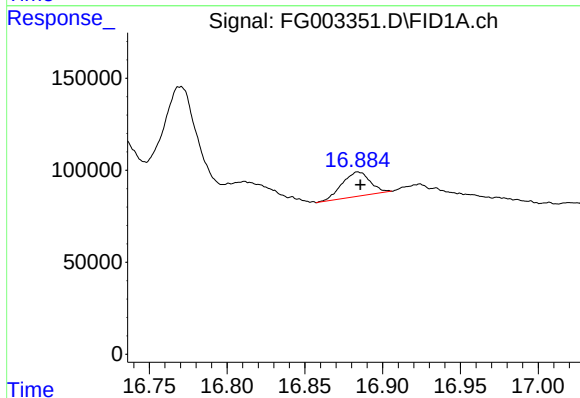


#12 N-OCTACOSANE

R.T.: 16.884 min
Delta R.T.: -0.001 min
Response: 165105
Conc: 1.18 ug/ml

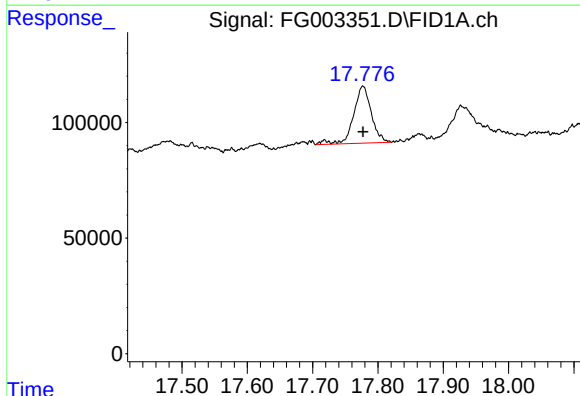


#13 N-TRIACONTANE

R.T.: 17.777 min
Delta R.T.: 0.000 min
Response: 468183
Conc: 3.30 ug/ml

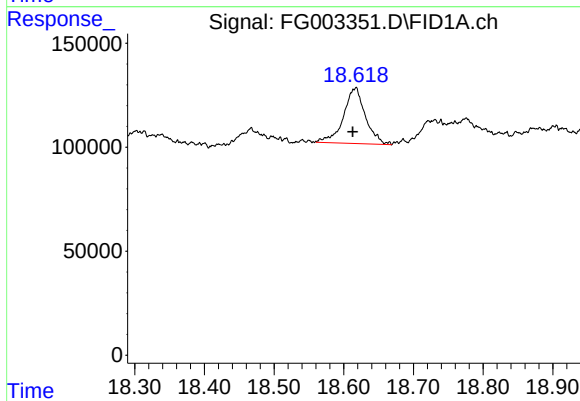

#14 N-DOTRIACONTANE

R.T.: 18.617 min
Delta R.T.: 0.005 min
Response: 583803
Conc: 4.23 ug/ml

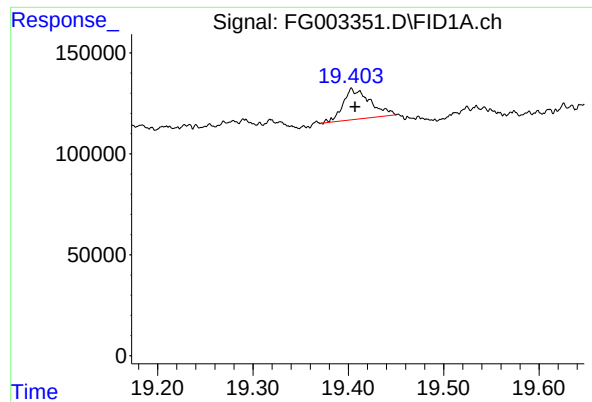


#15 N-TETRATRIACONTANE

R.T.: 19.403 min

Delta R.T.: -0.004 min

Response: 301460

Conc: 2.29 ug/ml

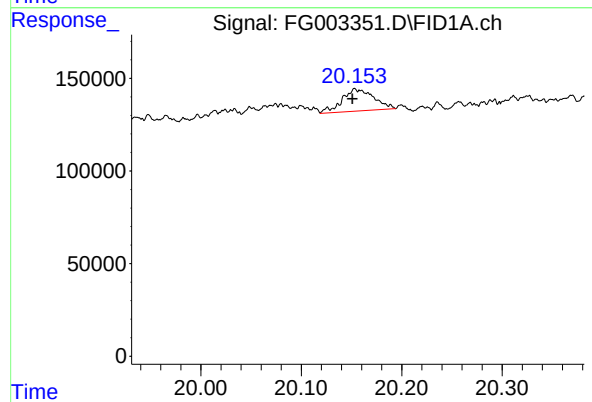

#16 N-HEXATRIACONTANE

R.T.: 20.153 min

Delta R.T.: 0.002 min

Response: 260245

Conc: 2.05 ug/ml