

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG122719\  
Data File : FG006429.D  
Signal(s) : FID1A.ch  
Acq On : 27 Dec 2019 14:33  
Operator : DD\AJ  
Sample : K6435-02  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Dec 27 23:54:41 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG122619.M  
Quant Title :  
QLast Update : Fri Dec 27 04:12:53 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 14.509 | 3194106  | 30.258 ug/ml |
| Target Compounds              |        |          |              |
| 11) N-HEXACOSANE              | 15.710 | 345738   | 2.897 ug/ml  |
| 12) N-OCTACOSANE              | 16.643 | 391071   | 3.306 ug/ml  |
| 13) N-TRIACONTANE             | 17.514 | 399551   | 3.388 ug/ml  |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_G\Data\FG122719\  
Data File : FG006429.D  
Signal(s) : FID1A.ch  
Acq On : 27 Dec 2019 14:33  
Operator : DD\AJ  
Sample : K6435-02  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
FID\_G  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Dec 27 23:54:41 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_G\Method\FG122619.M  
Quant Title :  
QLast Update : Fri Dec 27 04:12:53 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

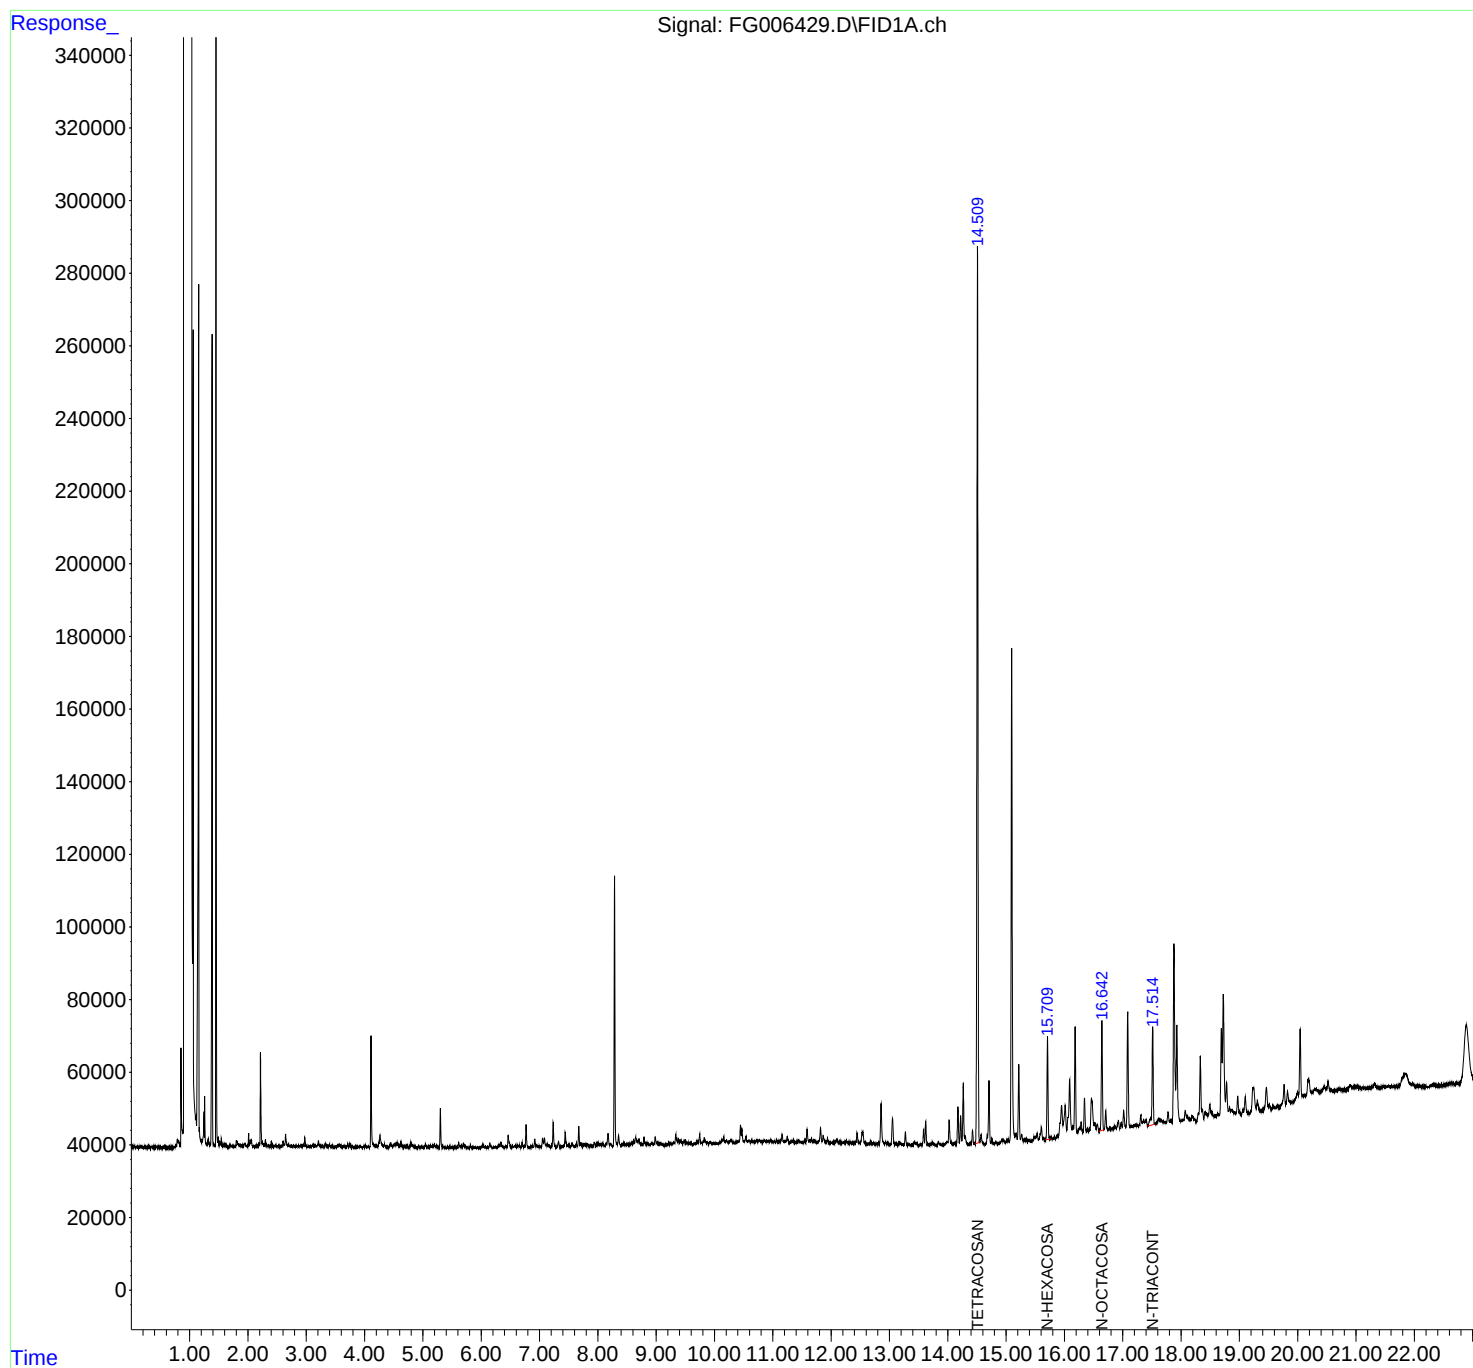


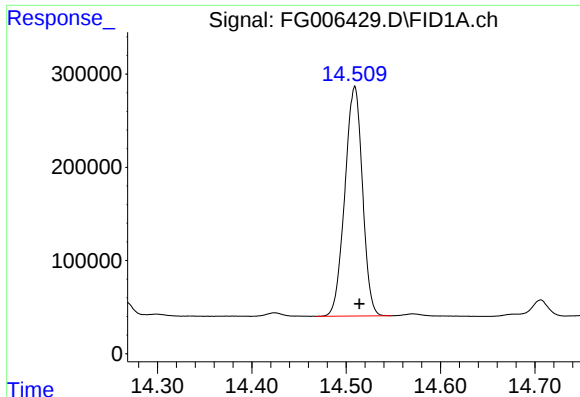

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.509 min  
Delta R.T.: -0.005 min  
Response: 3194106  
Conc: 30.26 ug/ml

Instrument :  
FID\_G  
ClientSampleId :

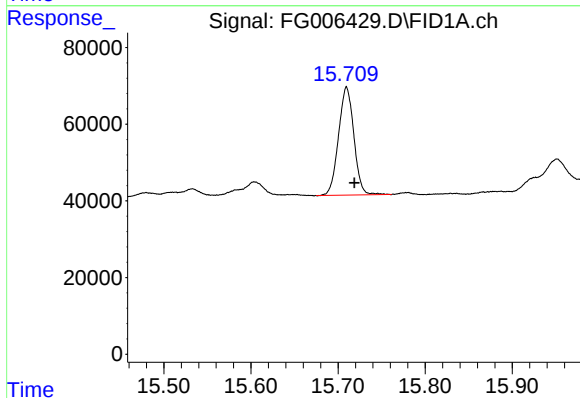


#11 N-HEXACOSANE

R.T.: 15.710 min  
Delta R.T.: -0.009 min  
Response: 345738  
Conc: 2.90 ug/ml

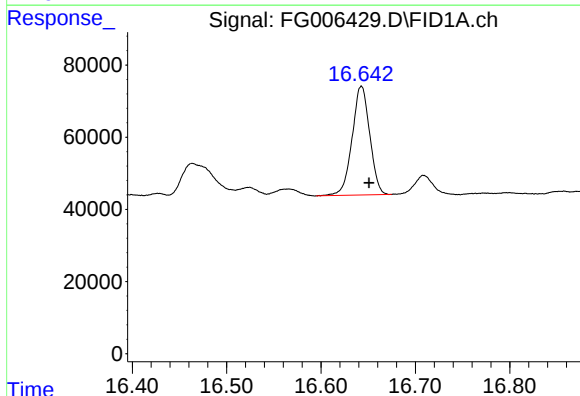

#12 N-OCTACOSANE

R.T.: 16.643 min  
Delta R.T.: -0.008 min  
Response: 391071  
Conc: 3.31 ug/ml

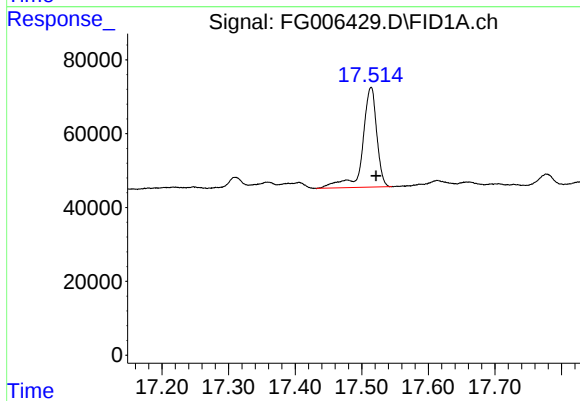

#13 N-TRIACONTANE

R.T.: 17.514 min  
Delta R.T.: -0.008 min  
Response: 399551  
Conc: 3.39 ug/ml