

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG123020\
 Data File : FG007492.D
 Signal(s) : FID1A.ch
 Acq On : 30 Dec 2020 12:28
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 31 01:38:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG120220.M
 Quant Title :
 QLast Update : Thu Dec 03 08:50:10 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.458	5784213	38.387 ug/ml
6) N-OCTADECANE	11.310	101318	0.661 ug/ml
12) N-OCTACOSANE	16.903	4798273	34.559 ug/ml
13) N-TRIACONTANE	17.789	208983	1.598 ug/ml
14) N-DOTRIACONTANE	18.622	306222	2.671 ug/ml
15) N-TETRATRIACONTANE	19.406	221244	2.463 ug/ml
16) N-HEXATRIACONTANE	20.150	175504	2.649 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG123020\
Data File : FG007492.D
Signal(s) : FID1A.ch
Acq On : 30 Dec 2020 12:28
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 31 01:38:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG120220.M
Quant Title :
QLast Update : Thu Dec 03 08:50:10 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

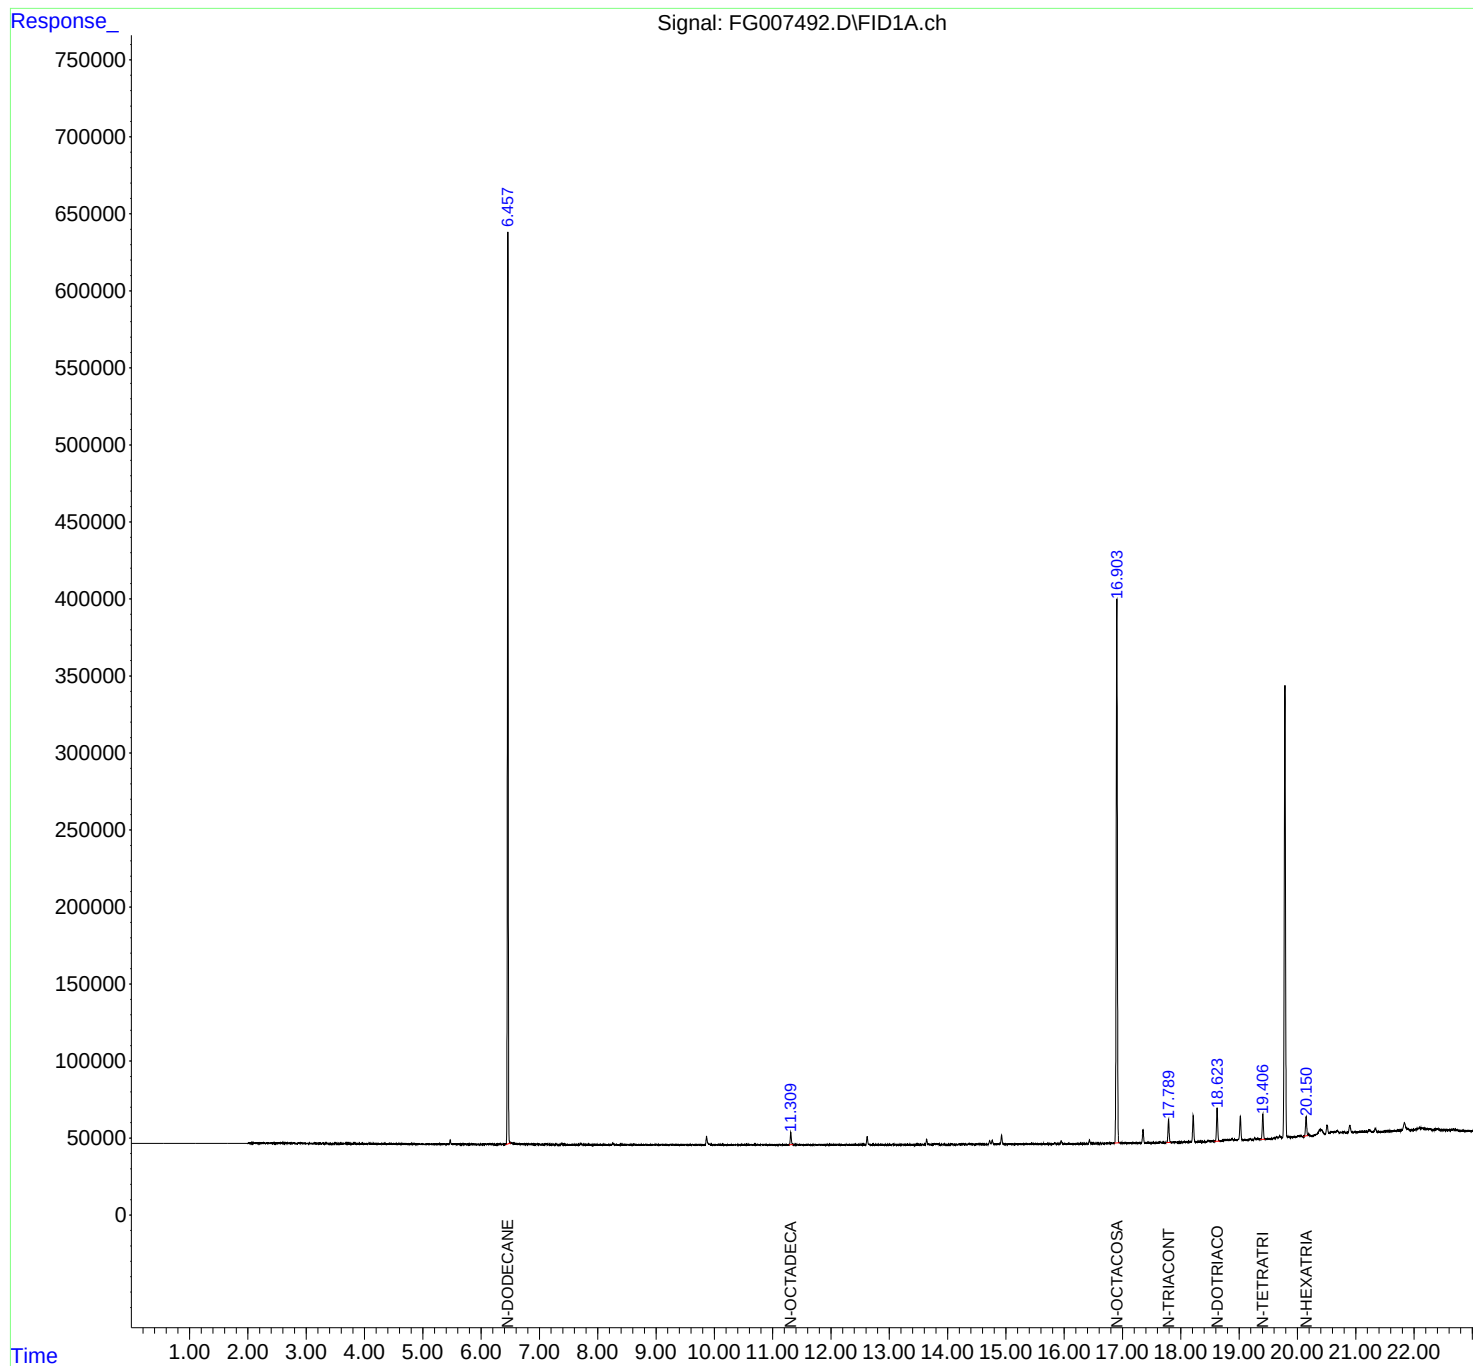


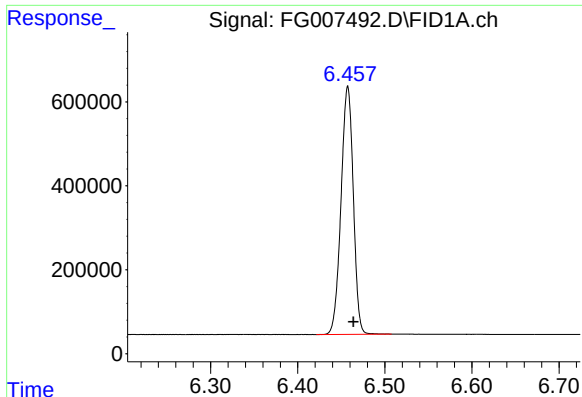

#3 N-DODECANE


R.T.: 6.458 min
Delta R.T.: -0.006 min
Response: 5784213
Conc: 38.39 ug/ml

Instrument :
FID_G
ClientSampleId :

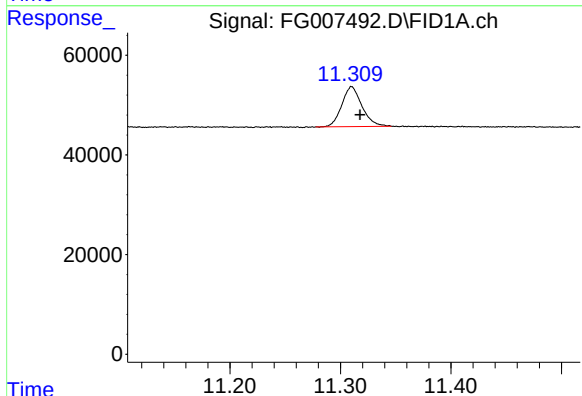


#6 N-OCTADECANE

R.T.: 11.310 min
Delta R.T.: -0.008 min
Response: 101318
Conc: 0.66 ug/ml

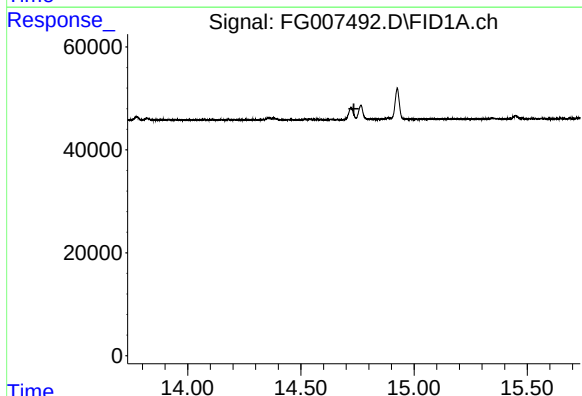


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.734 min
Response: 0
Conc: N.D.

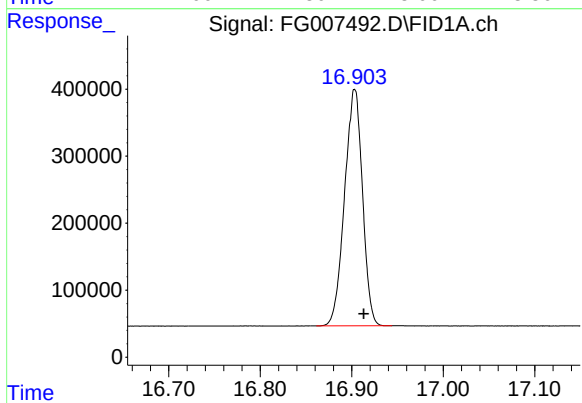

#12 N-OCTACOSANE


R.T.: 16.903 min
Delta R.T.: -0.010 min
Response: 4798273
Conc: 34.56 ug/ml

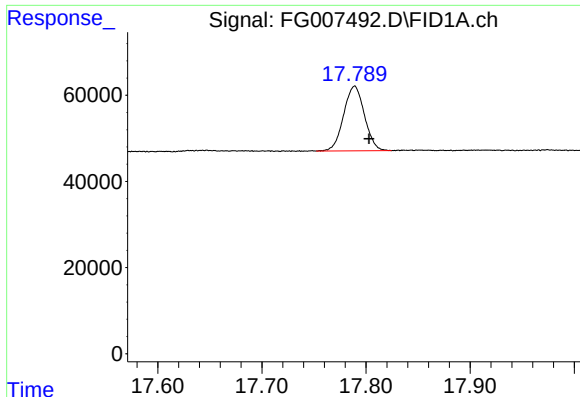

#13 N-TRIACONTANE


R.T.: 17.789 min
Delta R.T.: -0.014 min
Response: 208983
Conc: 1.60 ug/ml

Instrument :
FID_G
ClientSampleId :

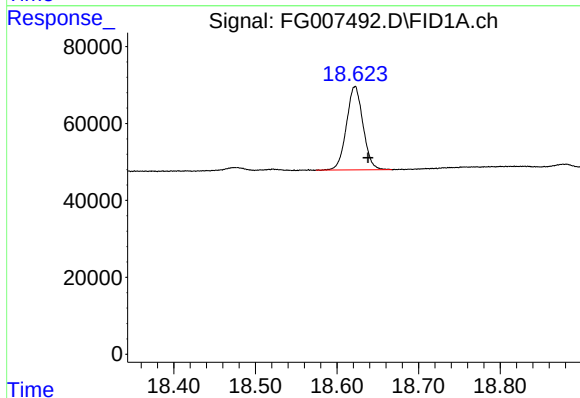


#14 N-DOTRIACONTANE

R.T.: 18.622 min
Delta R.T.: -0.016 min
Response: 306222
Conc: 2.67 ug/ml

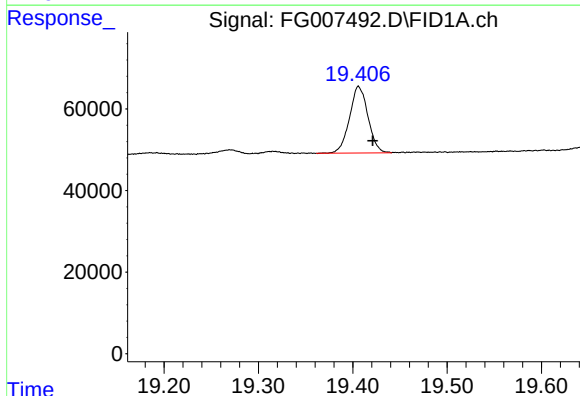

#15 N-TETRATRIACONTANE

R.T.: 19.406 min
Delta R.T.: -0.015 min
Response: 221244
Conc: 2.46 ug/ml

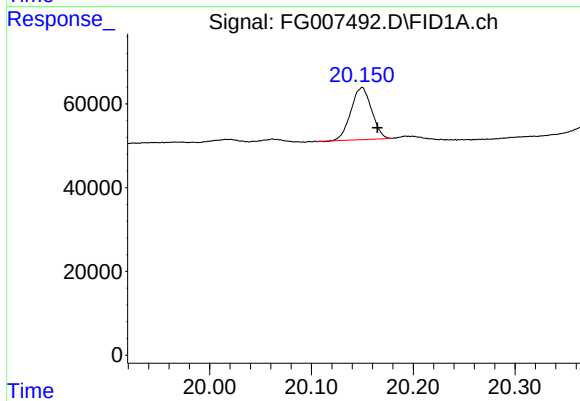

#16 N-HEXATRIACONTANE

R.T.: 20.150 min
Delta R.T.: -0.015 min
Response: 175504
Conc: 2.65 ug/ml