

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG123124AL\
 Data File : FG015039.D
 Signal(s) : FID1A.ch
 Acq On : 31 Dec 2024 08:09
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jan 01 01:05:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 122024.M
 Quant Title : GC Extractables
 QLast Update : Fri Dec 20 13:49:57 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

11) T	n-Heneicosane (C21)	13.556	57078	0.394 ug/ml
13) T	n-Docosane (C22)	14.100f	76805	0.526 ug/ml
14) T	n-Tetracosane (C24)	15.256	83732	0.561 ug/ml
15) T	n-Hexacosane (C26)	16.281	82628	0.551 ug/ml
16) T	n-Octacosane (C28)	17.235	98092	0.655 ug/ml
17) T	n-Tricontane (C30)	18.125	98848	0.644 ug/ml
18) T	n-Dotriacontane (C32)	18.962	154325	1.046 ug/ml
19) T	n-Tetratriacontane (C34)	19.747	65802	0.516 ug/ml
20) T	n-Hexatriacontane (C36)	20.490	57545	0.533 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG123124AL\
Data File : FG015039.D
Signal(s) : FID1A.ch
Acq On : 31 Dec 2024 08:09
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 01 01:05:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 122024.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 13:49:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

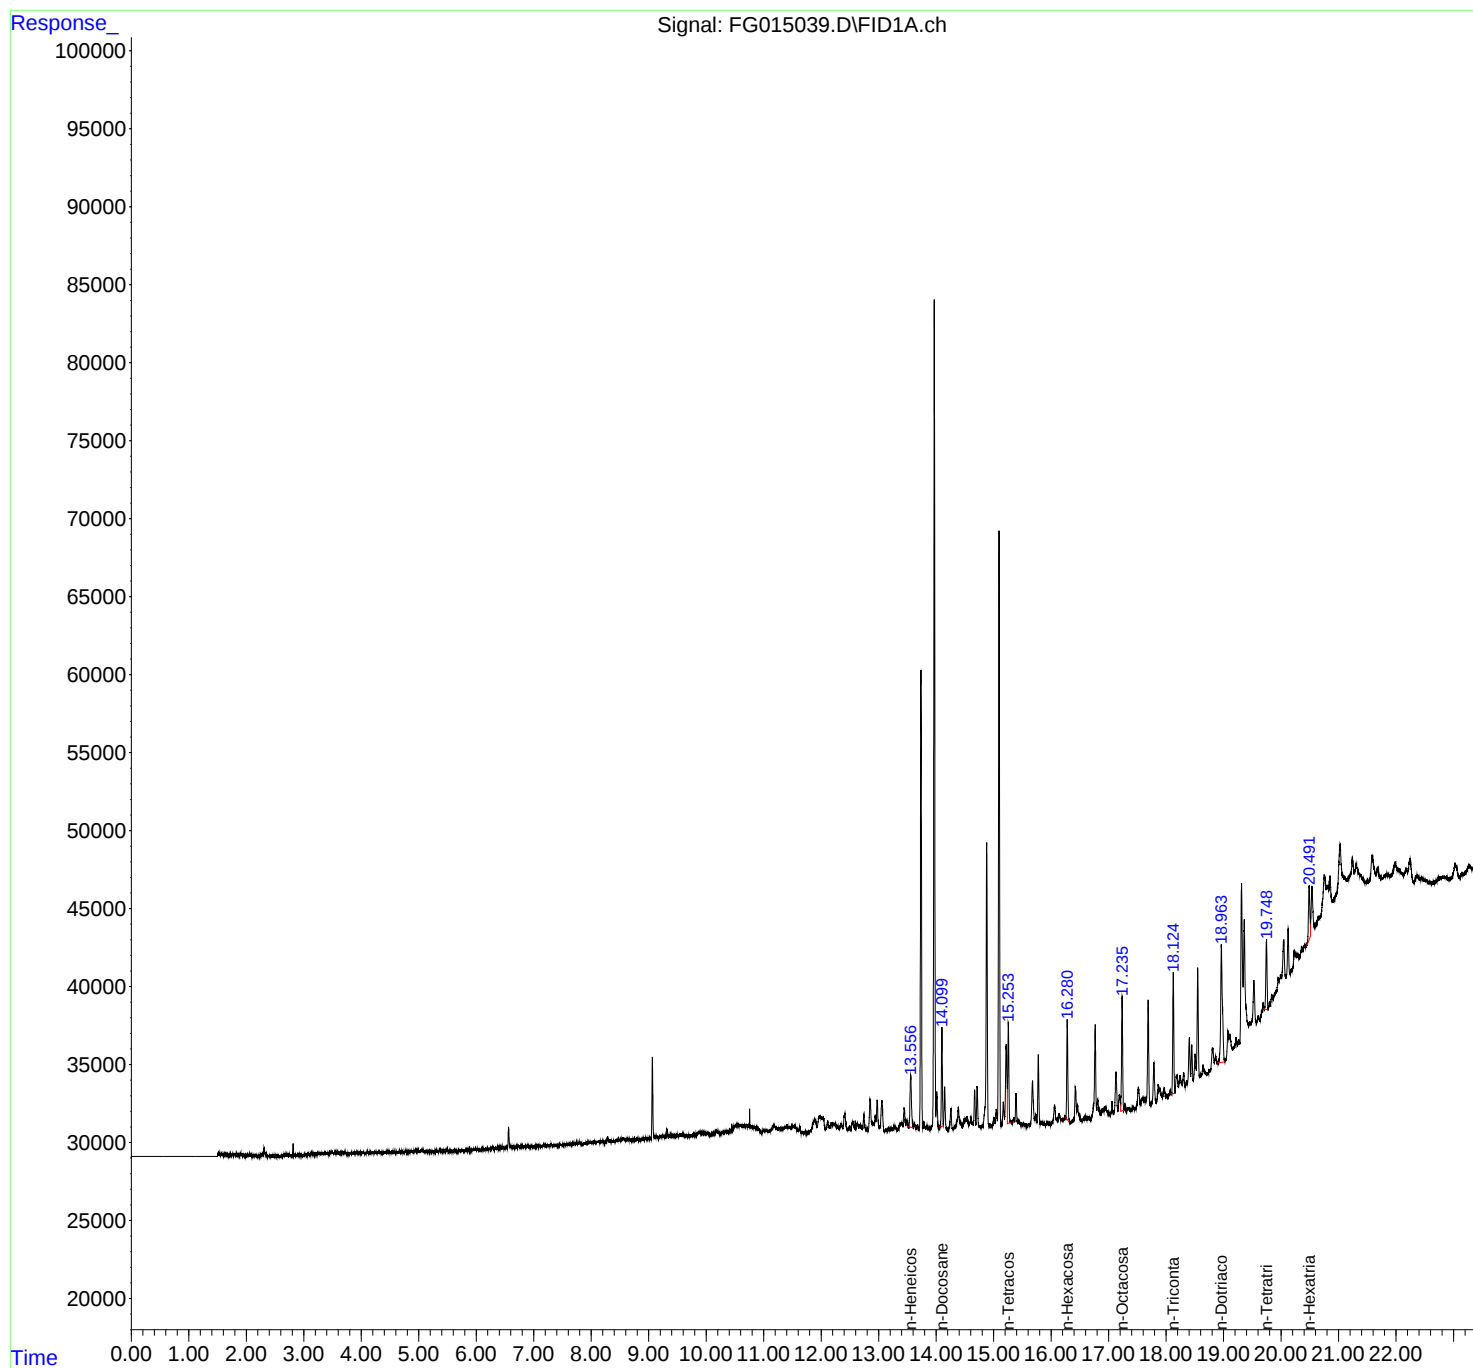


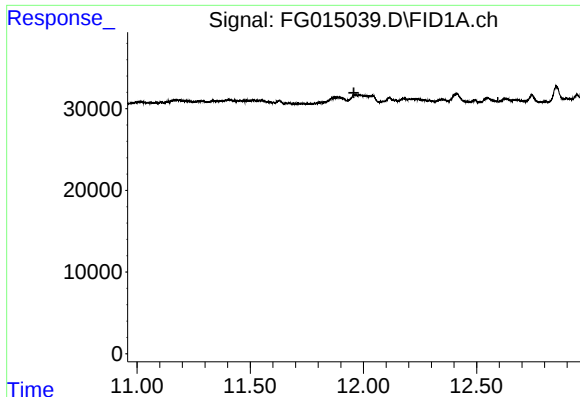

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.958 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

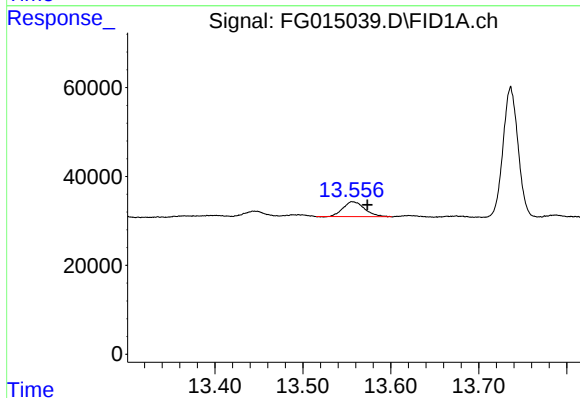


#11 n-Heneicosane (C21)

R.T.: 13.556 min
Delta R.T.: -0.017 min
Response: 57078
Conc: 0.39 ug/ml

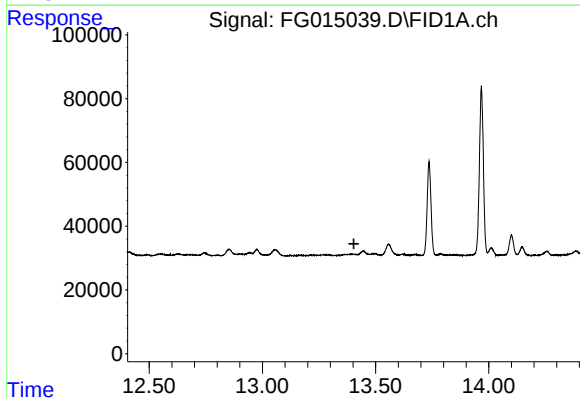


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.404 min
Response: 0
Conc: N.D.

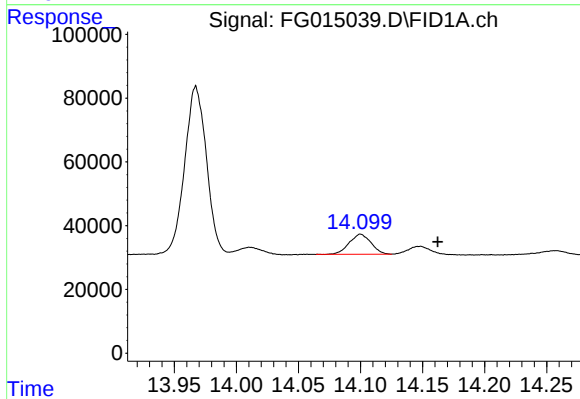

#13 n-Docosane (C22)


R.T.: 14.100 min
Delta R.T.: -0.062 min
Response: 76805
Conc: 0.53 ug/ml

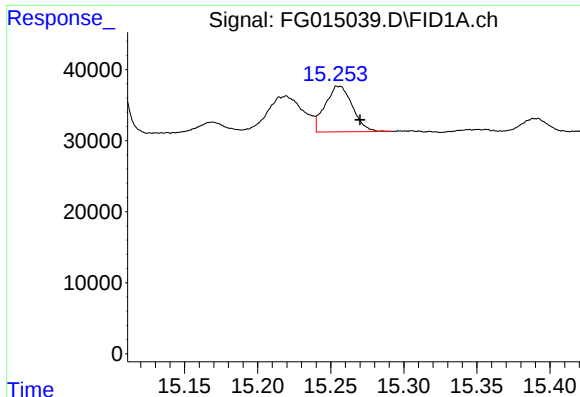

#14 n-Tetracosane (C24)


R.T.: 15.256 min
Delta R.T.: -0.014 min
Response: 83732
Conc: 0.56 ug/ml

Instrument :
FID_G
ClientSampleId :

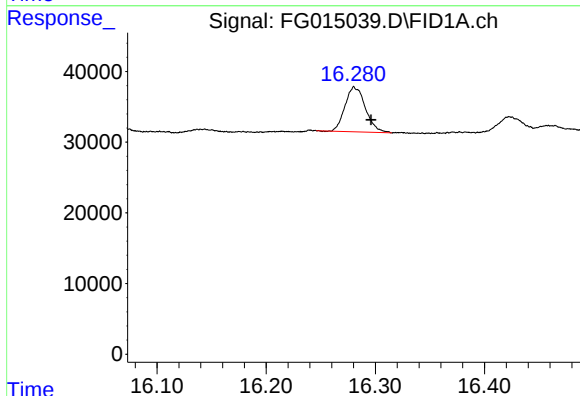


#15 n-Hexacosane (C26)

R.T.: 16.281 min
Delta R.T.: -0.016 min
Response: 82628
Conc: 0.55 ug/ml

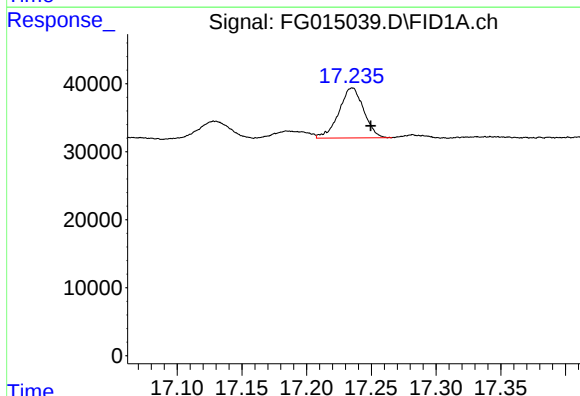


#16 n-Octacosane (C28)

R.T.: 17.235 min
Delta R.T.: -0.014 min
Response: 98092
Conc: 0.66 ug/ml

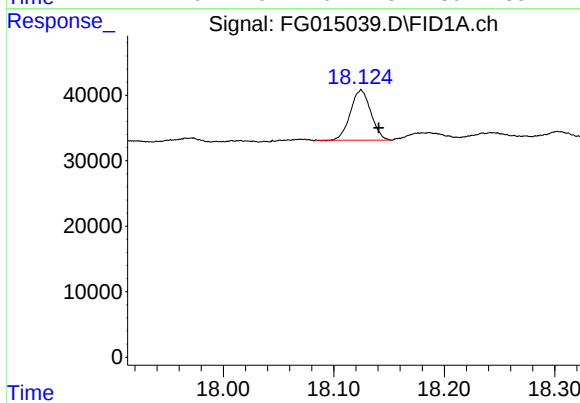

#17 n-Tricontane (C30)


R.T.: 18.125 min
Delta R.T.: -0.016 min
Response: 98848
Conc: 0.64 ug/ml

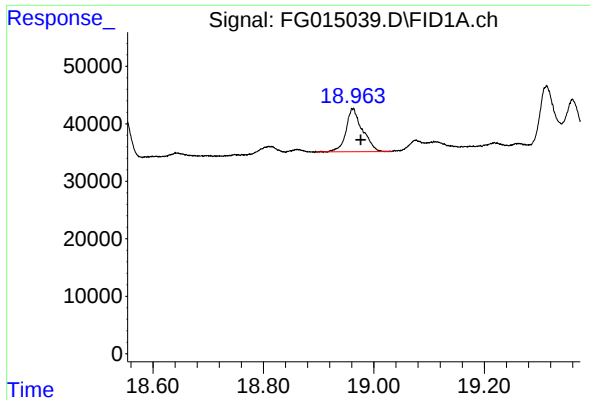

#18 n-Dotriacontane (C32)


R.T.: 18.962 min
Delta R.T.: -0.014 min
Response: 154325
Conc: 1.05 ug/ml

Instrument :
FID_G
ClientSampleId :

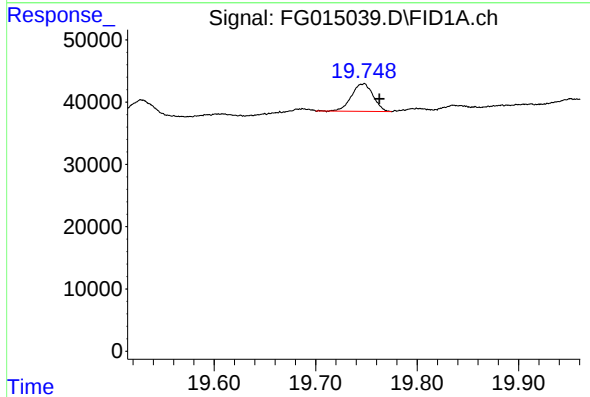

#19 n-Tetratriacontane (C34)

R.T.: 19.747 min
Delta R.T.: -0.016 min
Response: 65802
Conc: 0.52 ug/ml

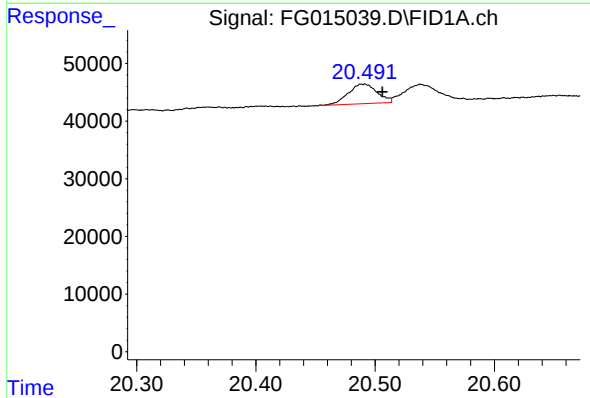

#20 n-Hexatriacontane (C36)

R.T.: 20.490 min
Delta R.T.: -0.017 min
Response: 57545
Conc: 0.53 ug/ml