

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG123124AL\
Data File : FG015040.D
Signal(s) : FID1A.ch
Acq On : 31 Dec 2024 08:37
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 01 01:05:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 122024.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 13:49:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
13) T	n-Docosane (C22)	14.098f	79731	0.546 ug/ml
14) T	n-Tetracosane (C24)	15.254	63650	0.426 ug/ml
15) T	n-Hexacosane (C26)	16.279	81092	0.540 ug/ml
16) T	n-Octacosane (C28)	17.232	93093	0.622 ug/ml
17) T	n-Tricontane (C30)	18.123	100029	0.652 ug/ml
18) T	n-Dotriacontane (C32)	18.958	101833	0.690 ug/ml
19) T	n-Tetratriacontane (C34)	19.743	60316	0.473 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG123124AL\
Data File : FG015040.D
Signal(s) : FID1A.ch
Acq On : 31 Dec 2024 08:37
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 01 01:05:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 122024.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 13:49:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

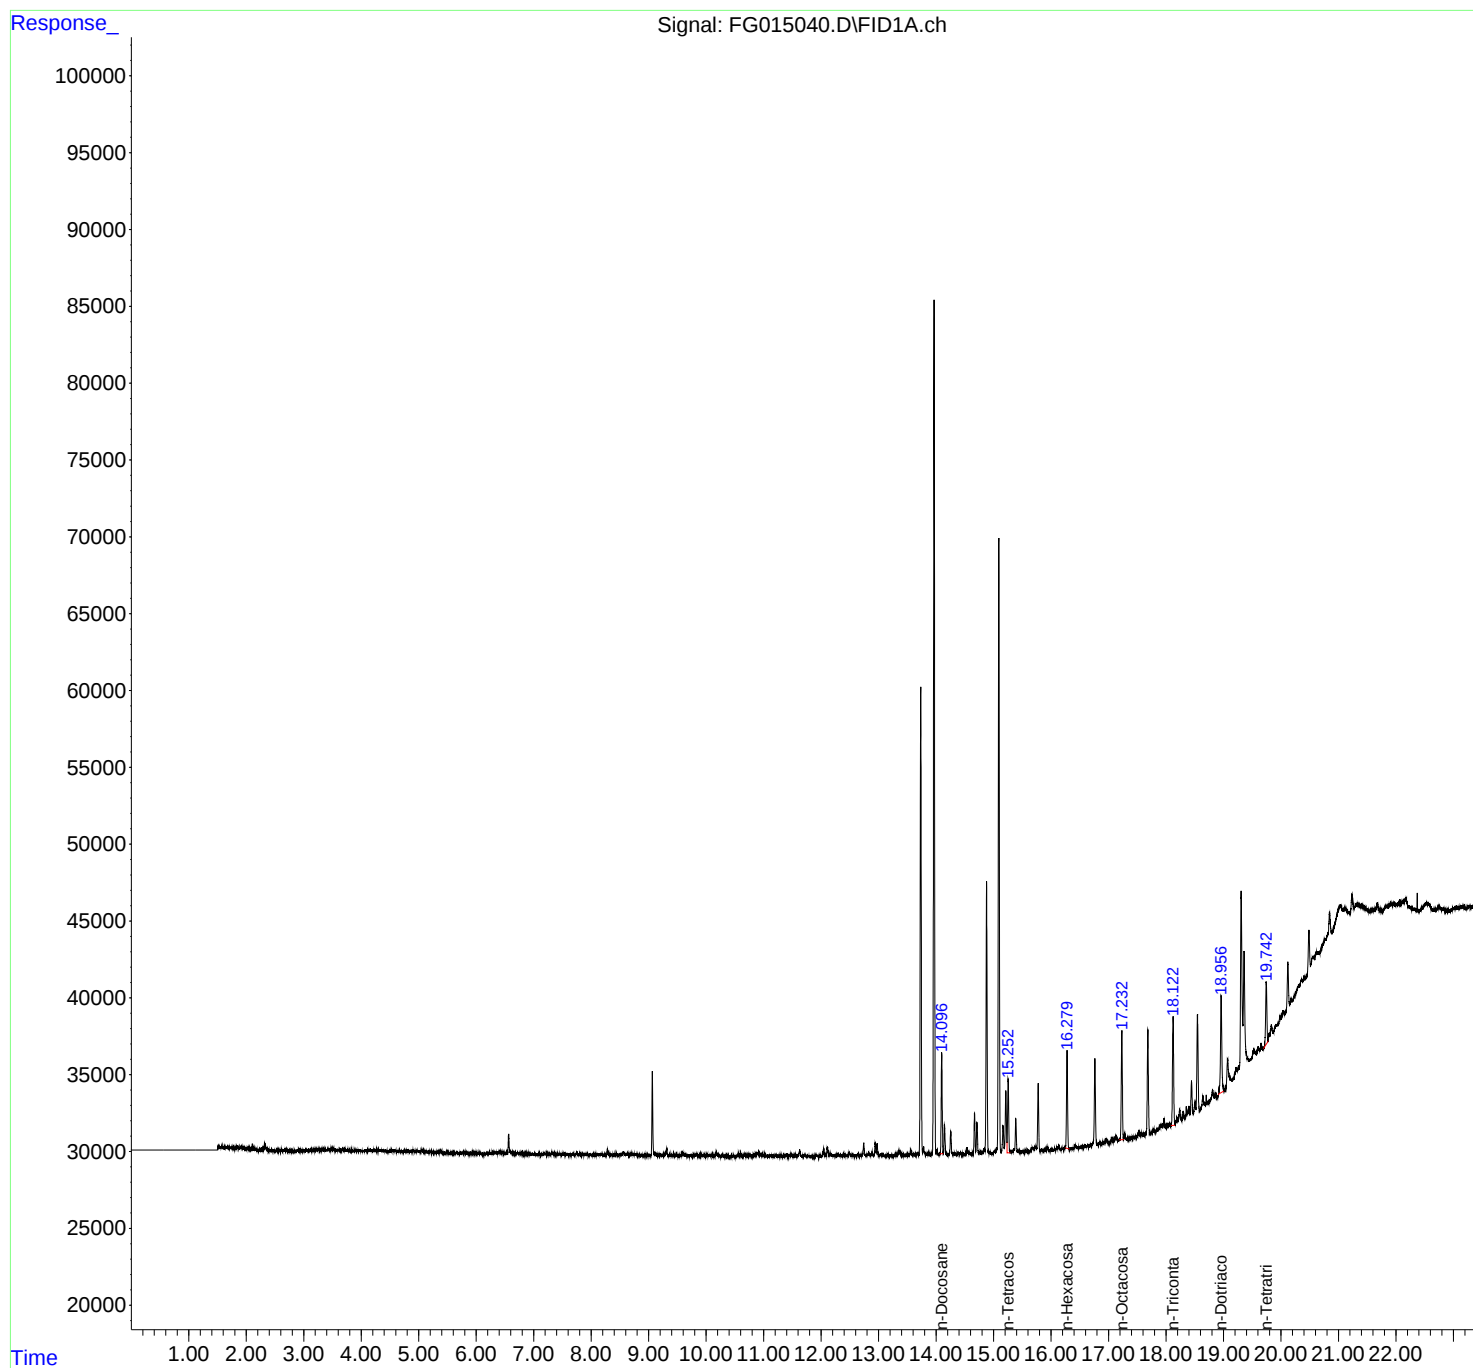


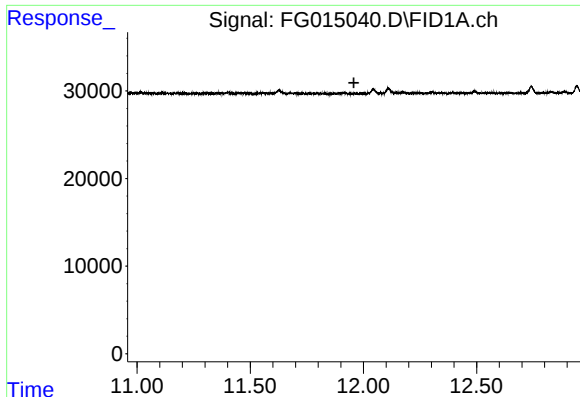

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.958 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

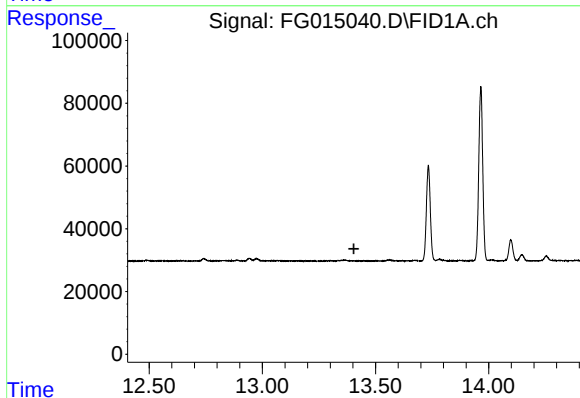


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.404 min
Response: 0
Conc: N.D.

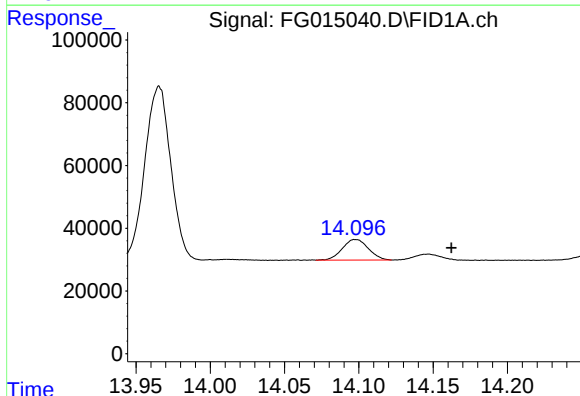


#13 n-Docosane (C22)

R.T.: 14.098 min
Delta R.T.: -0.064 min
Response: 79731
Conc: 0.55 ug/ml

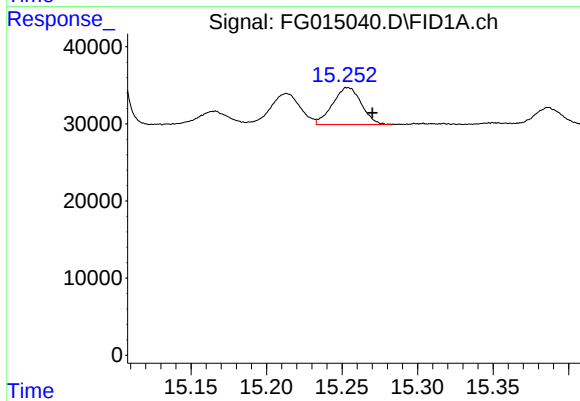

#14 n-Tetracosane (C24)


R.T.: 15.254 min
Delta R.T.: -0.016 min
Response: 63650
Conc: 0.43 ug/ml

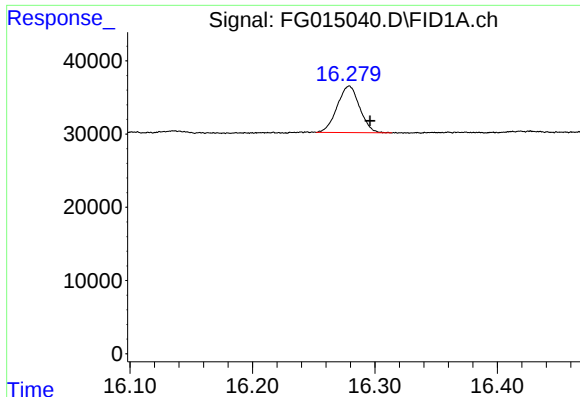

#15 n-Hexacosane (C26)


R.T.: 16.279 min
Delta R.T.: -0.017 min
Response: 81092
Conc: 0.54 ug/ml

Instrument :
FID_G
ClientSampleId :

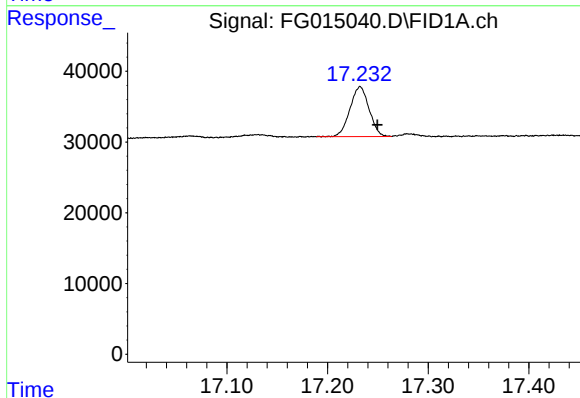


#16 n-Octacosane (C28)

R.T.: 17.232 min
Delta R.T.: -0.017 min
Response: 93093
Conc: 0.62 ug/ml

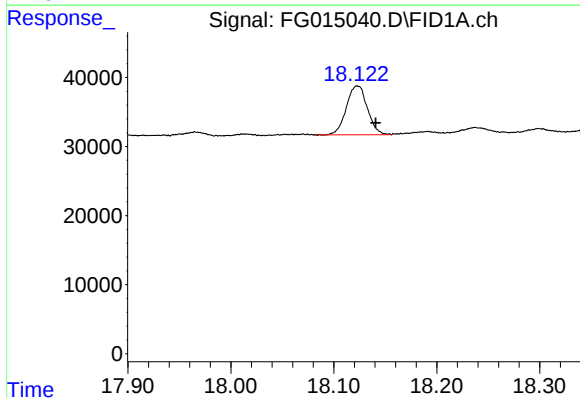


#17 n-Tricontane (C30)

R.T.: 18.123 min
Delta R.T.: -0.018 min
Response: 100029
Conc: 0.65 ug/ml

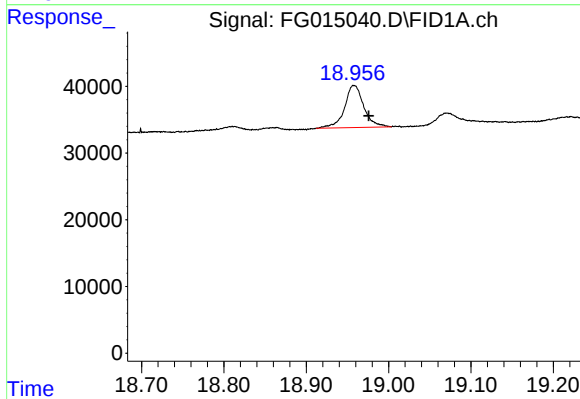

#18 n-Dotriacontane (C32)

R.T.: 18.958 min
Delta R.T.: -0.018 min
Response: 101833
Conc: 0.69 ug/ml

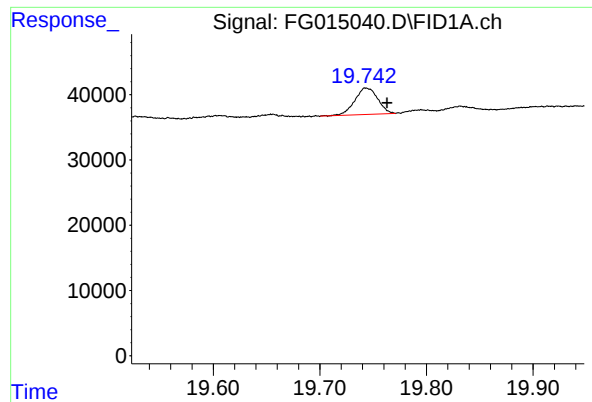

#19 n-Tetratriacontane (C34)

R.T.: 19.743 min
Delta R.T.: -0.020 min
Response: 60316
Conc: 0.47 ug/ml

Instrument :

FID_G

ClientSampleId :