

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG123124AL\
Data File : FG015043.D
Signal(s) : FID1A.ch
Acq On : 31 Dec 2024 10:33
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 01 01:06:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 122024.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 13:49:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
13) T	n-Docosane (C22)	14.099f	75542	0.517 ug/ml
14) T	n-Tetracosane (C24)	15.254	57050	0.382 ug/ml
15) T	n-Hexacosane (C26)	16.278	74289	0.495 ug/ml
16) T	n-Octacosane (C28)	17.232	85438	0.571 ug/ml
17) T	n-Tricontane (C30)	18.122	90555	0.590 ug/ml
18) T	n-Dotriacontane (C32)	18.957	97092	0.658 ug/ml
19) T	n-Tetratriacontane (C34)	19.743	56723	0.444 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG123124AL\
Data File : FG015043.D
Signal(s) : FID1A.ch
Acq On : 31 Dec 2024 10:33
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 01 01:06:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 122024.M
Quant Title : GC Extractables
QLast Update : Fri Dec 20 13:49:57 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

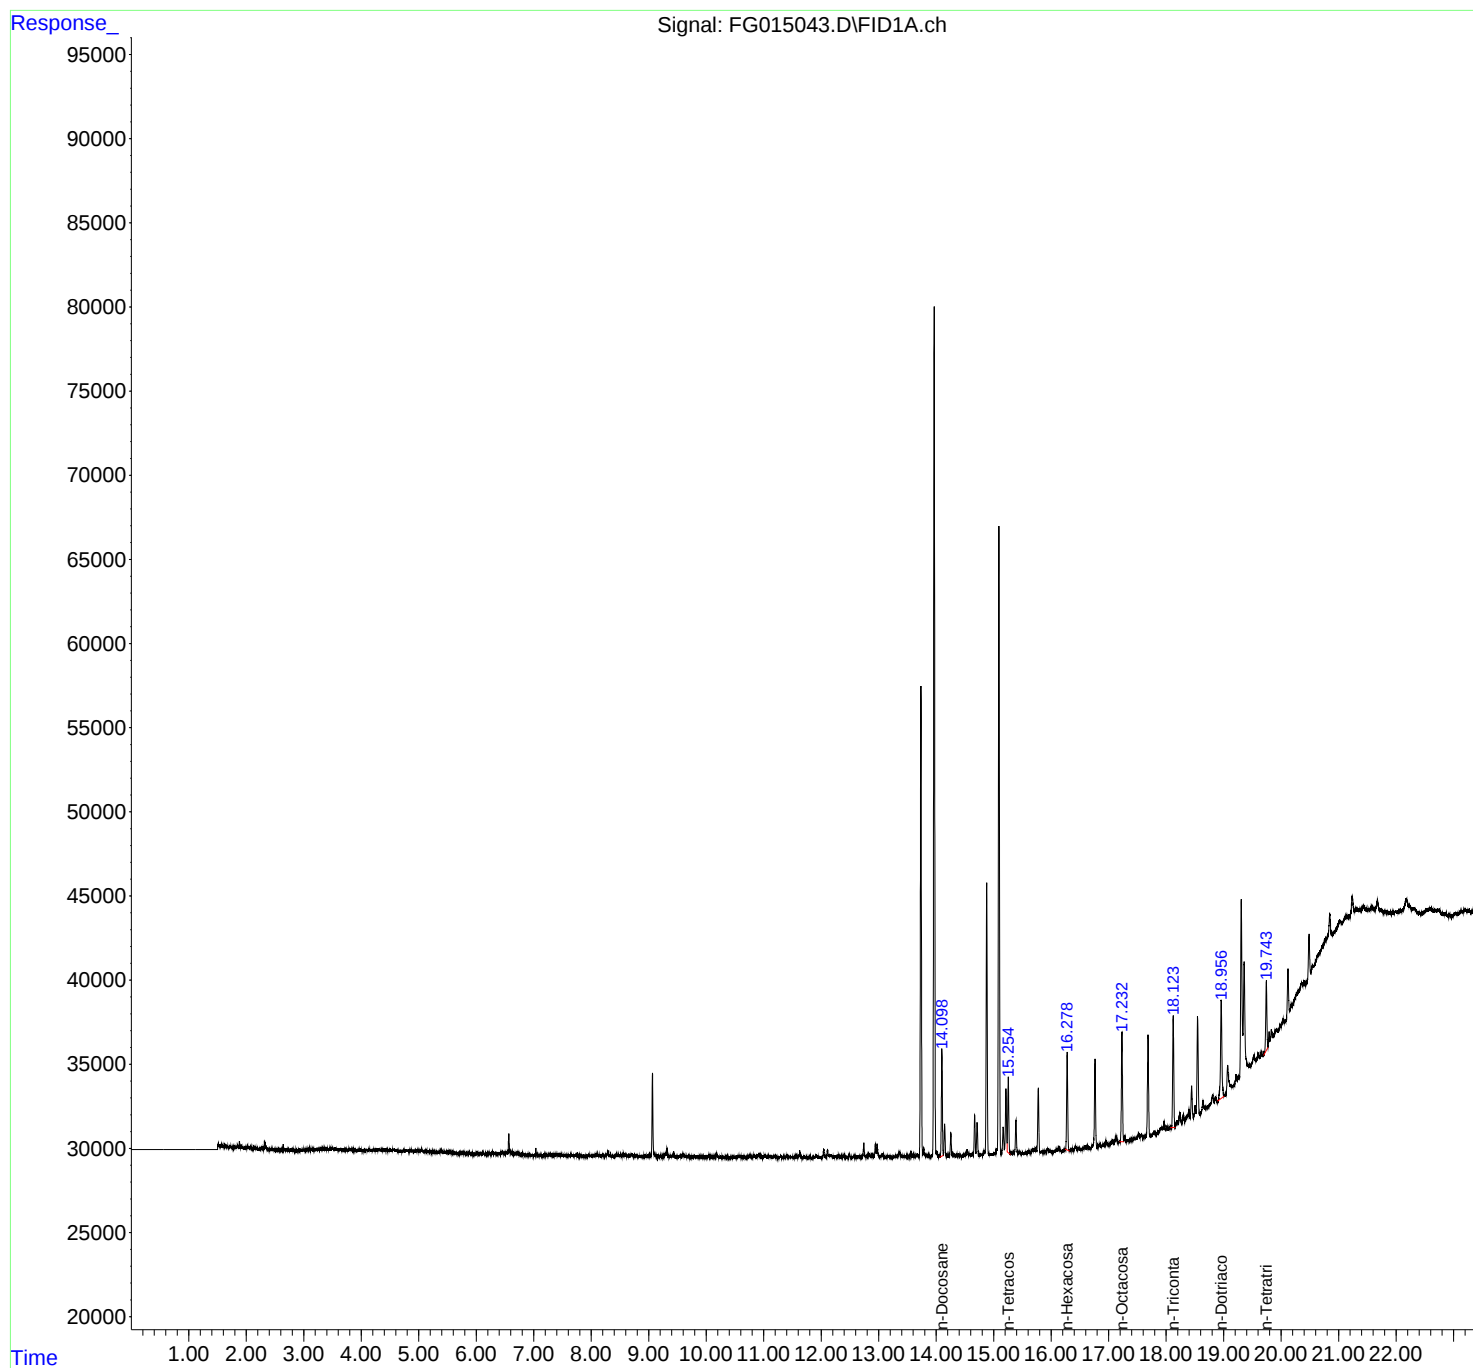


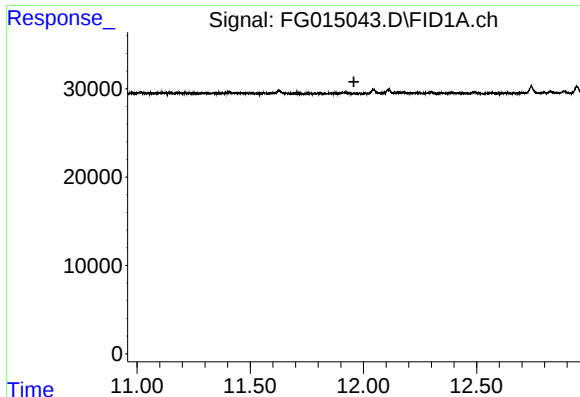

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 11.958 min
Response: 0
Conc: N.D.

Instrument :
FID_G
ClientSampleId :

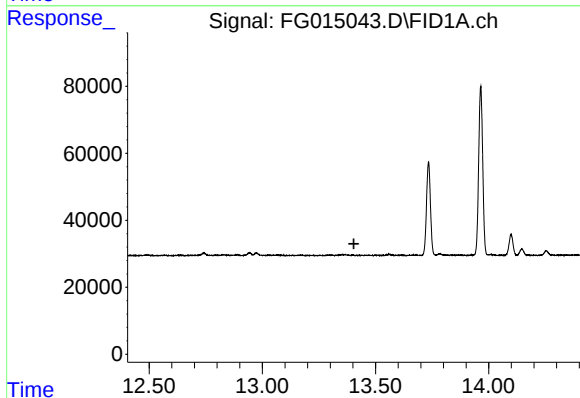


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 13.404 min
Response: 0
Conc: N.D.

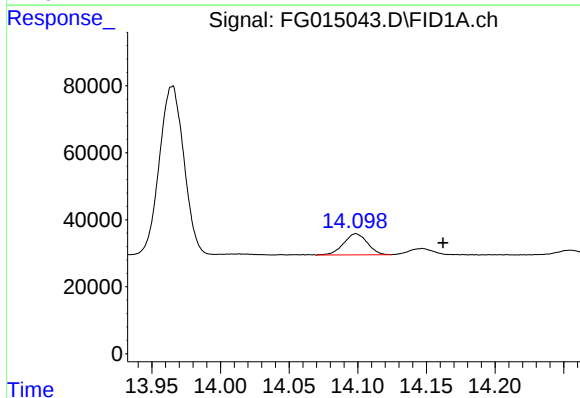


#13 n-Docosane (C22)

R.T.: 14.099 min
Delta R.T.: -0.064 min
Response: 75542
Conc: 0.52 ug/ml

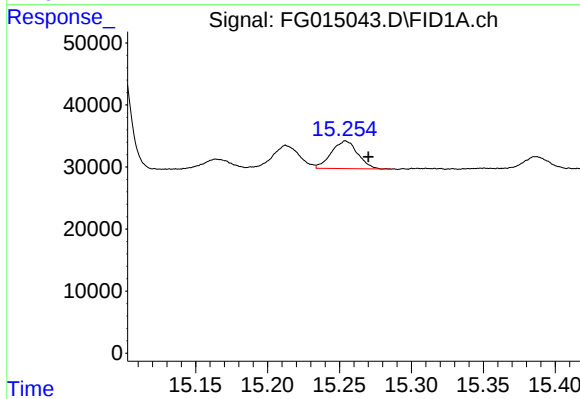

#14 n-Tetracosane (C24)


R.T.: 15.254 min
Delta R.T.: -0.016 min
Response: 57050
Conc: 0.38 ug/ml

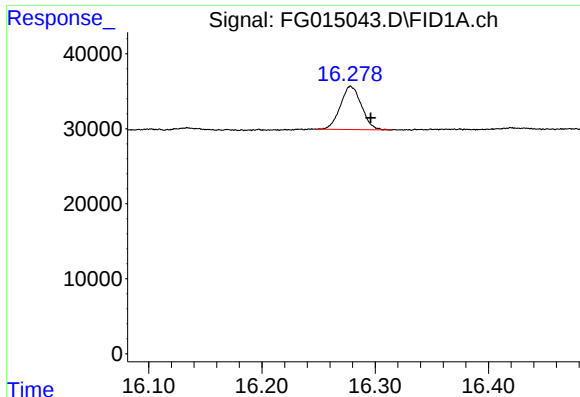

#15 n-Hexacosane (C26)


R.T.: 16.278 min
Delta R.T.: -0.018 min
Response: 74289
Conc: 0.50 ug/ml

Instrument :
FID_G
ClientSampleId :

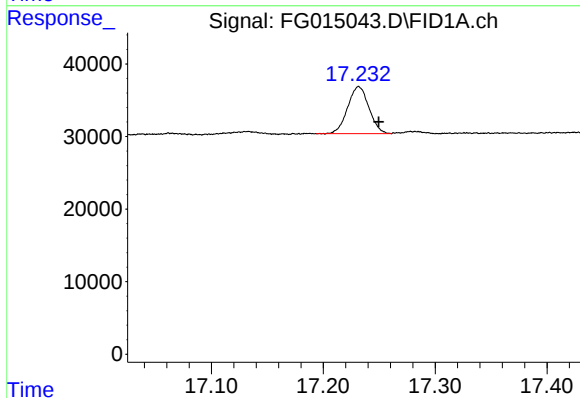


#16 n-Octacosane (C28)

R.T.: 17.232 min
Delta R.T.: -0.018 min
Response: 85438
Conc: 0.57 ug/ml

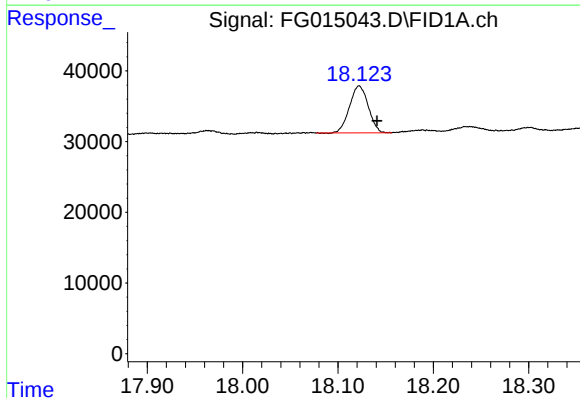


#17 n-Tricontane (C30)

R.T.: 18.122 min
Delta R.T.: -0.018 min
Response: 90555
Conc: 0.59 ug/ml

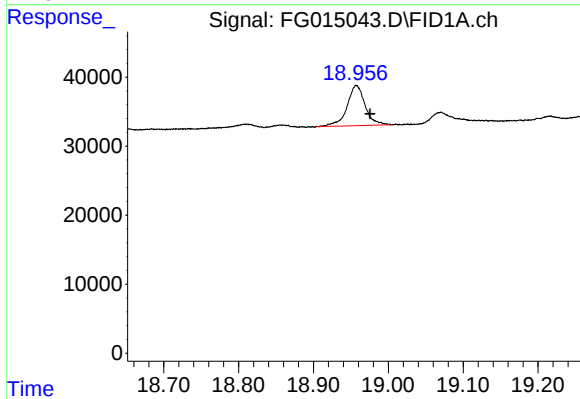

#18 n-Dotriacontane (C32)

R.T.: 18.957 min
Delta R.T.: -0.019 min
Response: 97092
Conc: 0.66 ug/ml

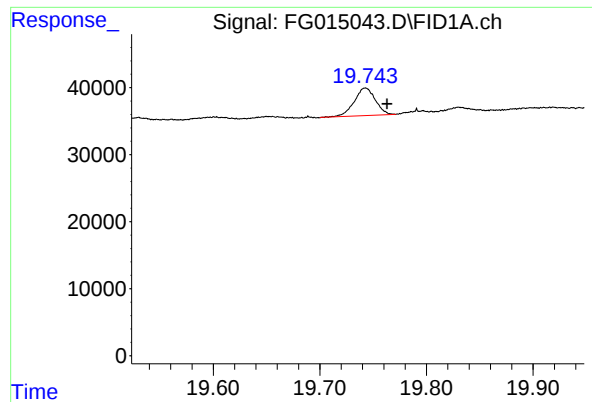

#19 n-Tetratriacontane (C34)

R.T.: 19.743 min
Delta R.T.: -0.020 min
Response: 56723
Conc: 0.44 ug/ml

Instrument :

FID_G

ClientSampleId :