

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121319\
Data File : FG006356.D
Signal(s) : FID1A.ch
Acq On : 13 Dec 2019 16:44
Operator : DD\AJ
Sample : K6204-13RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
K072-AB-WC-1RE

Integration File: autoint1.e
Quant Time: Dec 13 17:00:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112619.M
Quant Title :
QLast Update : Wed Nov 27 02:46:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.497	2695310	34.336 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG121319\
Data File : FG006356.D
Signal(s) : FID1A.ch
Acq On : 13 Dec 2019 16:44
Operator : DD\AJ
Sample : K6204-13RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :
K072-AB-WC-1RE

Integration File: autoint1.e
Quant Time: Dec 13 17:00:51 2019
Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG112619.M
Quant Title :
QLast Update : Wed Nov 27 02:46:06 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

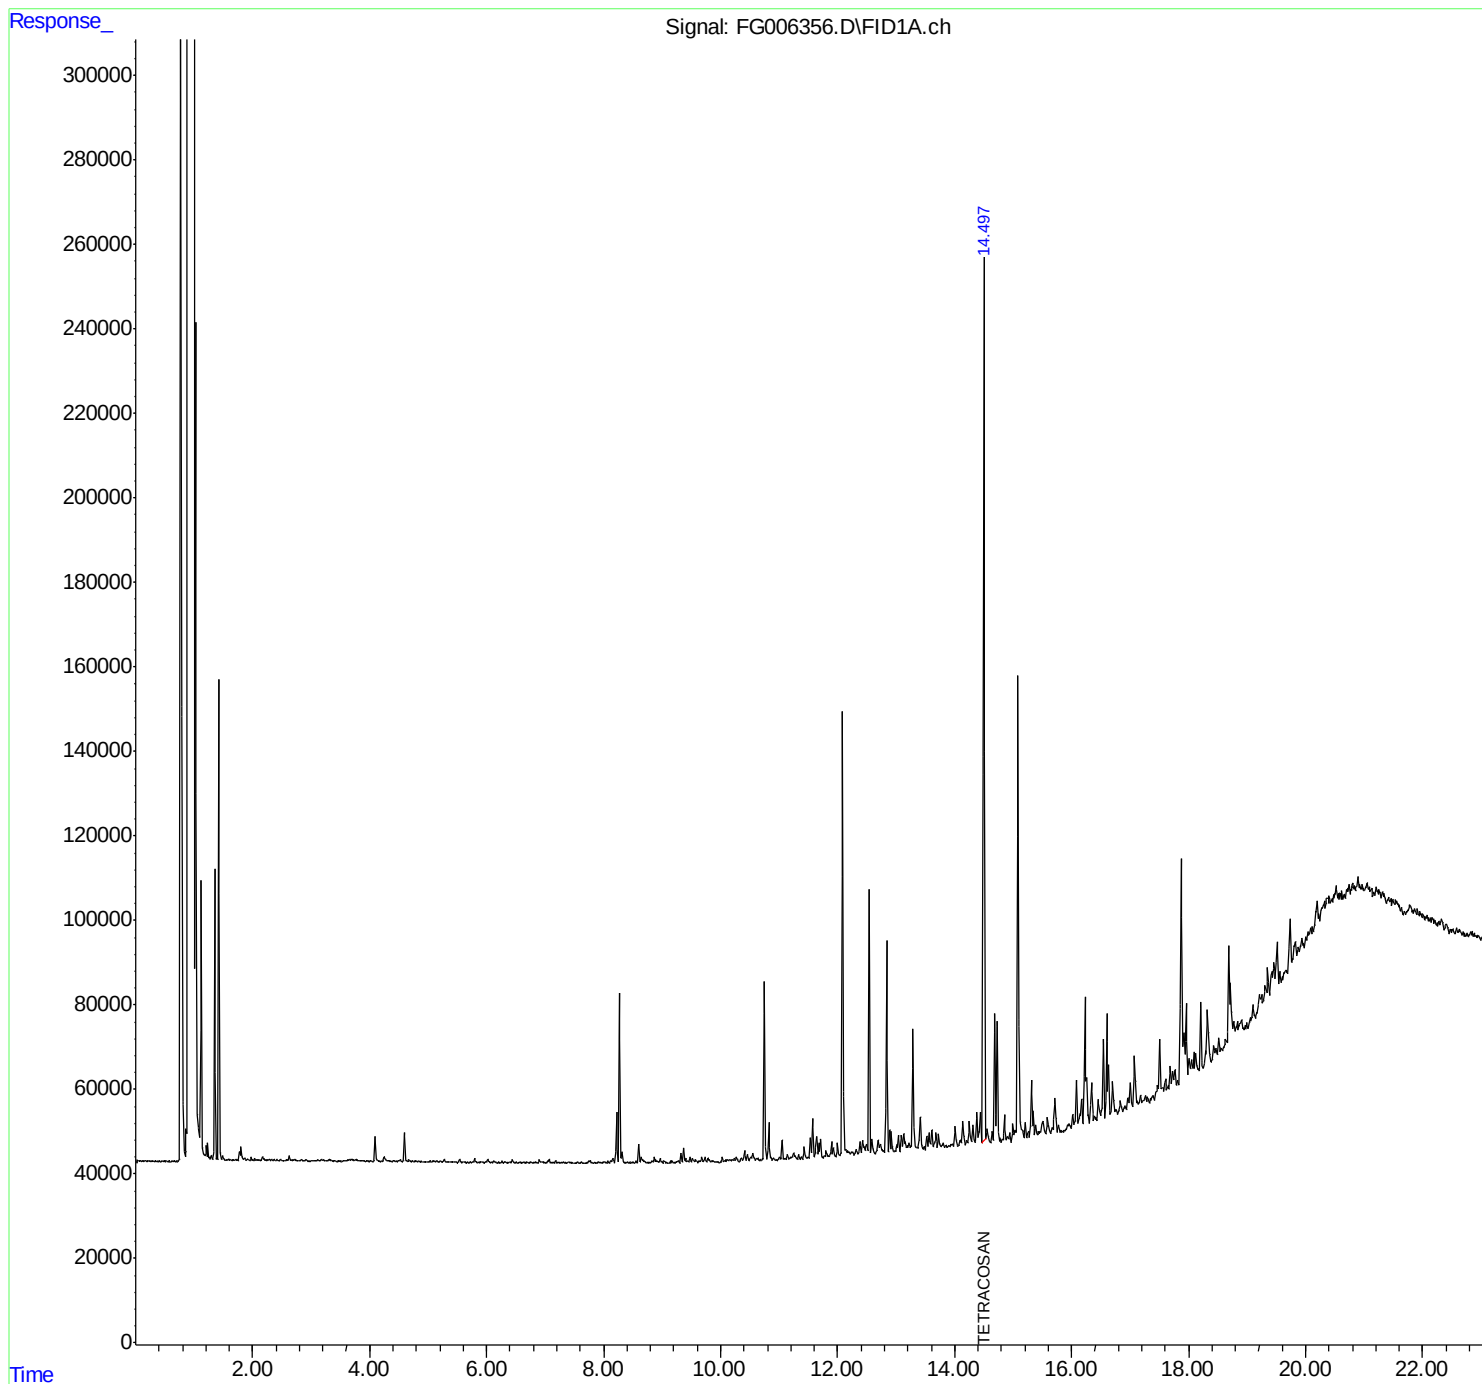

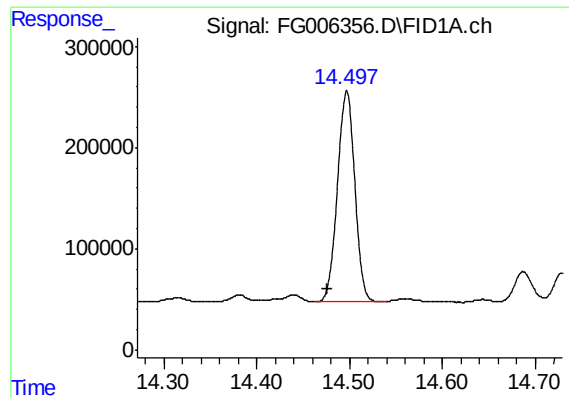

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.497 min
Delta R.T.: 0.020 min
Response: 2695310
Conc: 34.34 ug/ml

Instrument :
FID_G
ClientSampleId :
K072-AB-WC-1RE