

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072018\
Data File : FG001740.D
Signal(s) : FID1A.ch
Acq On : 20 Jul 2018 19:19
Operator : AJ\SJ
Sample : J3762-09
Misc : FID_G MDL WATER 1 PPB
ALS Vial : 7 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 20 22:52:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.509	2950877	25.363 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.569	226860	1.741 ug/ml
14) N-DOTRIACONTANE	18.402	260060	2.043 ug/ml
15) N-TETRATRIACONTANE	19.188	194370	1.544 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG072018\
Data File : FG001740.D
Signal(s) : FID1A.ch
Acq On : 20 Jul 2018 19:19
Operator : AJ\SJ
Sample : J3762-09
Misc : FID_G MDL WATER 1 PPB
ALS Vial : 7 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 20 22:52:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG070218.M
Quant Title :
QLast Update : Mon Jul 02 14:11:21 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

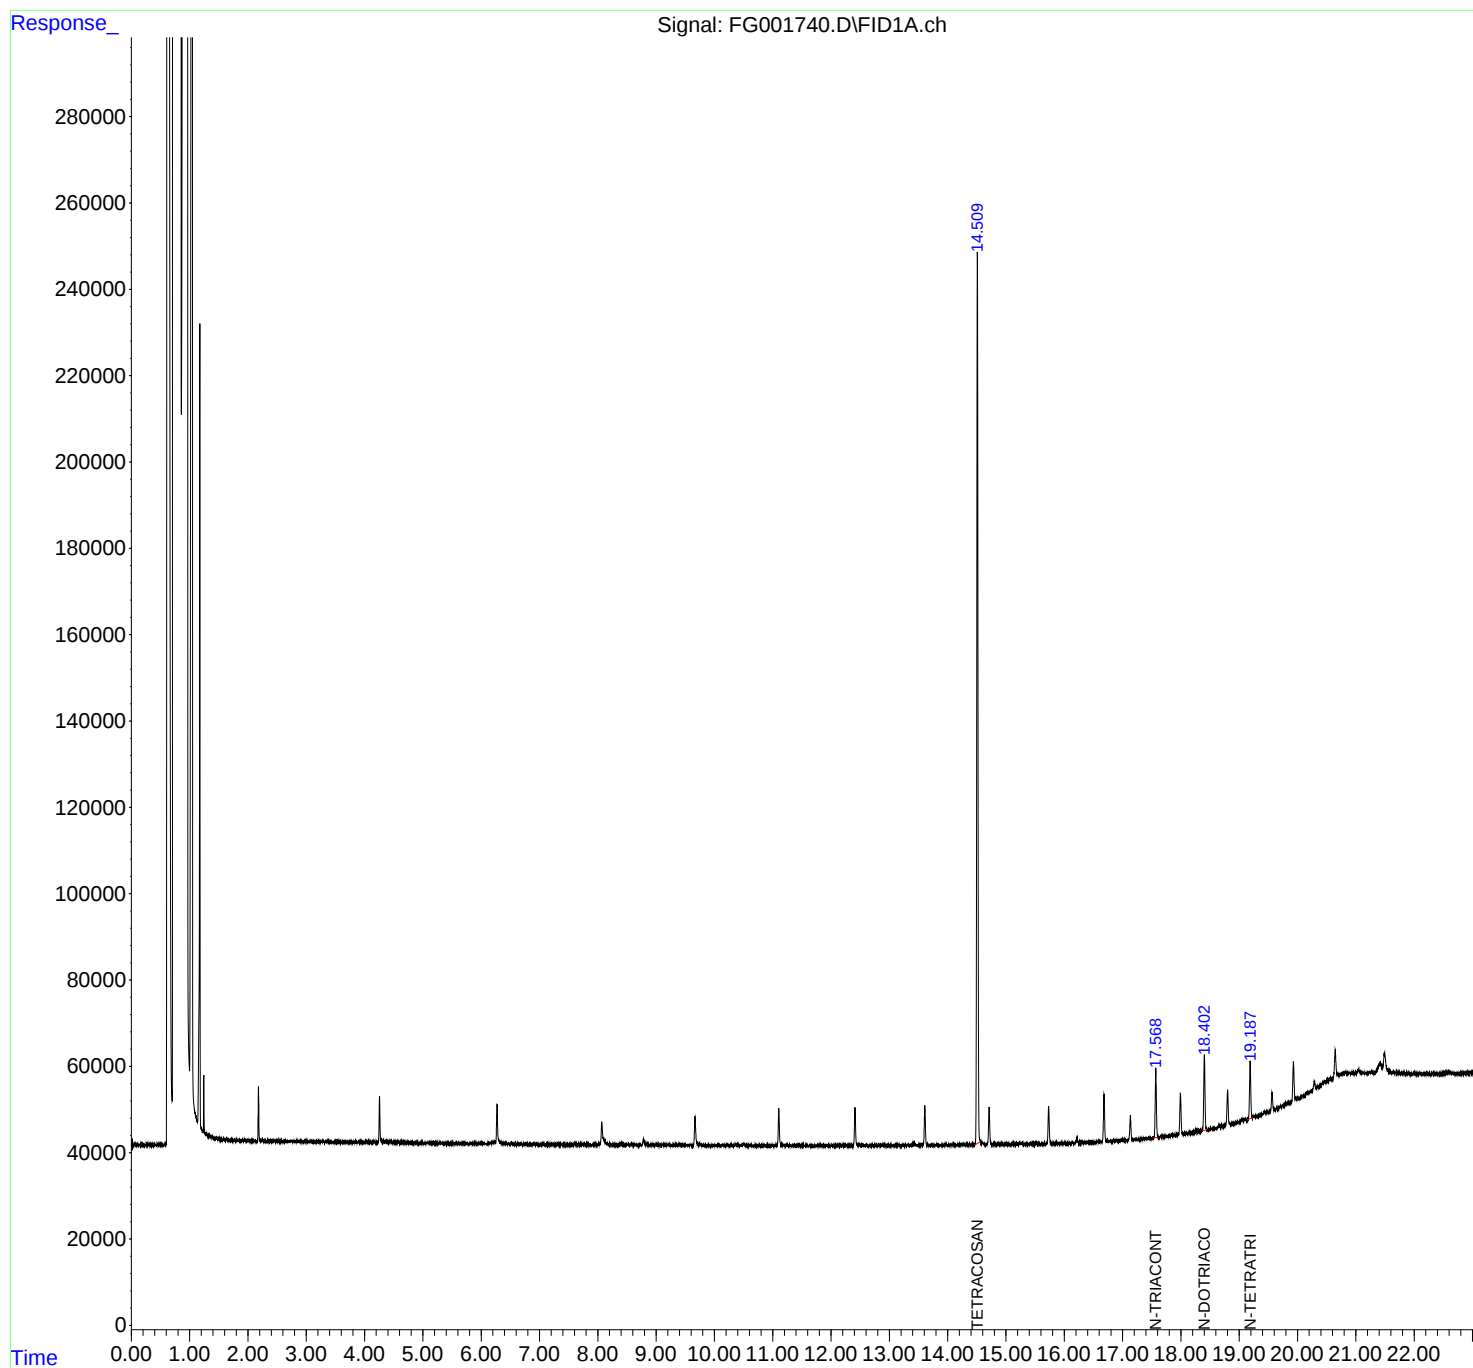

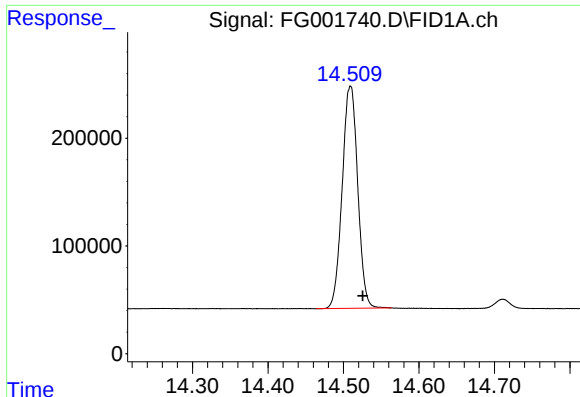


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.509 min
Delta R.T.: -0.016 min
Response: 2950877
Conc: 25.36 ug/ml

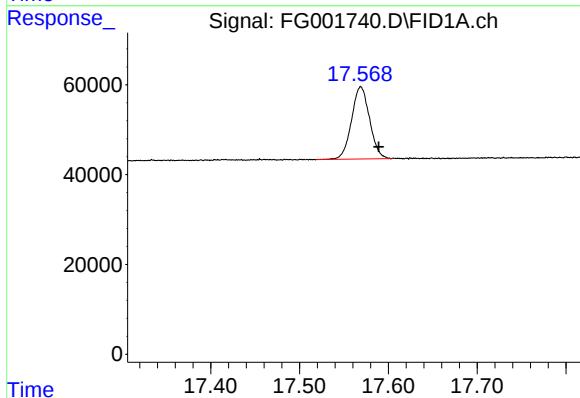


#13 N-TRIACONTANE

R.T.: 17.569 min
Delta R.T.: -0.020 min
Response: 226860
Conc: 1.74 ug/ml

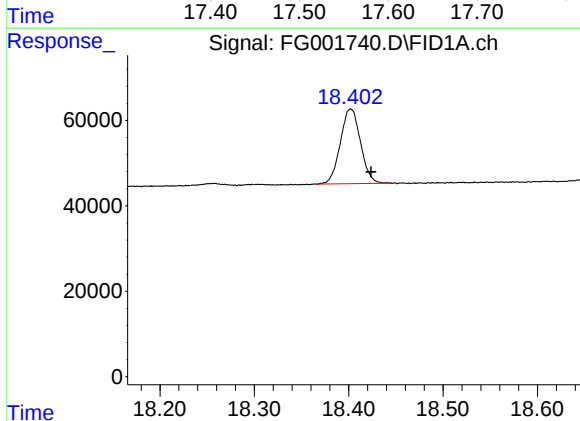

#14 N-DOTRIACONTANE

R.T.: 18.402 min
Delta R.T.: -0.022 min
Response: 260060
Conc: 2.04 ug/ml

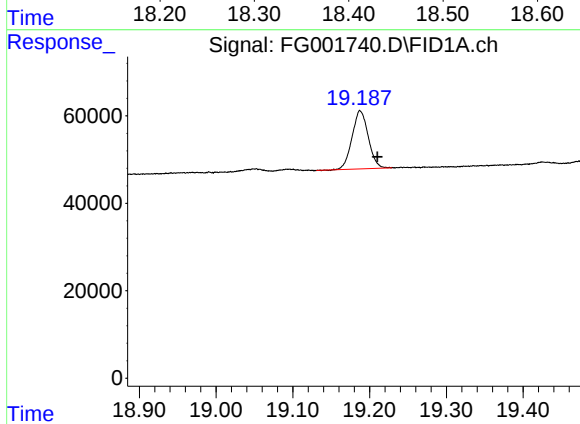

#15 N-TETRATRIACONTANE

R.T.: 19.188 min
Delta R.T.: -0.023 min
Response: 194370
Conc: 1.54 ug/ml