

Data Path : P:\HPCHEM1\FID_G\Data\FG030818\
 Data File : FG000298.D
 Signal(s) : FID1A.ch
 Acq On : 08 Mar 2018 17:59
 Operator : UA\AJ
 Sample : J1819-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 09 05:46:03 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FG022818.M
 Quant Title :
 QLast Update : Wed Feb 28 18:10:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.580	4188943	37.687 ug/ml
Target Compounds			
4) N-TETRADECANE	8.123	325237	2.366 ug/ml
5) N-HEXADECANE	9.727	3331209	25.171 ug/ml
6) N-OCTADECANE	11.171	2621410	19.792 ug/ml
7) N-EICOSANE	12.479	1286793	10.012 ug/ml
8) N-DOCOSANE	13.692	2537404	20.672 ug/ml
10) N-TETRACOSANE	14.754	6264897	51.195 ug/ml
11) N-HEXACOSANE	15.808	5064414	41.969 ug/ml
12) N-OCTACOSANE	16.756	11105562	93.594 ug/ml
13) N-TRIACONTANE	17.645	4971586	43.102 ug/ml
14) N-DOTRIACONTANE	18.410	2393597	23.960 ug/ml
15) N-TETRATRIACONTANE	19.269	381526	5.736 ug/ml
16) N-HEXATRIACONTANE	20.000	124824	3.526 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_G\Data\FG030818\
Data File : FG000298.D
Signal(s) : FID1A.ch
Acq On : 08 Mar 2018 17:59
Operator : UA\AJ
Sample : J1819-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 09 05:46:03 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FG022818.M
Quant Title :
QLast Update : Wed Feb 28 18:10:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

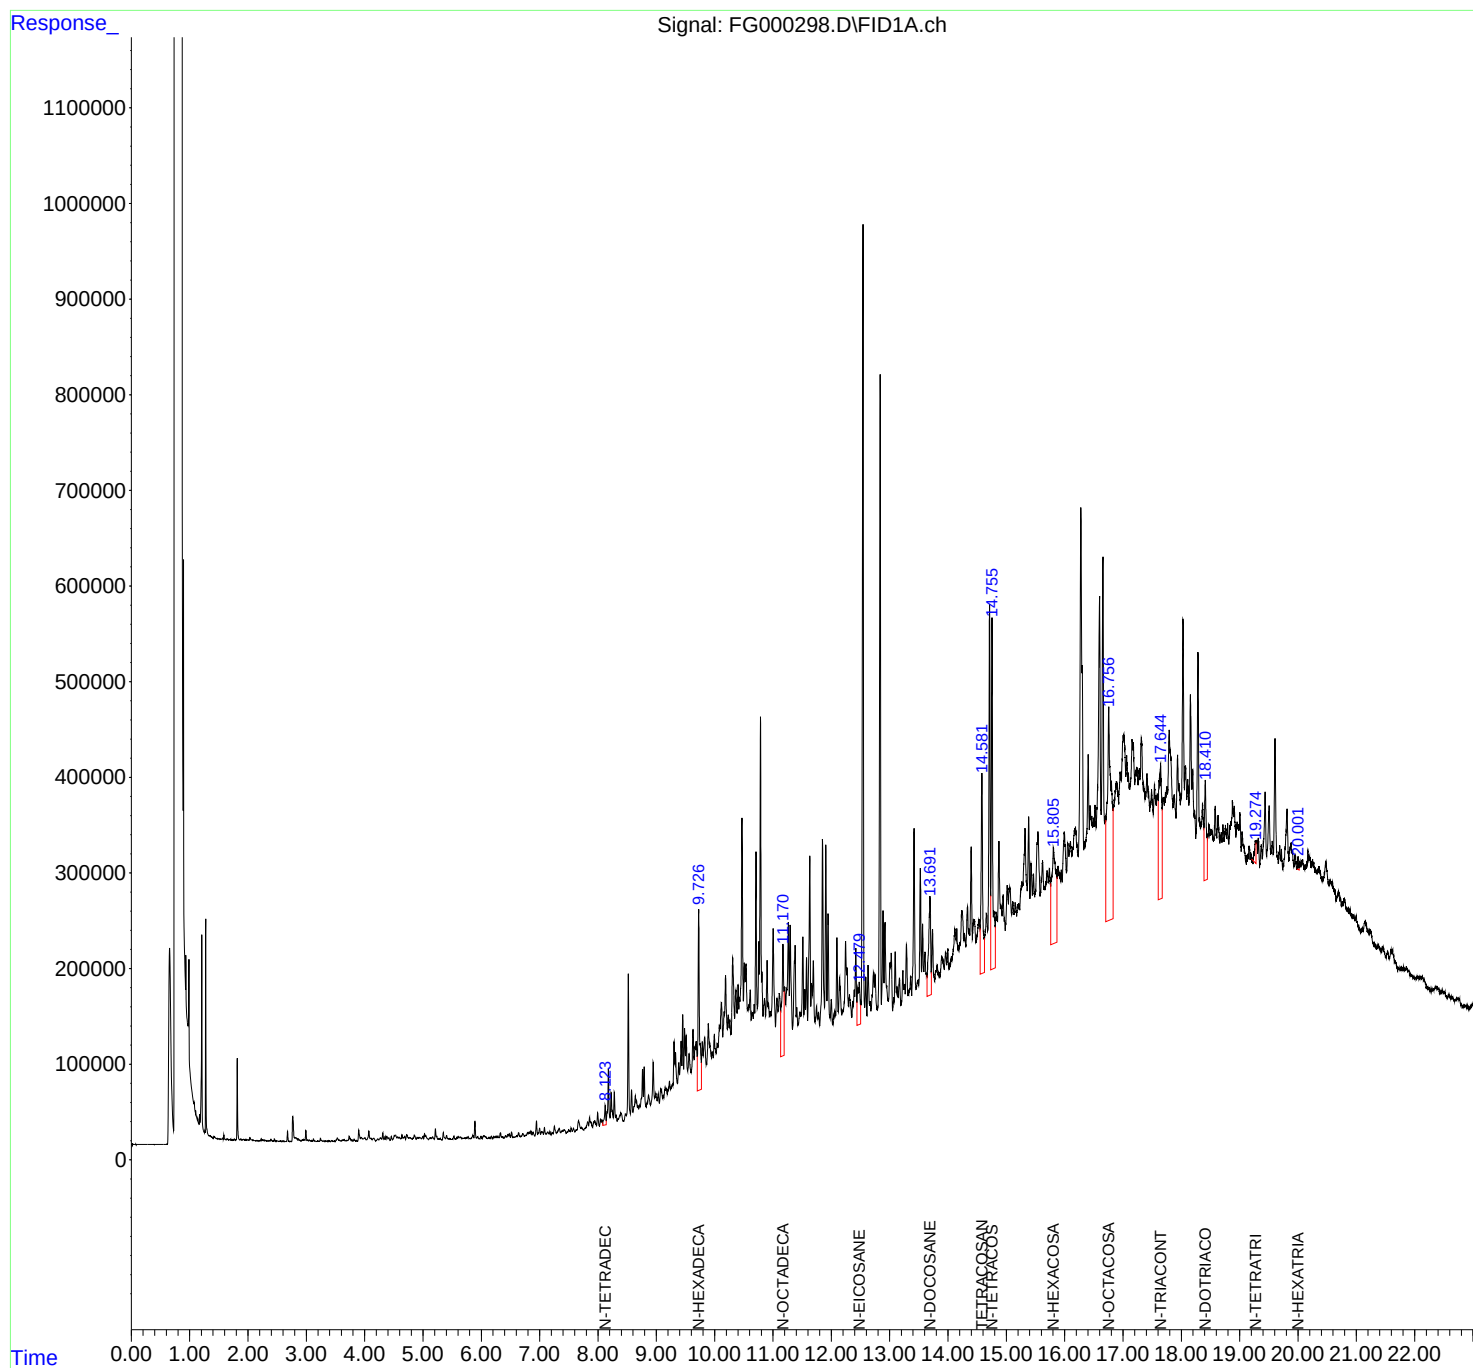


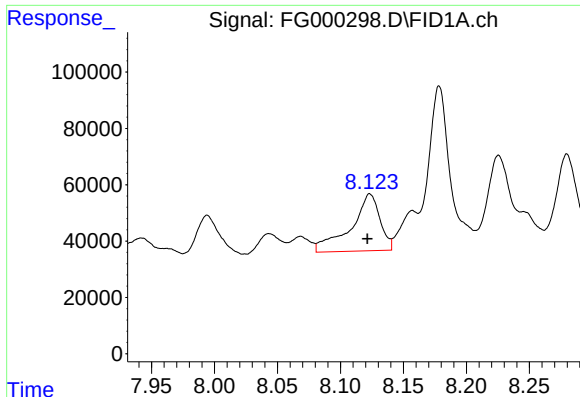

#4 N-TETRADECANE


R.T.: 8.123 min
Delta R.T.: 0.002 min
Response: 325237
Conc: 2.37 ug/ml

Instrument :
FID_G
ClientSampleId :

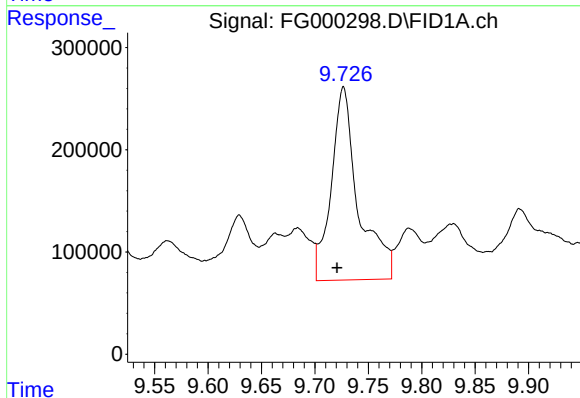


#5 N-HEXADECANE

R.T.: 9.727 min
Delta R.T.: 0.006 min
Response: 3331209
Conc: 25.17 ug/ml

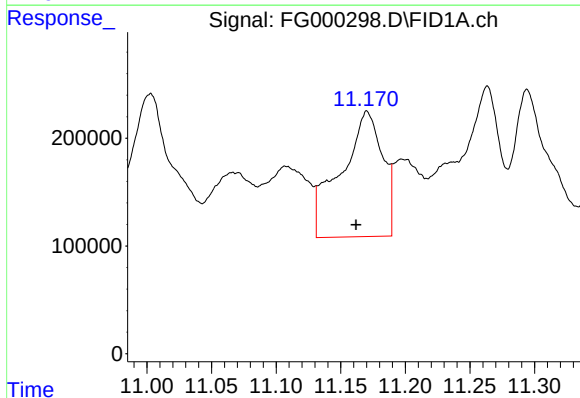


#6 N-OCTADECANE

R.T.: 11.171 min
Delta R.T.: 0.009 min
Response: 2621410
Conc: 19.79 ug/ml

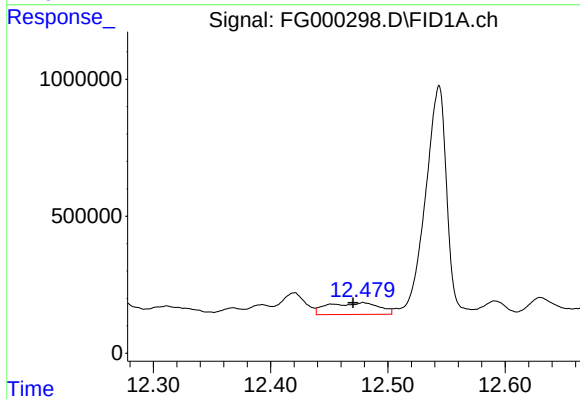

#7 N-EICOSANE


R.T.: 12.479 min
Delta R.T.: 0.009 min
Response: 1286793
Conc: 10.01 ug/ml

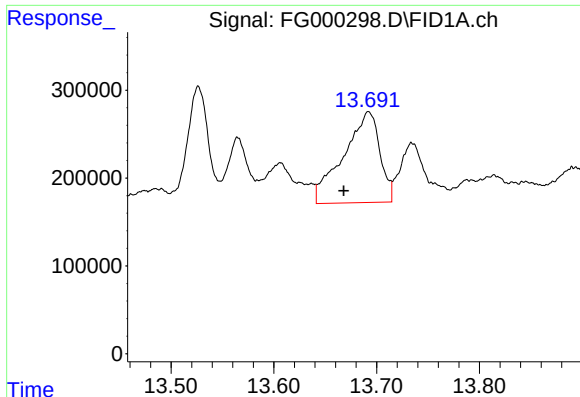

#8 N-DOCOSANE


R.T.: 13.692 min
Delta R.T.: 0.024 min
Response: 2537404
Conc: 20.67 ug/ml

Instrument :
FID_G
ClientSampleId :

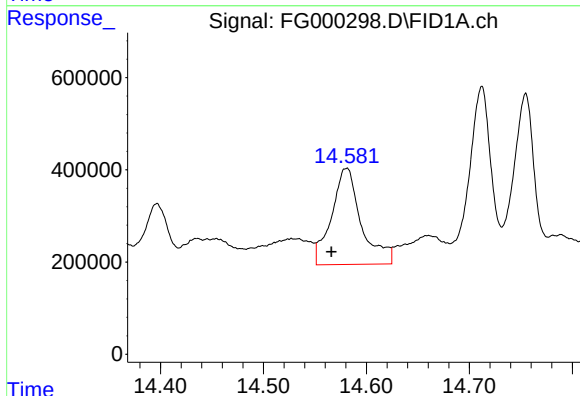


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.580 min
Delta R.T.: 0.015 min
Response: 4188943
Conc: 37.69 ug/ml

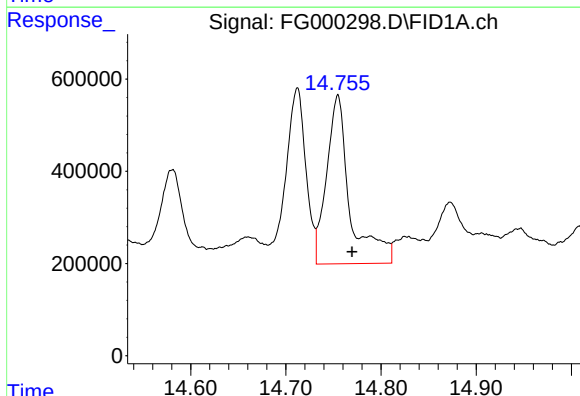


#10 N-TETRACOSANE

R.T.: 14.754 min
Delta R.T.: -0.015 min
Response: 6264897
Conc: 51.19 ug/ml

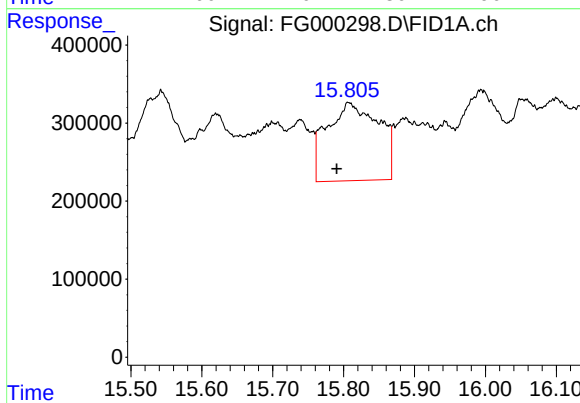

#11 N-HEXACOSANE


R.T.: 15.808 min
Delta R.T.: 0.018 min
Response: 5064414
Conc: 41.97 ug/ml

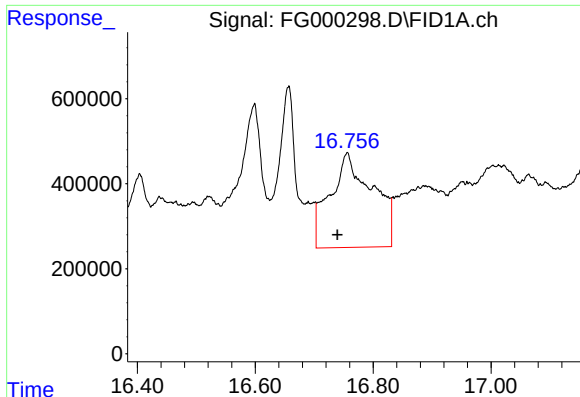

#12 N-OCTACOSANE


R.T.: 16.756 min
Delta R.T.: 0.017 min
Response: 11105562
Conc: 93.59 ug/ml

Instrument :
FID_G
ClientSampleId :

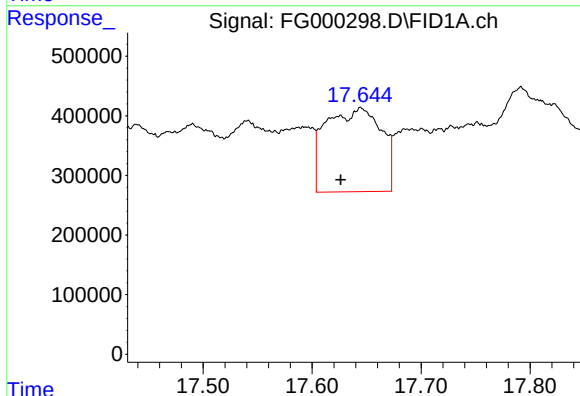


#13 N-TRIACONTANE

R.T.: 17.645 min
Delta R.T.: 0.019 min
Response: 4971586
Conc: 43.10 ug/ml

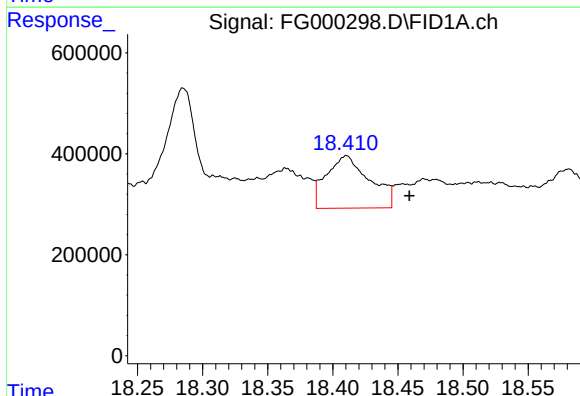


#14 N-DOTRIACONTANE

R.T.: 18.410 min
Delta R.T.: -0.049 min
Response: 2393597
Conc: 23.96 ug/ml

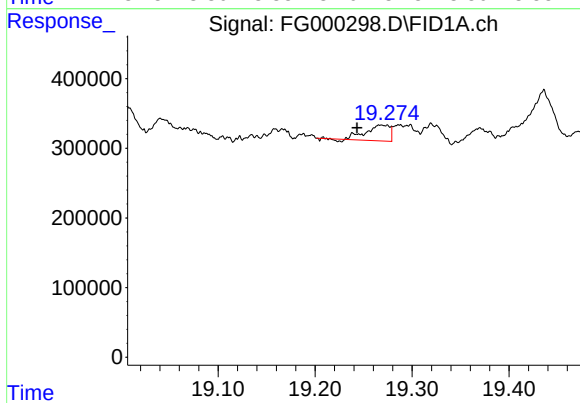

#15 N-TETRATRIACONTANE

R.T.: 19.269 min
Delta R.T.: 0.026 min
Response: 381526
Conc: 5.74 ug/ml

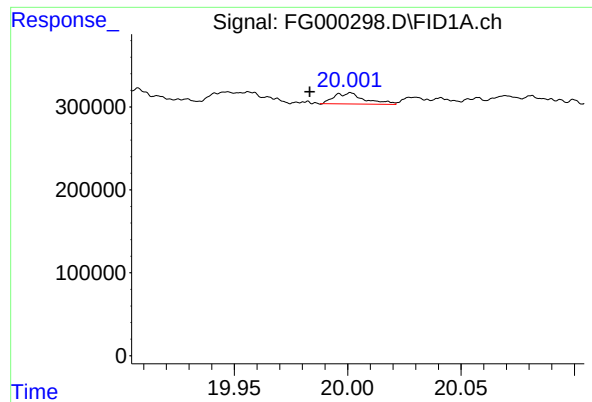

#16 N-HEXATRIACONTANE

R.T.: 20.000 min
Delta R.T.: 0.017 min
Response: 124824
Conc: 3.53 ug/ml

Instrument :
FID_G
ClientSampleId :