

Data Path : P:\HPCHEM1\FID_G\Data\FG030818\
 Data File : FG000301.D
 Signal(s) : FID1A.ch
 Acq On : 08 Mar 2018 19:26
 Operator : UA\AJ
 Sample : J1819-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 09 05:47:01 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FG022818.M
 Quant Title :
 QLast Update : Wed Feb 28 18:10:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.571	2061105	18.543 ug/ml
Target Compounds			
4) N-TETRADECANE	8.177f	332013	2.415 ug/ml
5) N-HEXADECANE	9.721	309366	2.338 ug/ml
13) N-TRIACONTANE	17.634	156321	1.355 ug/ml
14) N-DOTRIACONTANE	18.459	238154	2.384 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_G\Data\FG030818\
Data File : FG000301.D
Signal(s) : FID1A.ch
Acq On : 08 Mar 2018 19:26
Operator : UA\AJ
Sample : J1819-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 09 05:47:01 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FG022818.M
Quant Title :
QLast Update : Wed Feb 28 18:10:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

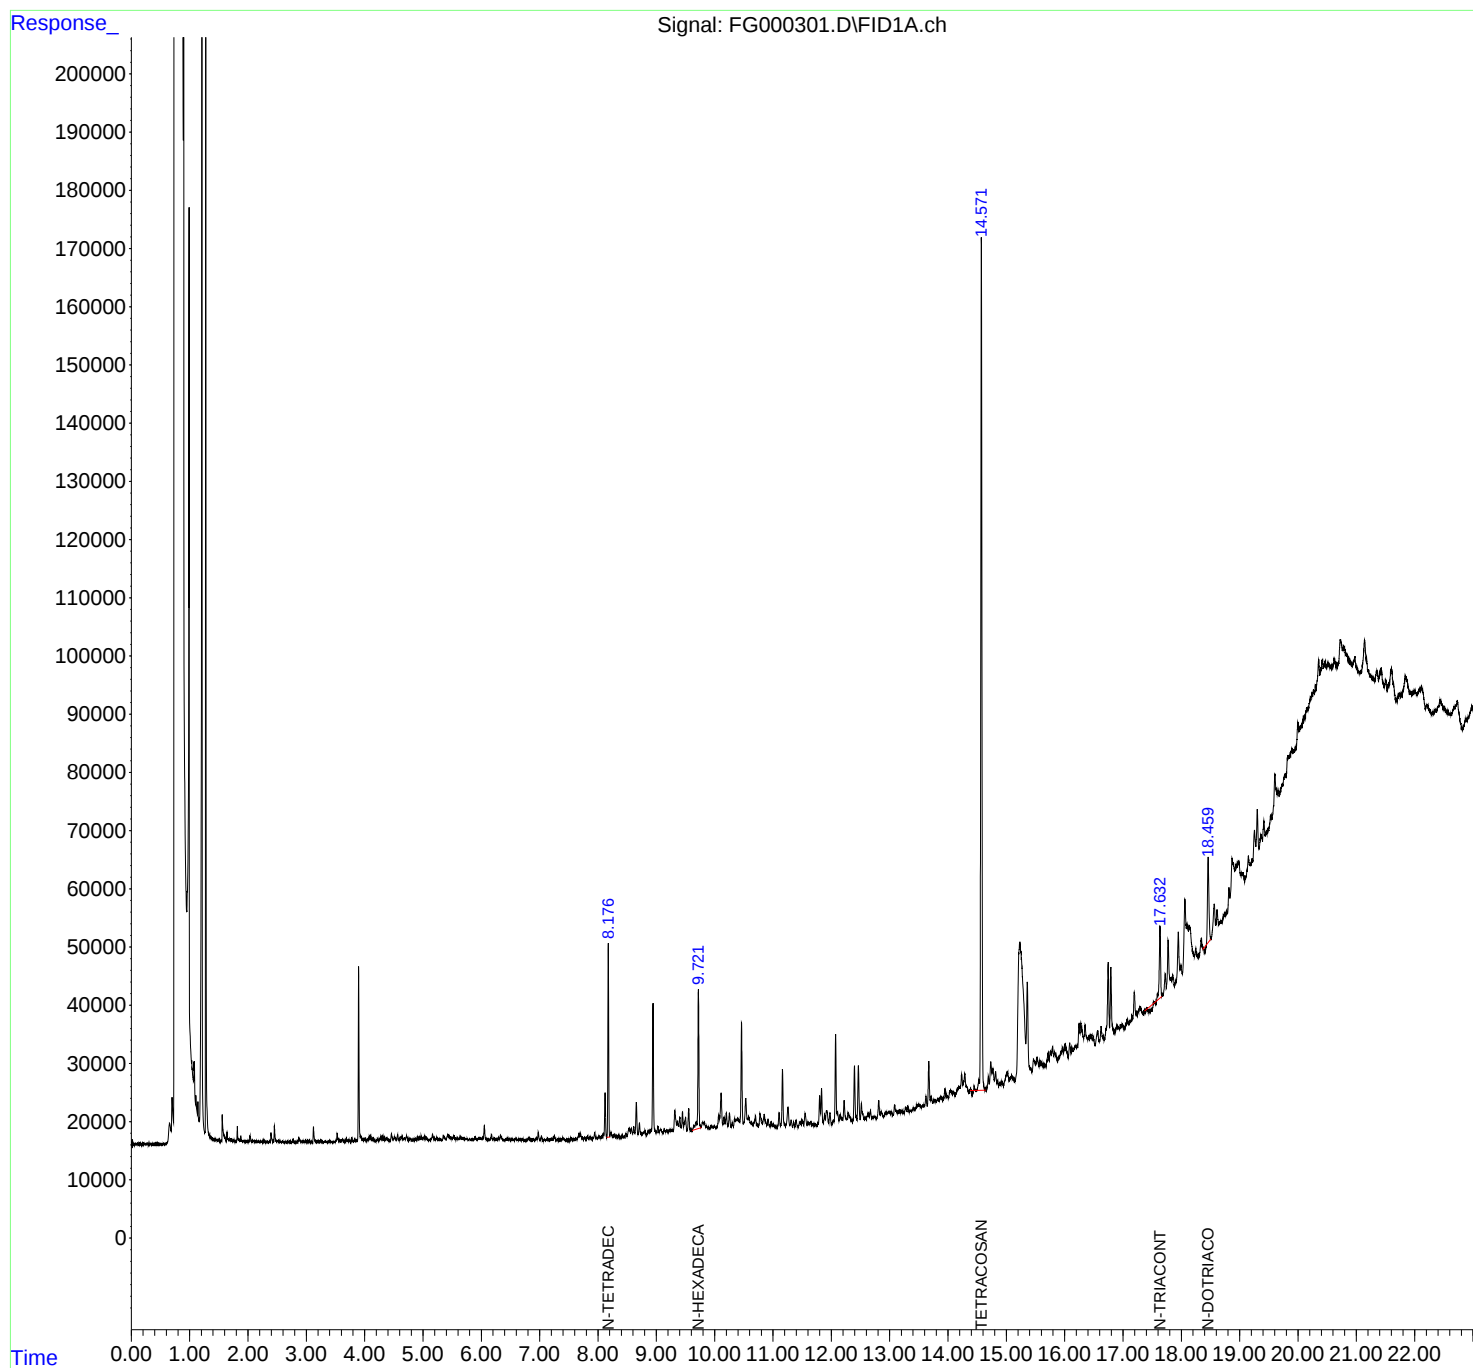


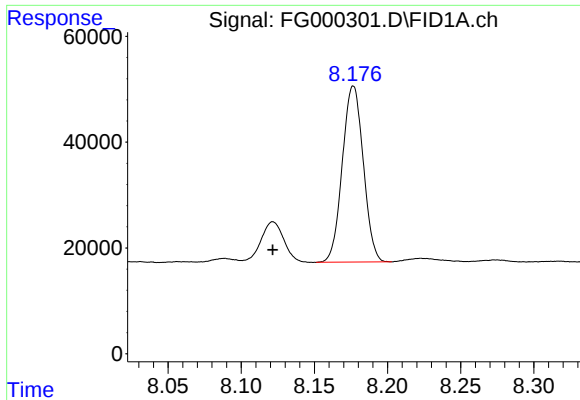

#4 N-TETRADECANE


R.T.: 8.177 min
Delta R.T.: 0.055 min
Response: 332013
Conc: 2.41 ug/ml

Instrument :
FID_G
ClientSampleId :

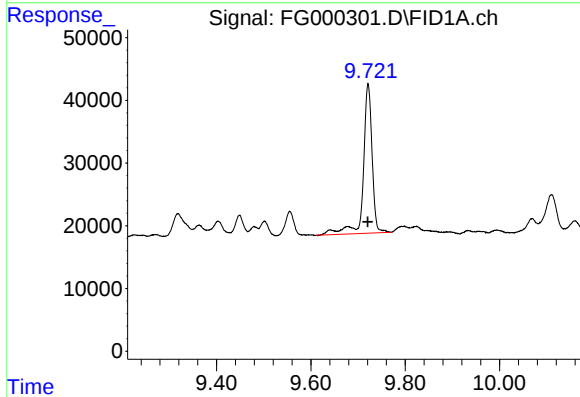


#5 N-HEXADECANE

R.T.: 9.721 min
Delta R.T.: 0.000 min
Response: 309366
Conc: 2.34 ug/ml

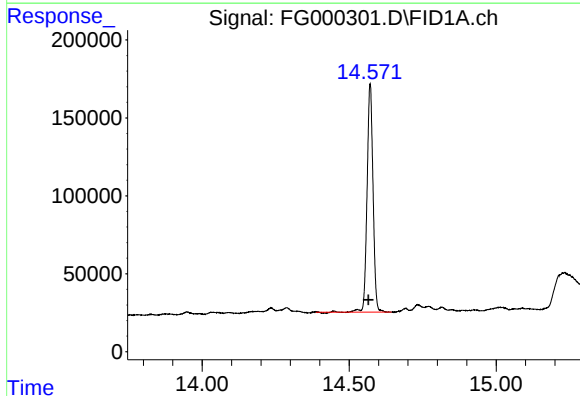


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.571 min
Delta R.T.: 0.005 min
Response: 2061105
Conc: 18.54 ug/ml

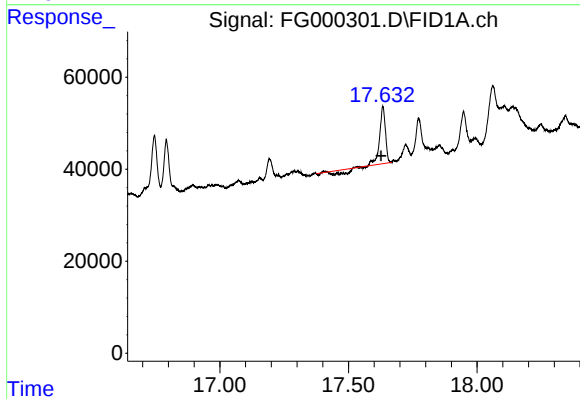

#13 N-TRIACONTANE

R.T.: 17.634 min
Delta R.T.: 0.007 min
Response: 156321
Conc: 1.36 ug/ml

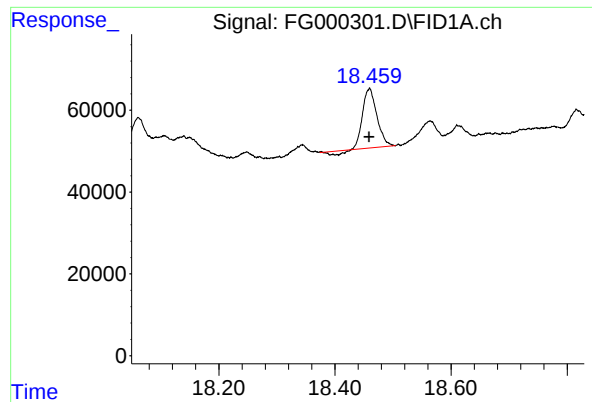

#14 N-DOTRIACONTANE

R.T.: 18.459 min
Delta R.T.: 0.000 min
Response: 238154
Conc: 2.38 ug/ml

Instrument :
FID_G
ClientSampleId :