

Data Path : P:\HPCHEM1\FID_G\Data\FG030818\
 Data File : FG000300.D
 Signal(s) : FID1A.ch
 Acq On : 08 Mar 2018 18:57
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Manual Integrations
 APPROVED

ugo
 3/9/2018 1:58:15 PM

Integration File: Sample.e
 Quant Time: Mar 09 05:46:38 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FG022818.M
 Quant Title :
 QLast Update : Wed Feb 28 18:10:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.574	5324281	47.901 ug/mlm
Target Compounds			
2) N-DECANE	4.312	6529307	46.123 ug/ml
3) N-DODECANE	6.331	6337268	45.274 ug/ml
4) N-TETRADECANE	8.125	6201704	45.110 ug/ml
5) N-HEXADECANE	9.725	6055686	45.757 ug/ml
6) N-OCTADECANE	11.166	6012826	45.399 ug/ml
7) N-EICOSANE	12.476	5911481	45.994 ug/ml
8) N-DOCOSANE	13.674	5919054	48.222 ug/ml
10) N-TETRACOSANE	14.777	5994477	48.985 ug/ml
11) N-HEXACOSANE	15.800	6001877	49.737 ug/ml
12) N-OCTACOSANE	16.749	5988514	50.469 ug/ml

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : P:\HPCHEM1\FID_G\Data\FG030818\
Data File : FG000300.D
Signal(s) : FID1A.ch
Acq On : 08 Mar 2018 18:57
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1


Instrument :
FID_G
ClientSampleId :


Manual Integrations
APPROVED

ugo
3/9/2018 1:58:15 PM

Integration File: Sample.e
Quant Time: Mar 09 05:46:38 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FG022818.M
Quant Title :
QLast Update : Wed Feb 28 18:10:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

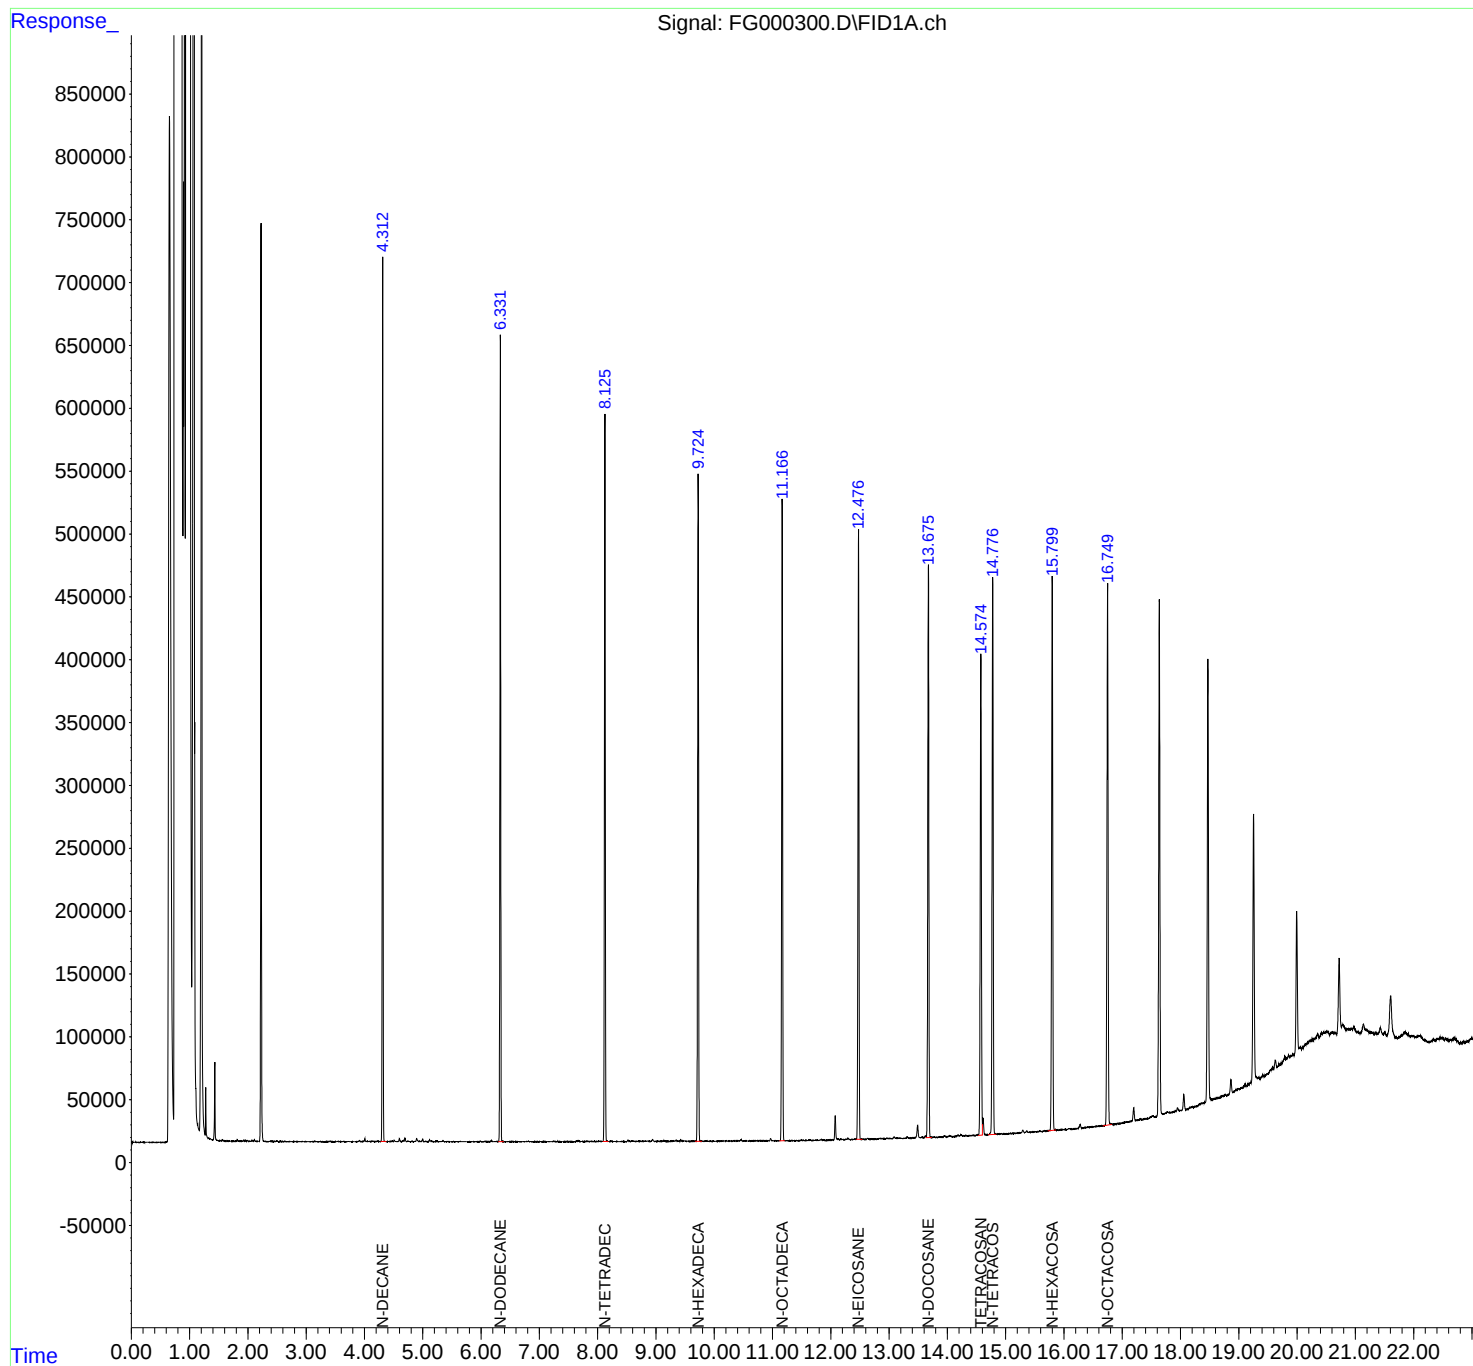

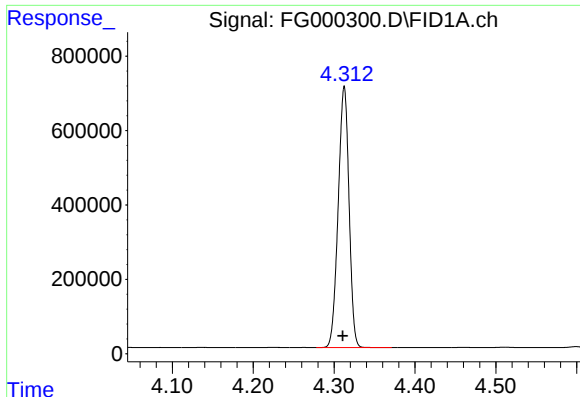


#2 N-DECANE

R.T.: 4.312 min
Delta R.T.: 0.002 min
Response: 6529307
Conc: 46.12 ug/ml

Instrument :
FID_G
ClientSampleId :


Manual Integrations
APPROVED

ugo
3/9/2018 1:58:15 PM

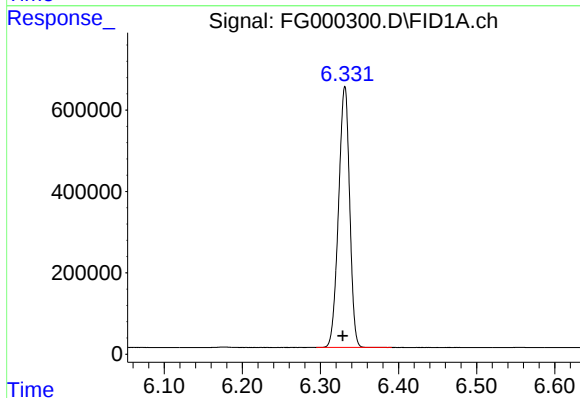


#3 N-DODECANE

R.T.: 6.331 min
Delta R.T.: 0.002 min
Response: 6337268
Conc: 45.27 ug/ml

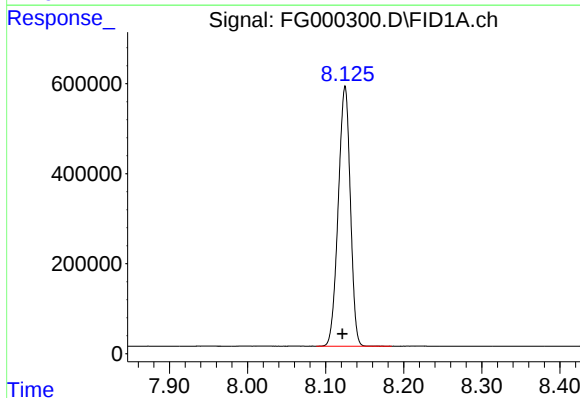


#4 N-TETRADECANE

R.T.: 8.125 min
Delta R.T.: 0.003 min
Response: 6201704
Conc: 45.11 ug/ml

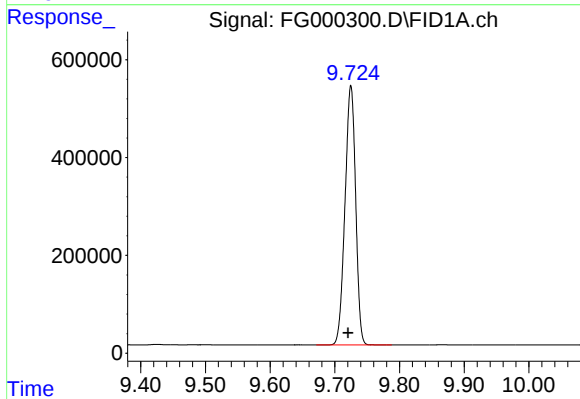

#5 N-HEXADECANE

R.T.: 9.725 min
Delta R.T.: 0.004 min
Response: 6055686
Conc: 45.76 ug/ml

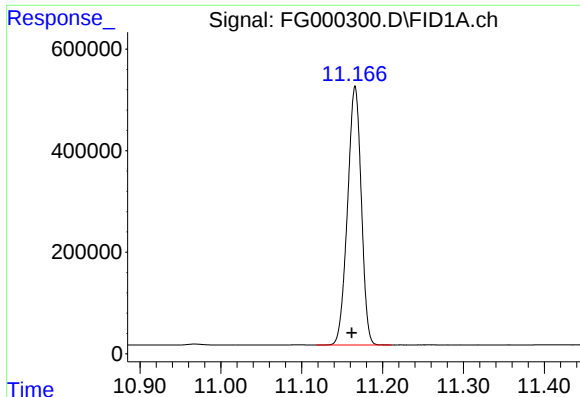


#6 N-OCTADECANE

R.T.: 11.166 min
Delta R.T.: 0.004 min
Response: 6012826
Conc: 45.40 ug/ml

Instrument :
FID_G
ClientSampleId :


Manual Integrations
APPROVED

ugo
3/9/2018 1:58:15 PM

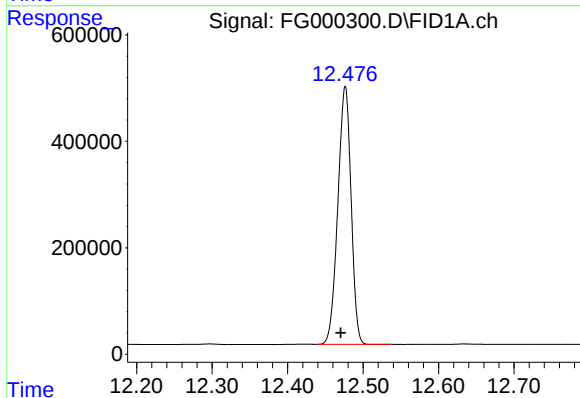


#7 N-EICOSANE

R.T.: 12.476 min
Delta R.T.: 0.006 min
Response: 5911481
Conc: 45.99 ug/ml

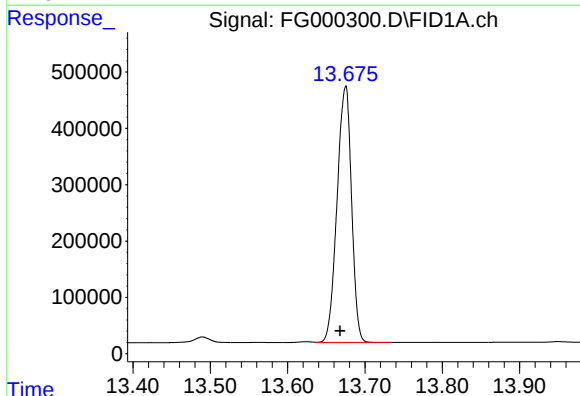


#8 N-DOCOSANE

R.T.: 13.674 min
Delta R.T.: 0.006 min
Response: 5919054
Conc: 48.22 ug/ml

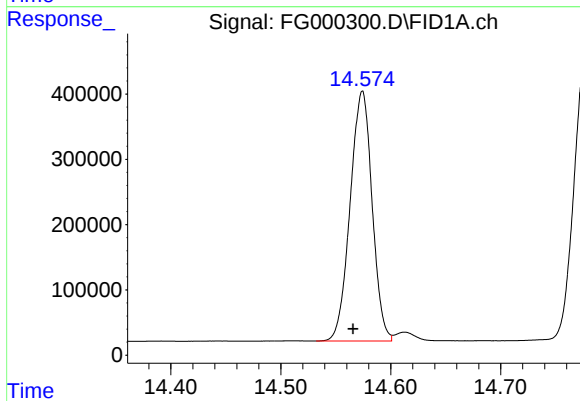

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.574 min
Delta R.T.: 0.008 min
Response: 5324281
Conc: 47.90 ug/ml m

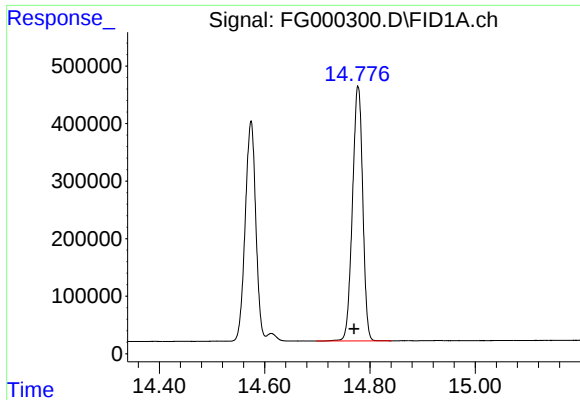


#10 N-TETRACOSANE

R.T.: 14.777 min
Delta R.T.: 0.008 min
Response: 5994477
Conc: 48.99 ug/ml

Instrument :
FID_G
ClientSampleId :


Manual Integrations
APPROVED

ugo
3/9/2018 1:58:15 PM

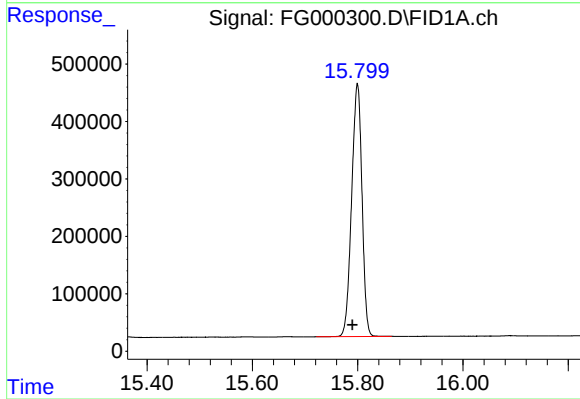

#11 N-HEXACOSANE

R.T.: 15.800 min
Delta R.T.: 0.009 min
Response: 6001877
Conc: 49.74 ug/ml

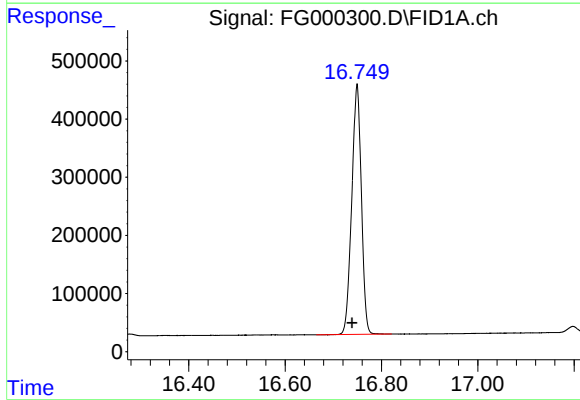

#12 N-OCTACOSANE

R.T.: 16.749 min
Delta R.T.: 0.010 min
Response: 5988514
Conc: 50.47 ug/ml