

Data Path : P:\HPCHEM1\FID_G\Data\FG030918\
 Data File : FG000318.D
 Signal(s) : FID1A.ch
 Acq On : 09 Mar 2018 10:17
 Operator : UA\AJ
 Sample : J1819-01 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 09 10:43:59 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FG022818.M
 Quant Title :
 QLast Update : Wed Feb 28 18:10:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.571	301668	2.714 ug/ml
Target Compounds			
5) N-HEXADECANE	9.723	224979	1.700 ug/ml
7) N-EICOSANE	12.519	961722	7.483 ug/ml
10) N-TETRACOSANE	14.735	379165	3.098 ug/ml
12) N-OCTACOSANE	16.732	352117	2.968 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_G\Data\FG030918\
Data File : FG000318.D
Signal(s) : FID1A.ch
Acq On : 09 Mar 2018 10:17
Operator : UA\AJ
Sample : J1819-01 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 09 10:43:59 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FG022818.M
Quant Title :
QLast Update : Wed Feb 28 18:10:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

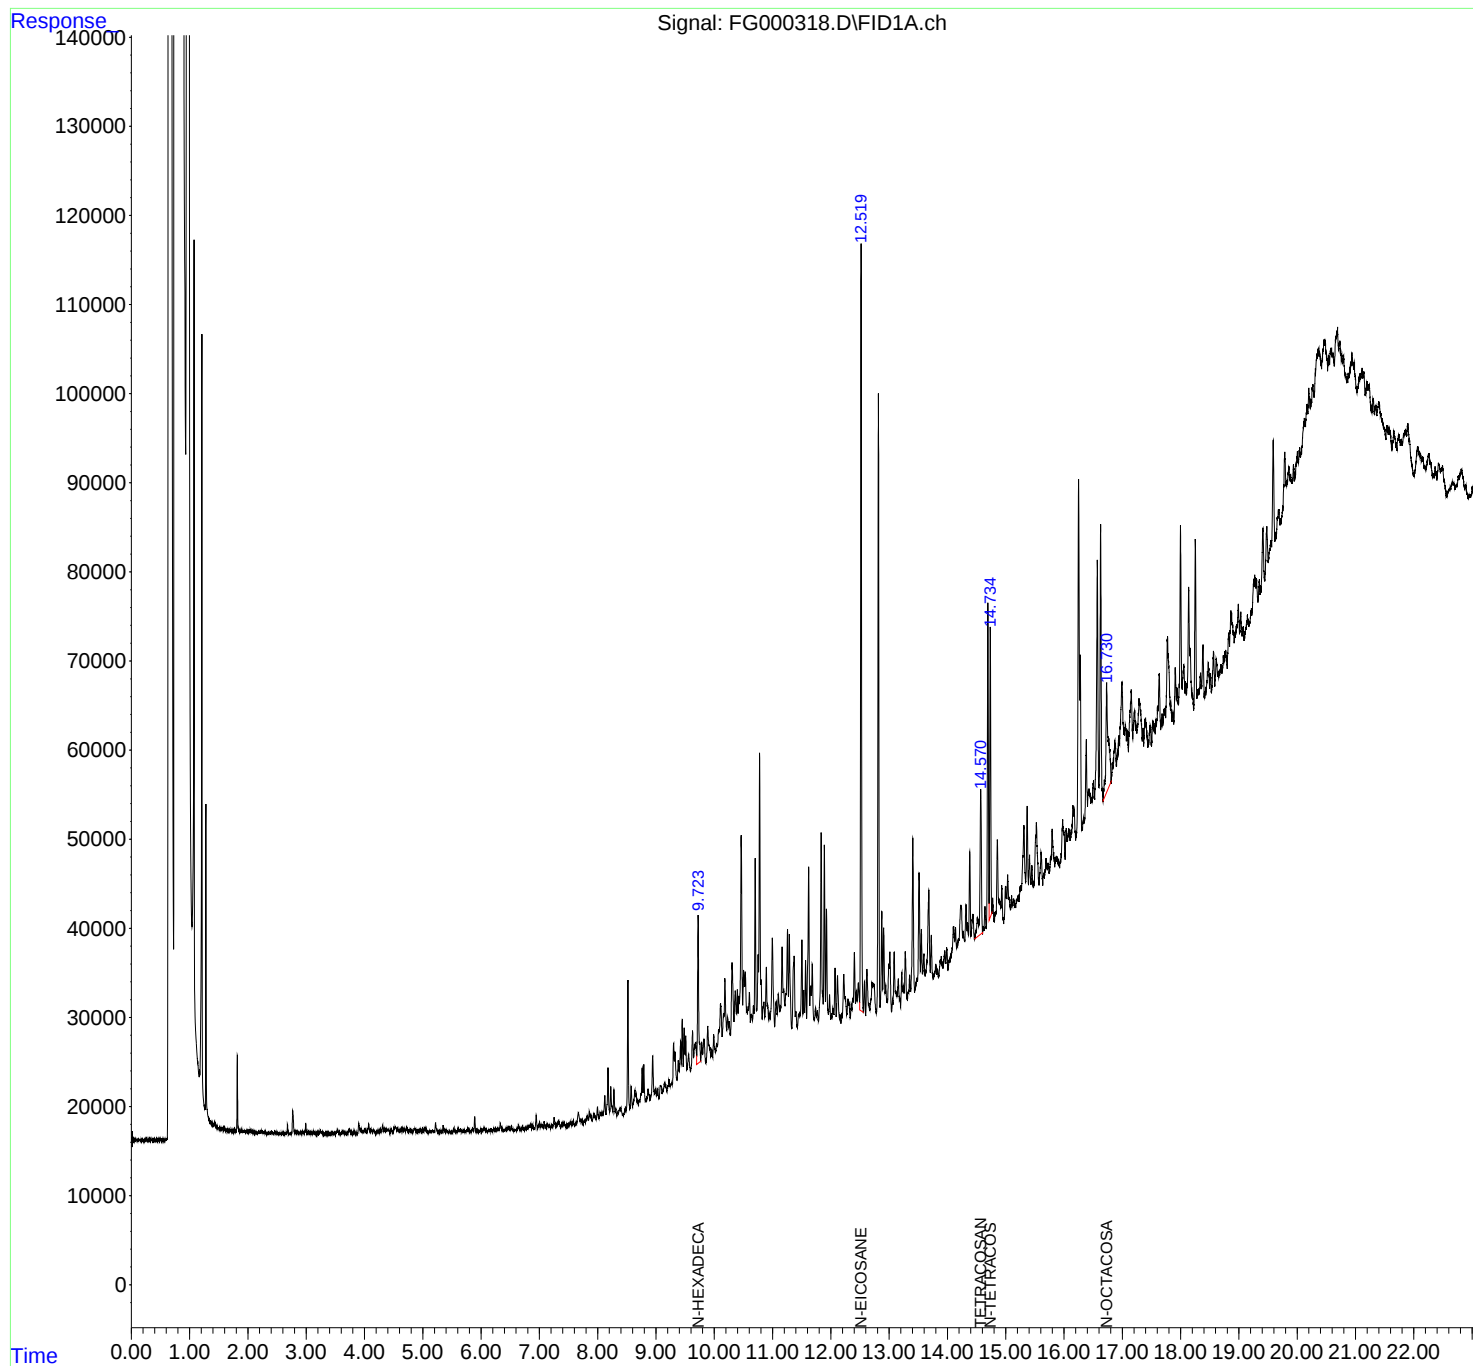


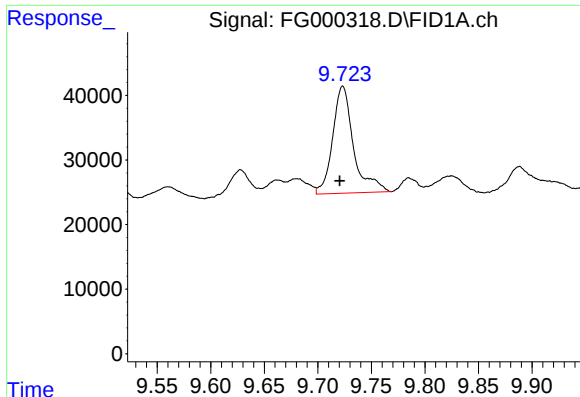

#5 N-HEXADECANE


R.T.: 9.723 min
Delta R.T.: 0.003 min
Response: 224979
Conc: 1.70 ug/ml

Instrument :
FID_G
ClientSampleId :

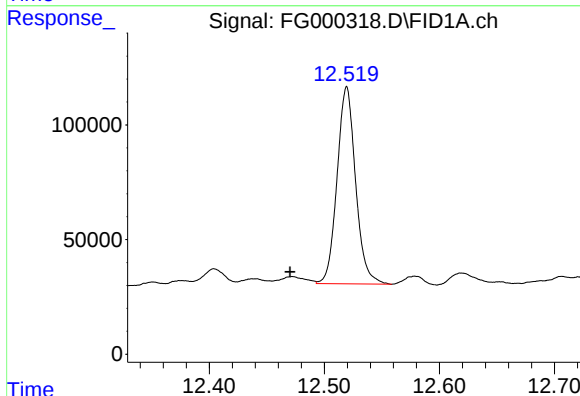


#7 N-EICOSANE

R.T.: 12.519 min
Delta R.T.: 0.049 min
Response: 961722
Conc: 7.48 ug/ml

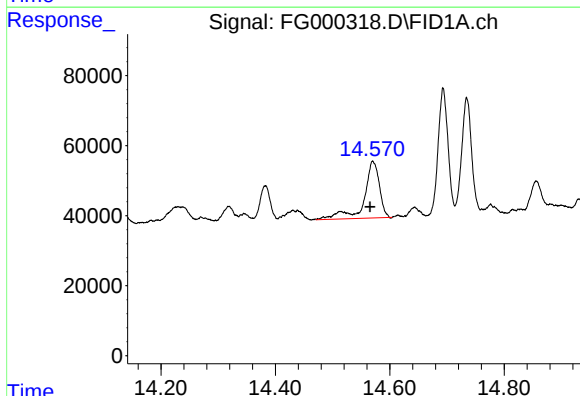


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.571 min
Delta R.T.: 0.005 min
Response: 301668
Conc: 2.71 ug/ml

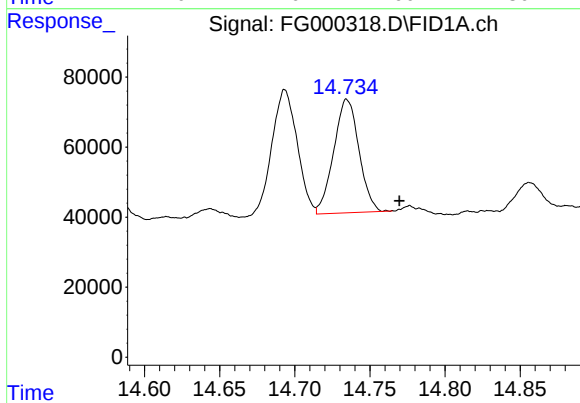

#10 N-TETRACOSANE

R.T.: 14.735 min
Delta R.T.: -0.035 min
Response: 379165
Conc: 3.10 ug/ml

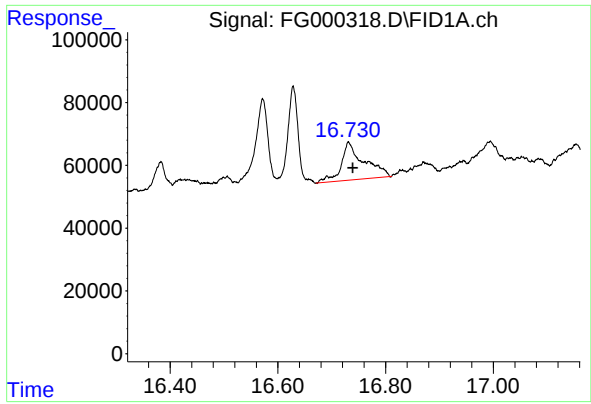

#12 N-OCTACOSANE

R.T.: 16.732 min
Delta R.T.: -0.007 min
Response: 352117
Conc: 2.97 ug/ml

Instrument :
FID_G
ClientSampleId :