

Data Path : P:\HPCHEM1\FID_G\Data\FG030918\
 Data File : FG000319.D
 Signal(s) : FID1A.ch
 Acq On : 09 Mar 2018 10:45
 Operator : UA\AJ
 Sample : J1741-02 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 09 14:13:11 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FG022818.M
 Quant Title :
 QLast Update : Wed Feb 28 18:10:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.570	459662	4.135 ug/ml
Target Compounds			
7) N-EICOSANE	12.520f	2577165	20.052 ug/ml
8) N-DOCOSANE	13.680	350756	2.858 ug/ml
10) N-TETRACOSANE	14.735	1275367	10.422 ug/ml
12) N-OCTACOSANE	16.731	326307	2.750 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_G\Data\FG030918\
Data File : FG000319.D
Signal(s) : FID1A.ch
Acq On : 09 Mar 2018 10:45
Operator : UA\AJ
Sample : J1741-02 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 09 14:13:11 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FG022818.M
Quant Title :
QLast Update : Wed Feb 28 18:10:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

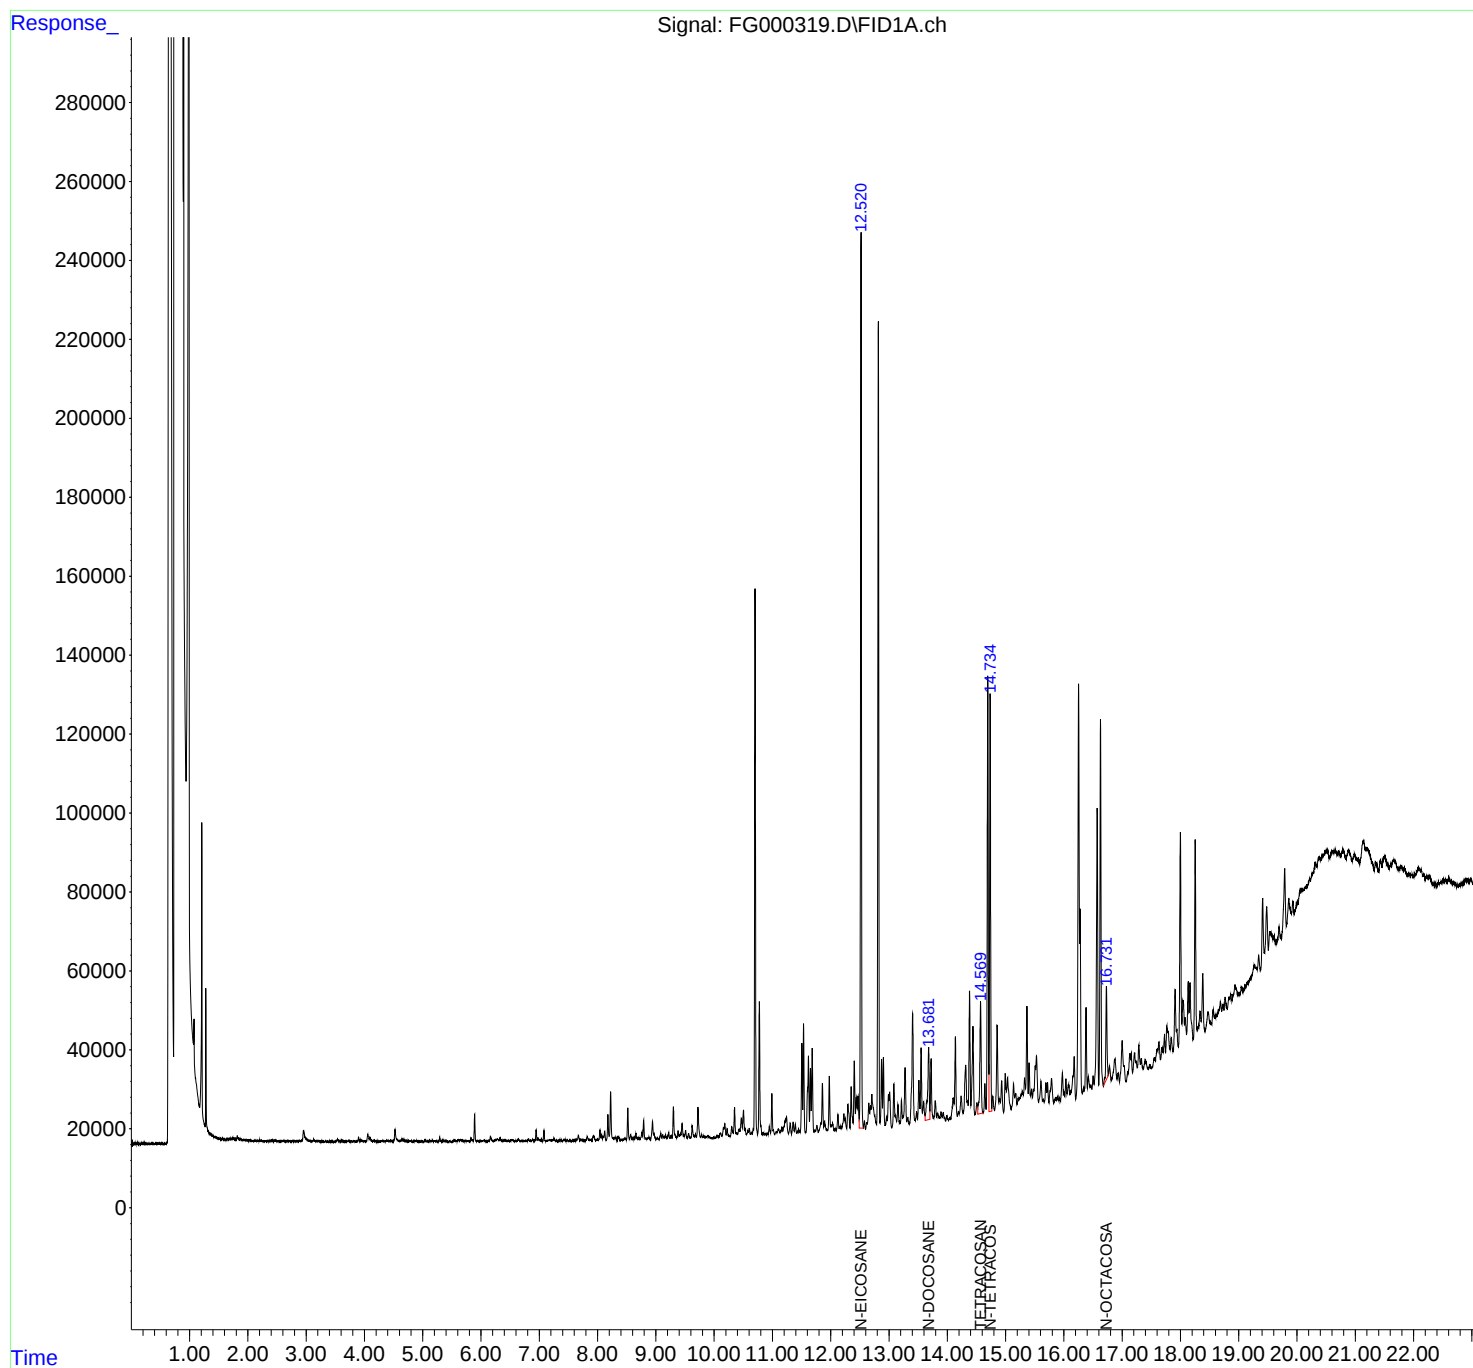


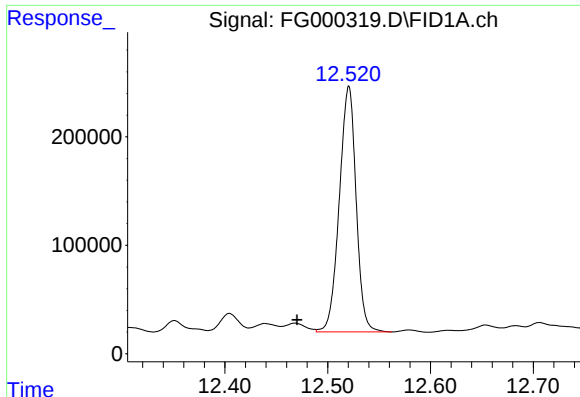

#7 N-EICOSANE


R.T.: 12.520 min
Delta R.T.: 0.050 min
Response: 2577165
Conc: 20.05 ug/ml

Instrument :
FID_G
ClientSampleId :

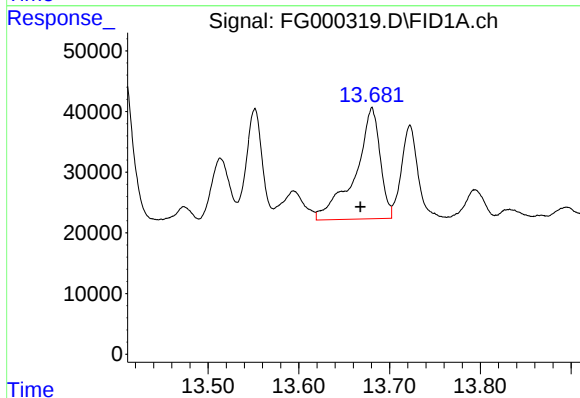


#8 N-DOCOSANE

R.T.: 13.680 min
Delta R.T.: 0.013 min
Response: 350756
Conc: 2.86 ug/ml

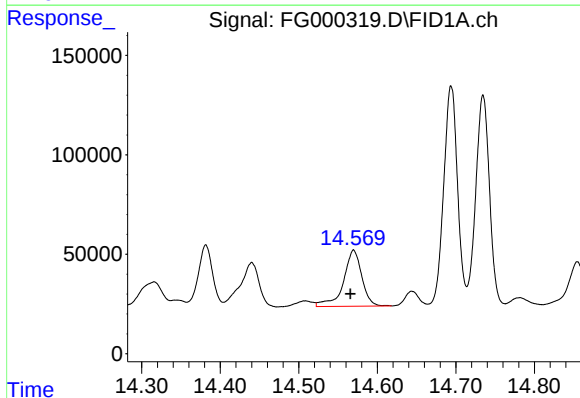


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.570 min
Delta R.T.: 0.004 min
Response: 459662
Conc: 4.14 ug/ml

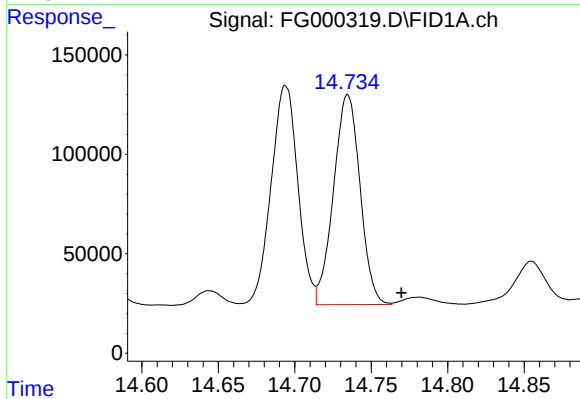

#10 N-TETRACOSANE

R.T.: 14.735 min
Delta R.T.: -0.035 min
Response: 1275367
Conc: 10.42 ug/ml

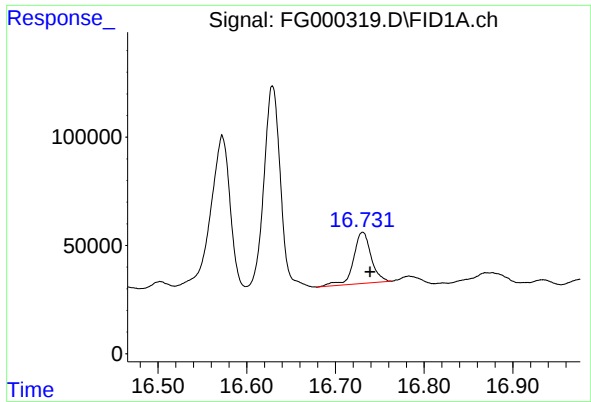

#12 N-OCTACOSANE

R.T.: 16.731 min

Delta R.T.: -0.008 min

Response: 326307

Conc: 2.75 ug/ml

Instrument :
FID_G
ClientSampleId :