

Data Path : P:\HPCHEM1\FID_G\Data\FG030918\
 Data File : FG000320.D
 Signal(s) : FID1A.ch
 Acq On : 09 Mar 2018 11:14
 Operator : UA\AJ
 Sample : J1829-02 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 09 14:13:20 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FG022818.M
 Quant Title :
 QLast Update : Wed Feb 28 18:10:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.570	561173	5.049 ug/ml
Target Compounds			
7) N-EICOSANE	12.518	1829555	14.235 ug/ml
8) N-DOCOSANE	13.680	233065	1.899 ug/ml
10) N-TETRACOSANE	14.734	1037671	8.480 ug/ml
12) N-OCTACOSANE	16.731	327232	2.758 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_G\Data\FG030918\
Data File : FG000320.D
Signal(s) : FID1A.ch
Acq On : 09 Mar 2018 11:14
Operator : UA\AJ
Sample : J1829-02 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 09 14:13:20 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FG022818.M
Quant Title :
QLast Update : Wed Feb 28 18:10:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

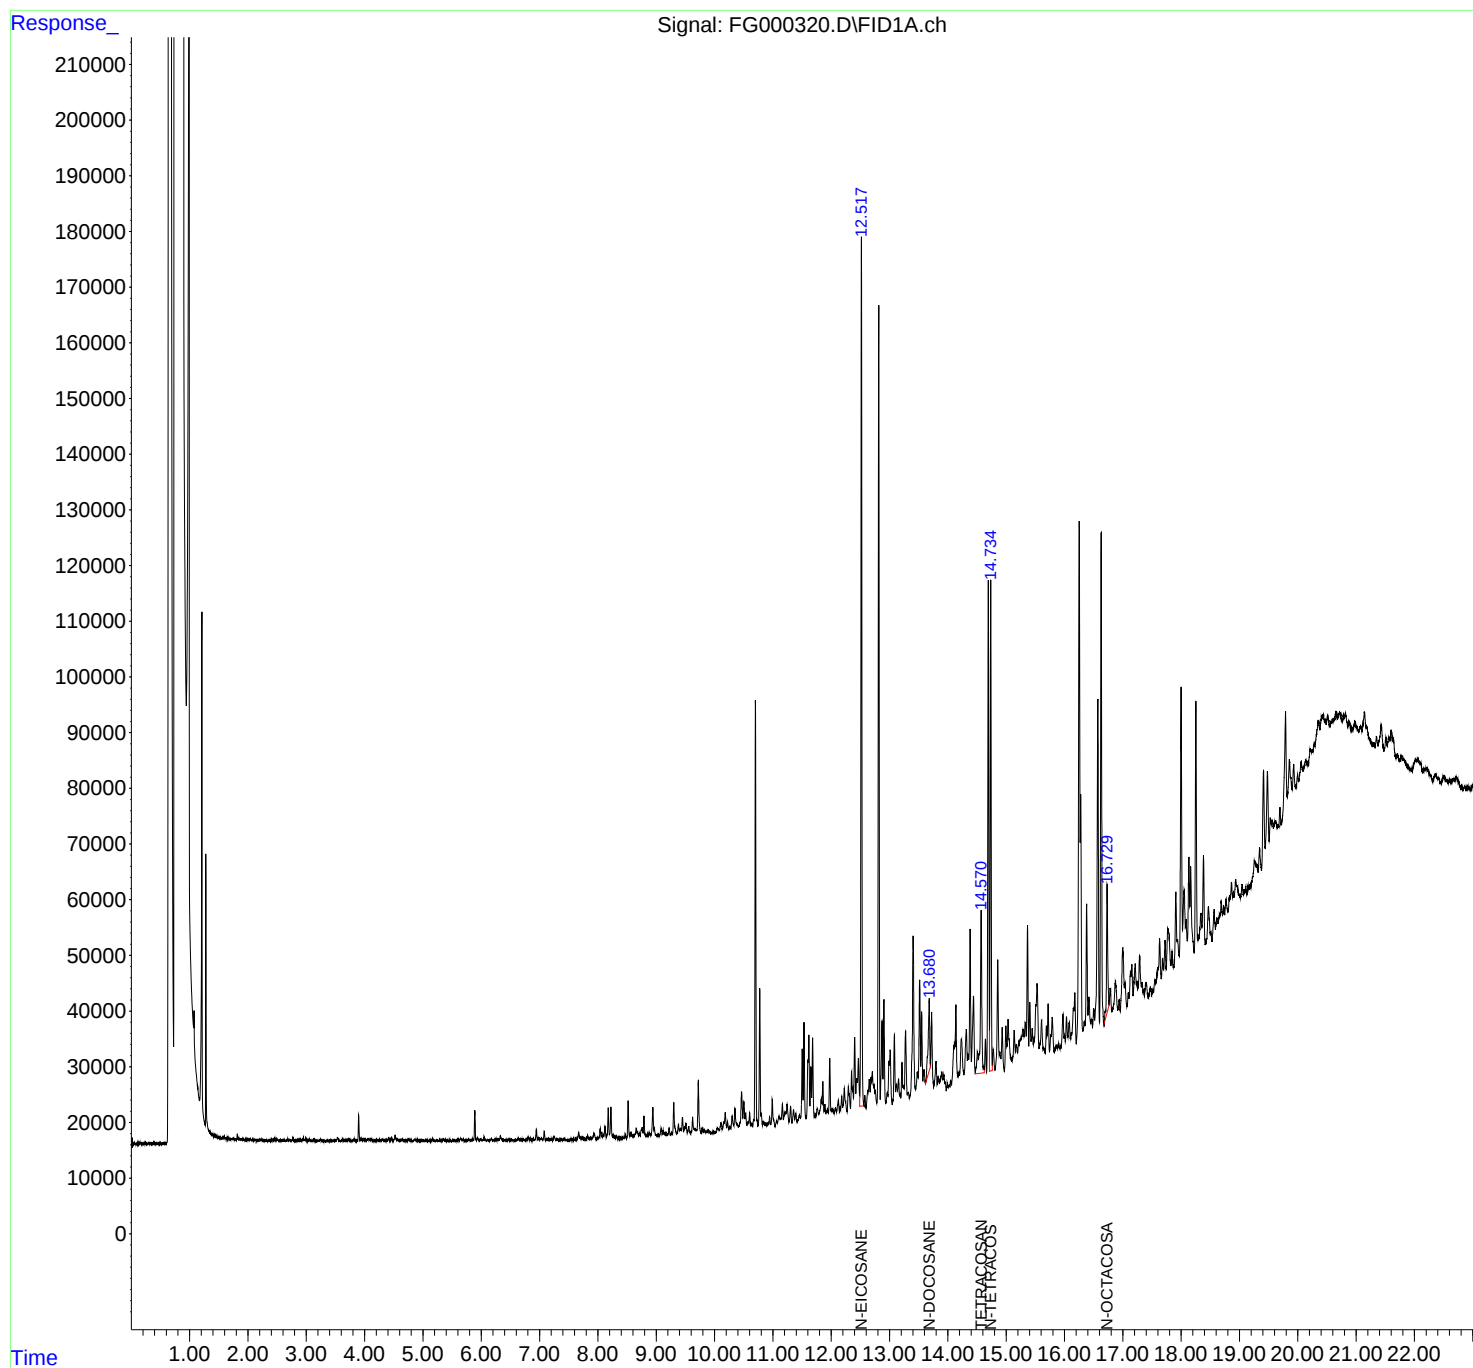


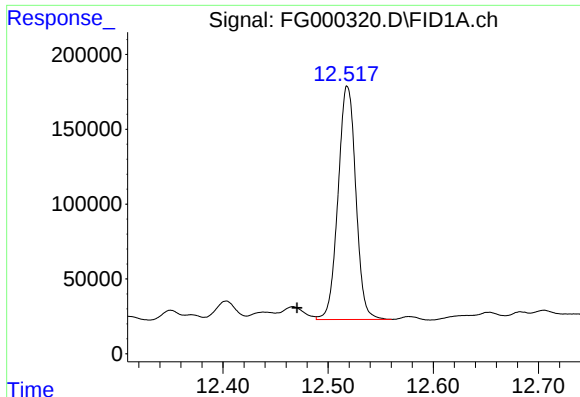

#7 N-EICOSANE


R.T.: 12.518 min
Delta R.T.: 0.048 min
Response: 1829555
Conc: 14.23 ug/ml

Instrument :
FID_G
ClientSampleId :

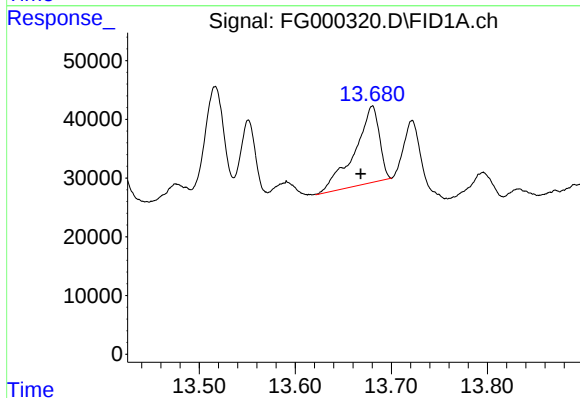


#8 N-DOCOSANE

R.T.: 13.680 min
Delta R.T.: 0.012 min
Response: 233065
Conc: 1.90 ug/ml

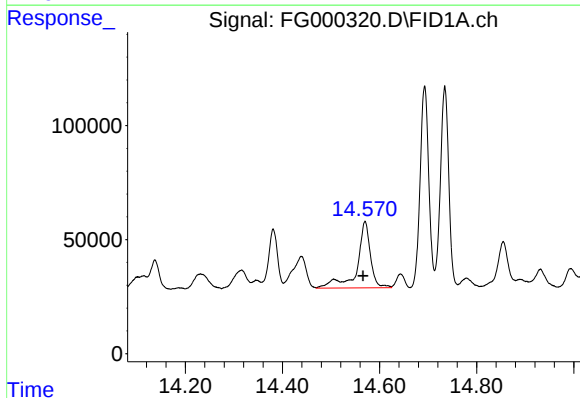


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.570 min
Delta R.T.: 0.004 min
Response: 561173
Conc: 5.05 ug/ml

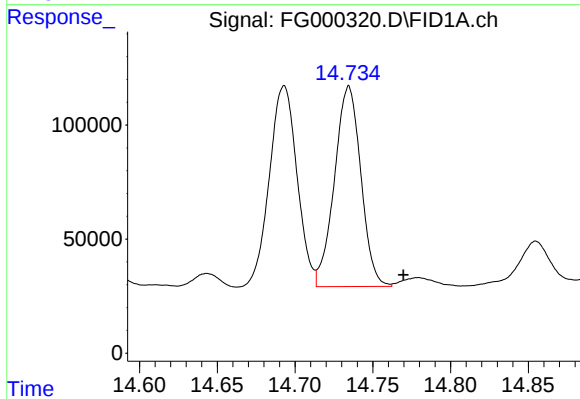

#10 N-TETRACOSANE

R.T.: 14.734 min
Delta R.T.: -0.035 min
Response: 1037671
Conc: 8.48 ug/ml

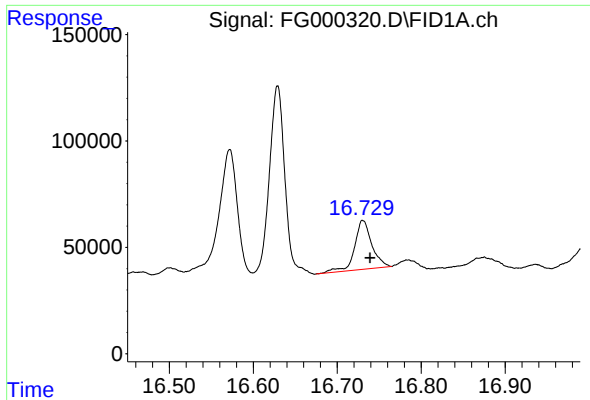

#12 N-OCTACOSANE

R.T.: 16.731 min

Delta R.T.: -0.008 min

Response: 327232

Conc: 2.76 ug/ml

Instrument :
FID_G
ClientSampleId :