

Data Path : P:\HPCHEM1\FID_G\Data\FG030918\
 Data File : FG000321.D
 Signal(s) : FID1A.ch
 Acq On : 09 Mar 2018 11:43
 Operator : UA\AJ
 Sample : J1829-05 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 09 14:13:29 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FG022818.M
 Quant Title :
 QLast Update : Wed Feb 28 18:10:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.569	469824	4.227 ug/ml
Target Compounds			
7) N-EICOSANE	12.518	1631025	12.690 ug/ml
8) N-DOCOSANE	13.679	326415	2.659 ug/ml
10) N-TETRACOSANE	14.733	1064514	8.699 ug/ml
12) N-OCTACOSANE	16.733	936004	7.888 ug/ml
13) N-TRIACONTANE	17.629	1724099	14.947 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_G\Data\FG030918\
Data File : FG000321.D
Signal(s) : FID1A.ch
Acq On : 09 Mar 2018 11:43
Operator : UA\AJ
Sample : J1829-05 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 09 14:13:29 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FG022818.M
Quant Title :
QLast Update : Wed Feb 28 18:10:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

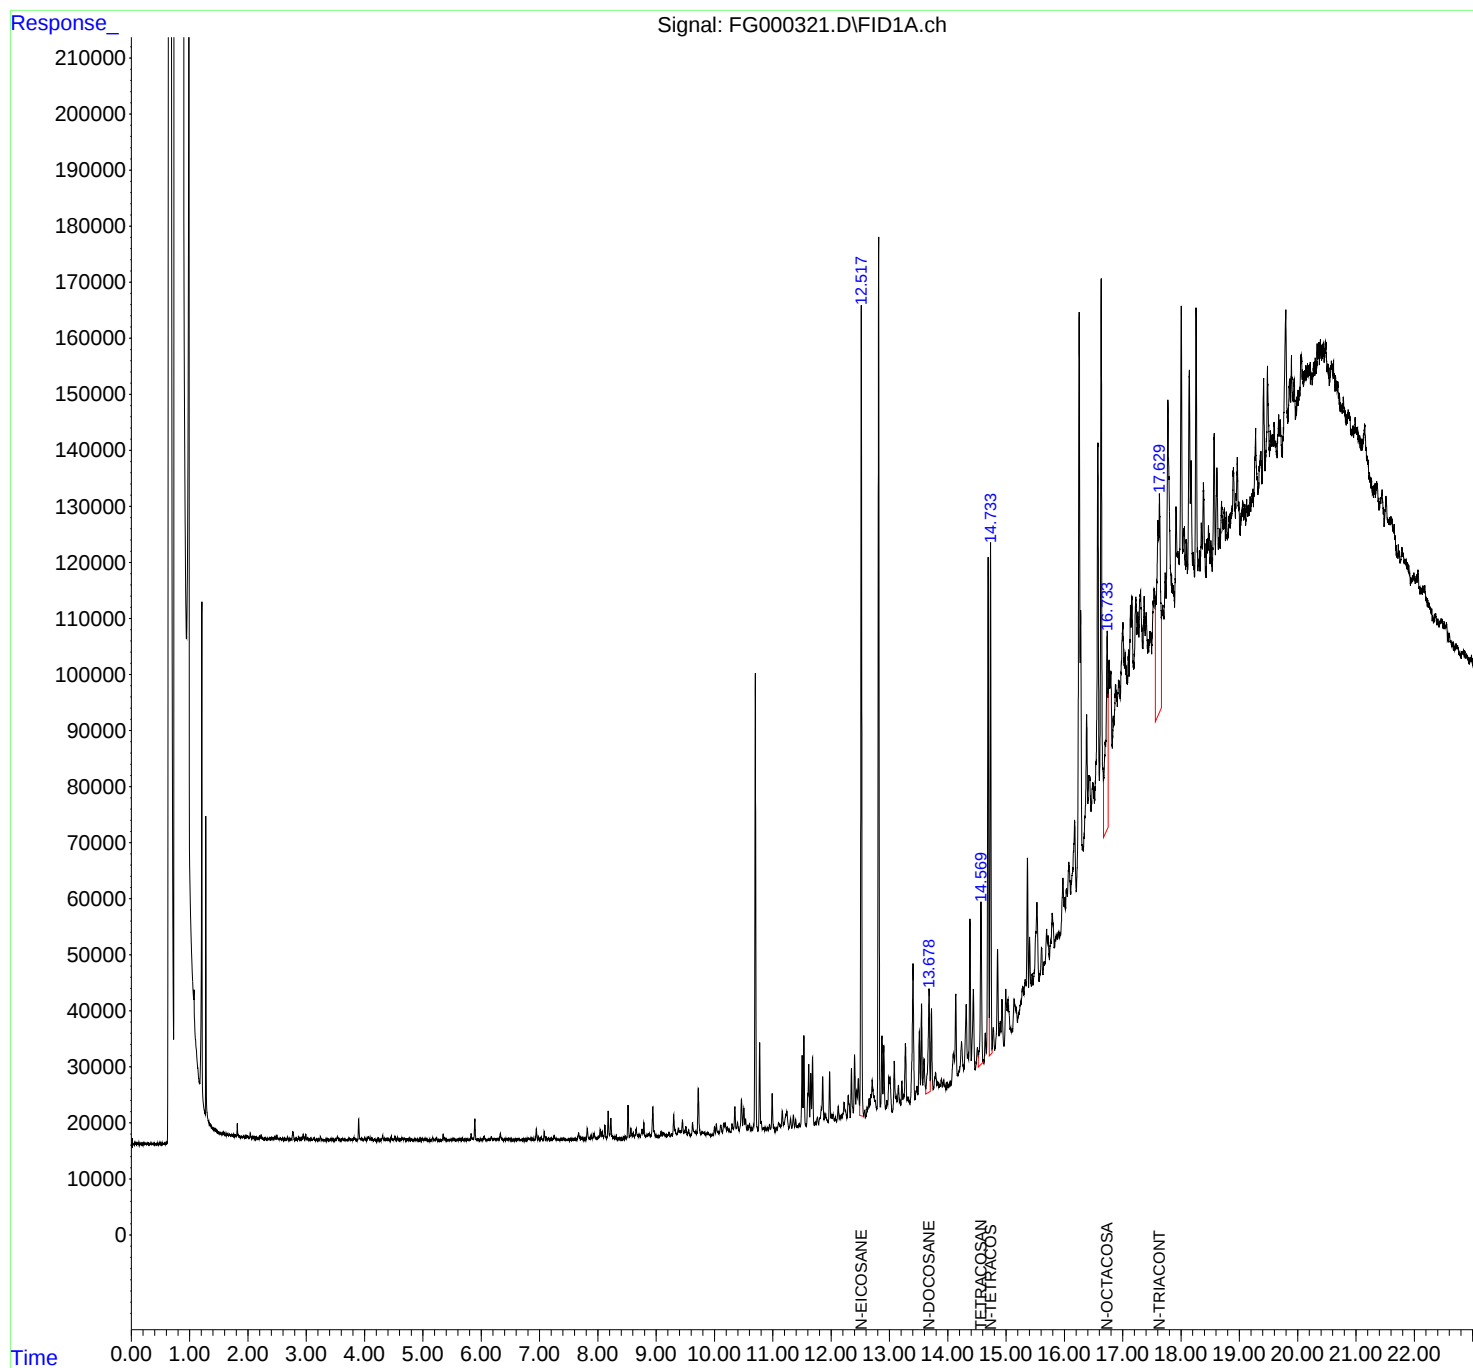


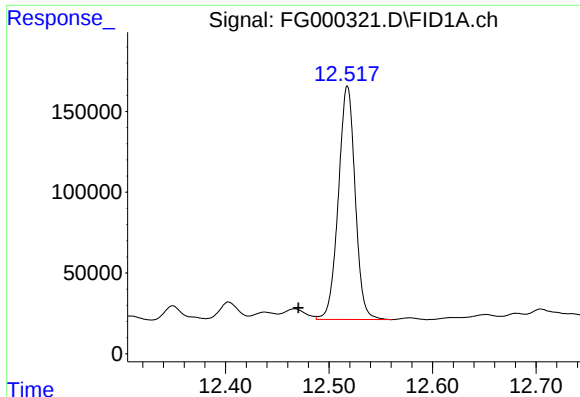

#7 N-EICOSANE


R.T.: 12.518 min
Delta R.T.: 0.047 min
Response: 1631025
Conc: 12.69 ug/ml

Instrument :
FID_G
ClientSampleId :

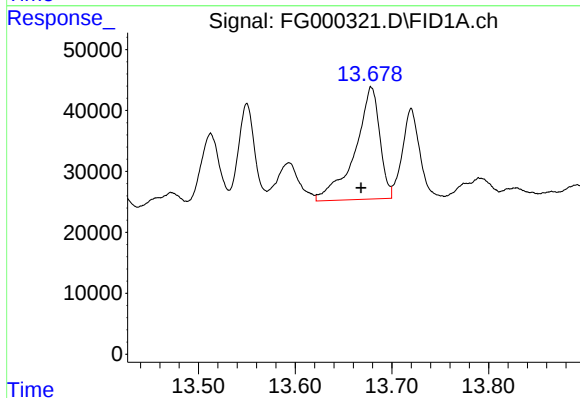


#8 N-DOCOSANE

R.T.: 13.679 min
Delta R.T.: 0.011 min
Response: 326415
Conc: 2.66 ug/ml

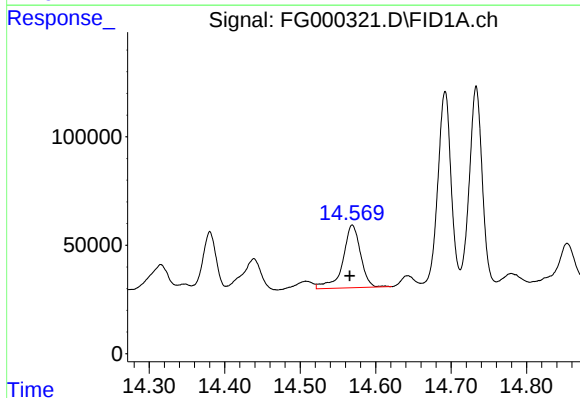


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.569 min
Delta R.T.: 0.003 min
Response: 469824
Conc: 4.23 ug/ml

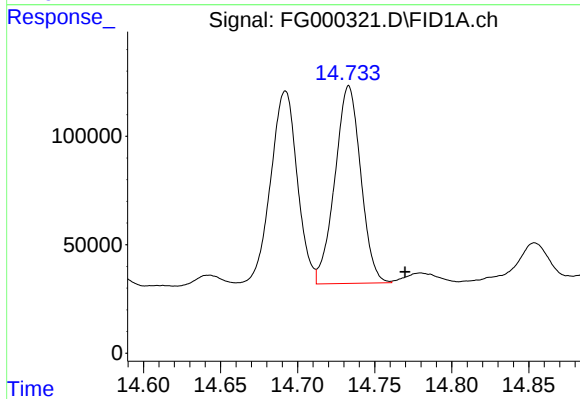

#10 N-TETRACOSANE


R.T.: 14.733 min
Delta R.T.: -0.036 min
Response: 1064514
Conc: 8.70 ug/ml

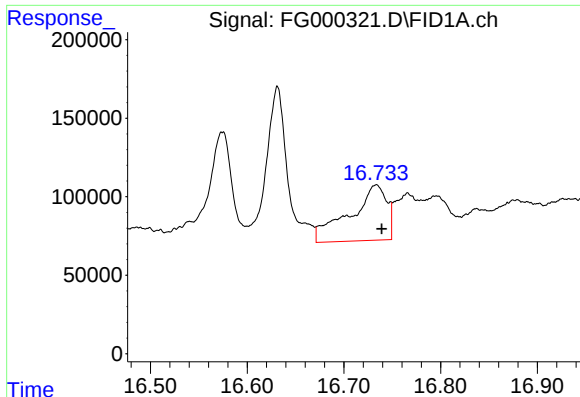

#12 N-OCTACOSANE

R.T.: 16.733 min
Delta R.T.: -0.006 min
Response: 936004
Conc: 7.89 ug/ml

Instrument :
FID_G
ClientSampleId :

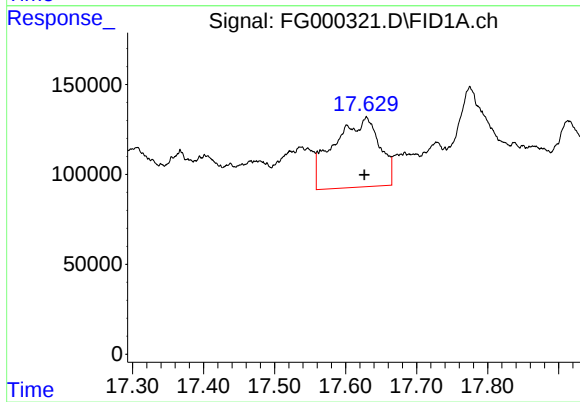

#13 N-TRIACONTANE

R.T.: 17.629 min
Delta R.T.: 0.003 min
Response: 1724099
Conc: 14.95 ug/ml