

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031219\
 Data File : FG004136.D
 Signal(s) : FID1A.ch
 Acq On : 12 Mar 2019 17:08
 Operator : AJ\SJ
 Sample : K1687-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 13 01:29:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
 Quant Title :
 QLast Update : Tue Mar 05 03:05:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.434	1651502	13.136 ug/ml
Target Compounds			
2) N-DECANE	4.167	3927982	29.379 ug/ml
3) N-DODECANE	6.195	13023342	96.065 ug/ml
4) N-TETRADECANE	7.987	8878482	63.670 ug/ml
5) N-HEXADECANE	9.583	2533353	17.801 ug/ml
6) N-OCTADECANE	11.023	860874	6.000 ug/ml
7) N-EICOSANE	12.333	307690	2.154 ug/ml
11) N-HEXACOSANE	15.656	210184	1.509 ug/ml
12) N-OCTACOSANE	16.609	475174	3.471 ug/ml
13) N-TRIACONTANE	17.497	634784	4.753 ug/ml
14) N-DOTRIACONTANE	18.329	579489	4.580 ug/ml
15) N-TETRATRIACONTANE	19.117	260786	2.201 ug/ml
16) N-HEXATRIACONTANE	19.858	223808	2.022 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031219\
Data File : FG004136.D
Signal(s) : FID1A.ch
Acq On : 12 Mar 2019 17:08
Operator : AJ\SJ
Sample : K1687-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 13 01:29:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

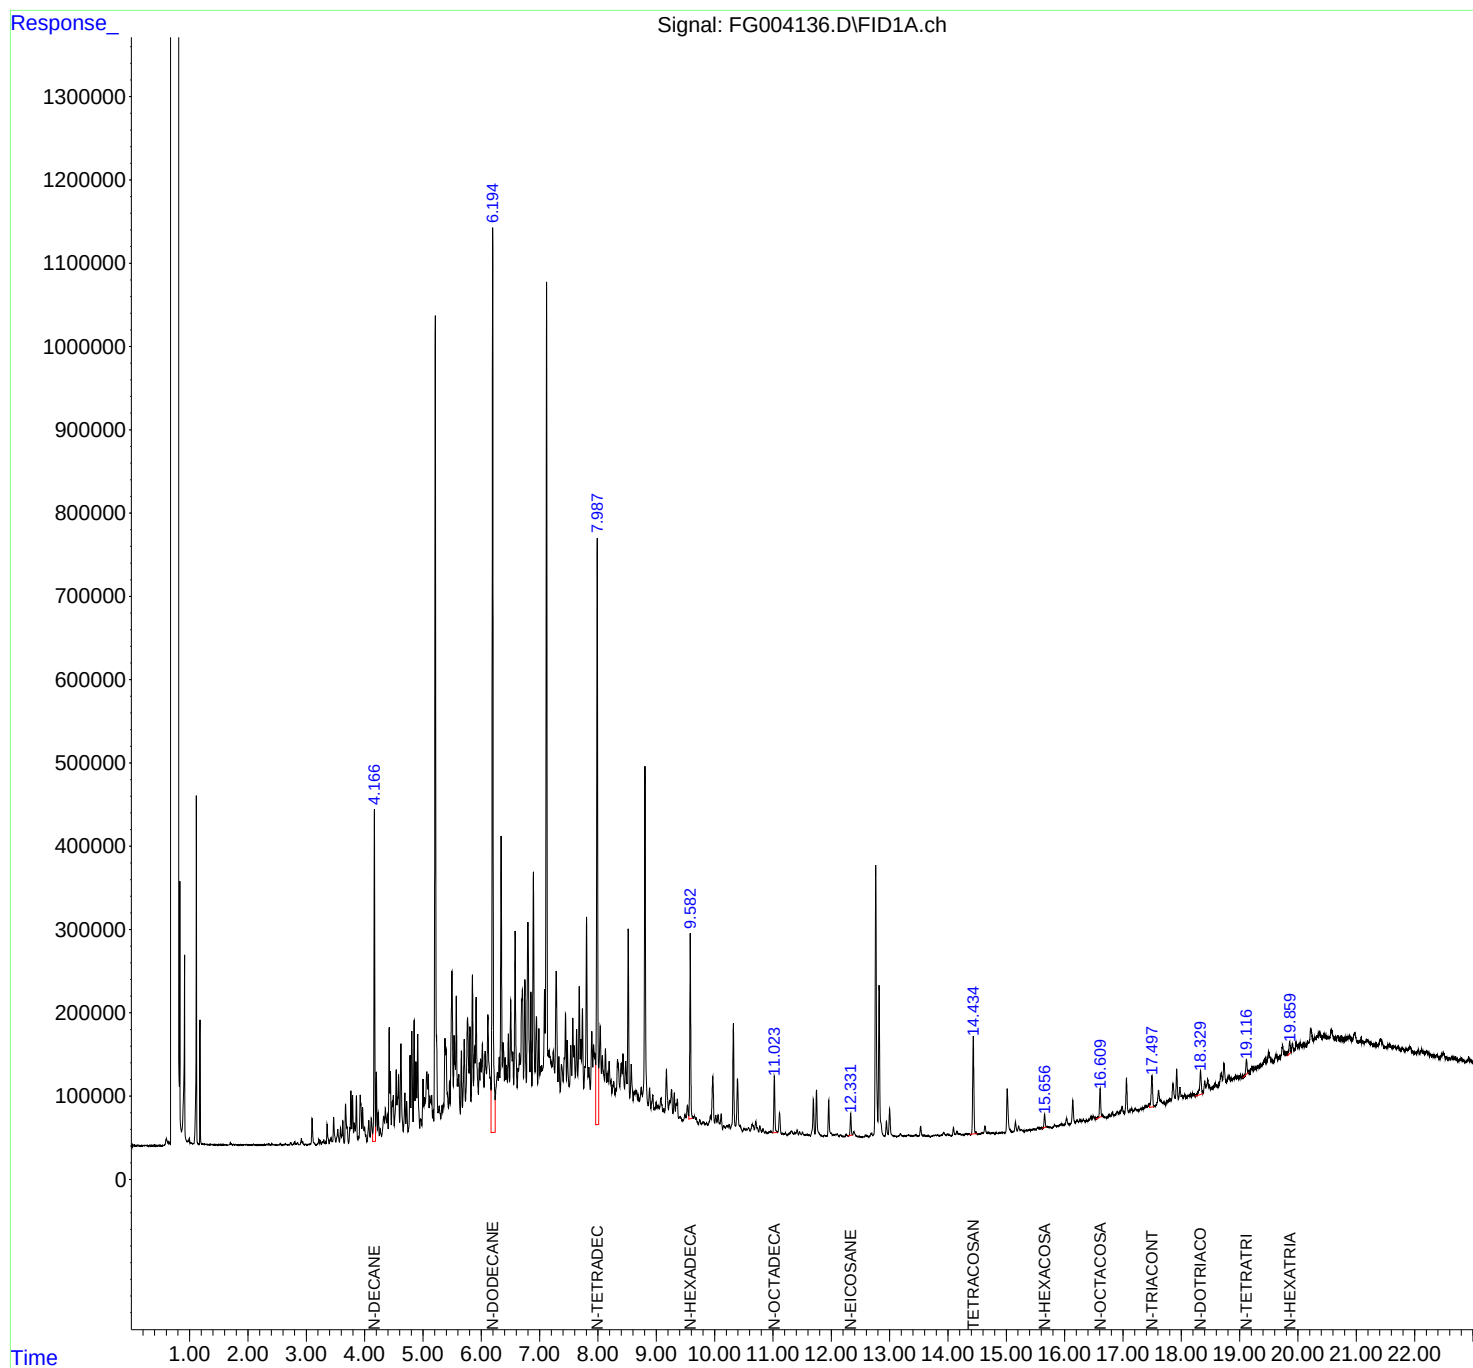


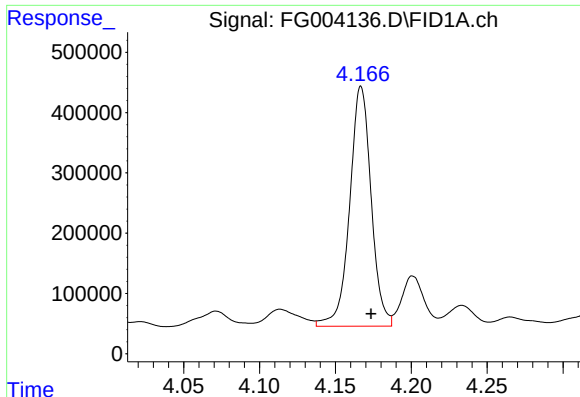

#2 N-DECANE


R.T.: 4.167 min
Delta R.T.: -0.007 min
Response: 3927982
Conc: 29.38 ug/ml

Instrument :
FID_G
ClientSampleId :

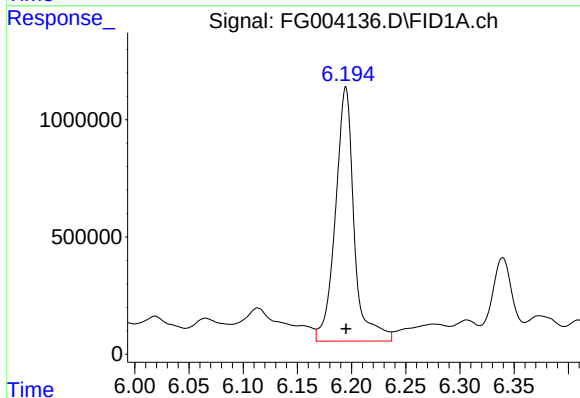


#3 N-DODECANE

R.T.: 6.195 min
Delta R.T.: 0.000 min
Response: 13023342
Conc: 96.07 ug/ml

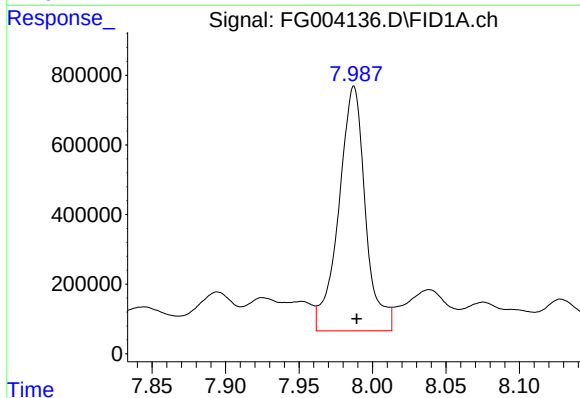


#4 N-TETRADECANE

R.T.: 7.987 min
Delta R.T.: -0.002 min
Response: 8878482
Conc: 63.67 ug/ml

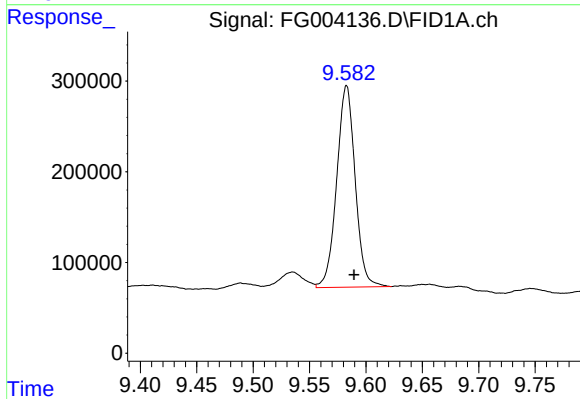

#5 N-HEXADECANE


R.T.: 9.583 min
Delta R.T.: -0.007 min
Response: 2533353
Conc: 17.80 ug/ml

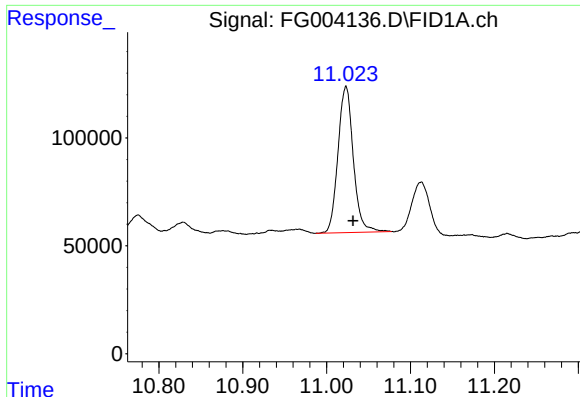

#6 N-OCTADECANE


R.T.: 11.023 min
Delta R.T.: -0.008 min
Response: 860874
Conc: 6.00 ug/ml

Instrument :
FID_G
ClientSampleId :

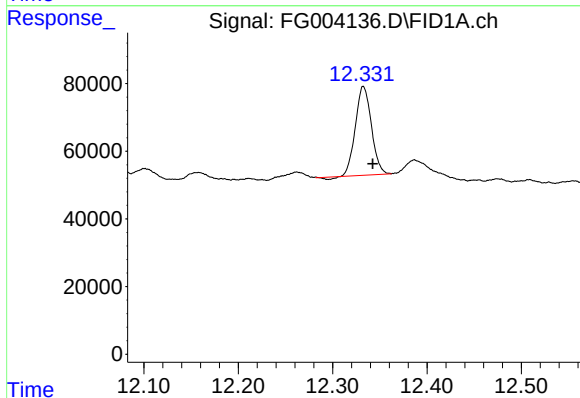


#7 N-EICOSANE

R.T.: 12.333 min
Delta R.T.: -0.010 min
Response: 307690
Conc: 2.15 ug/ml

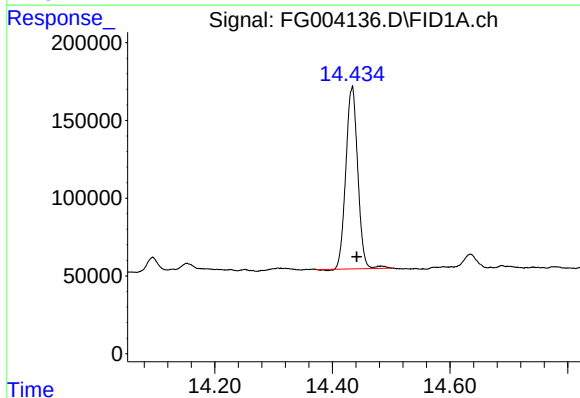


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.434 min
Delta R.T.: -0.008 min
Response: 1651502
Conc: 13.14 ug/ml

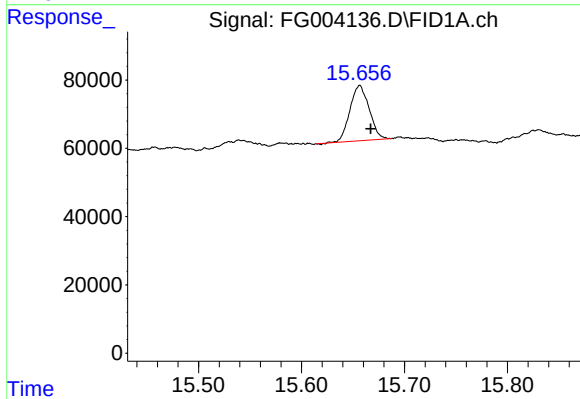

#11 N-HEXACOSANE


R.T.: 15.656 min
Delta R.T.: -0.011 min
Response: 210184
Conc: 1.51 ug/ml

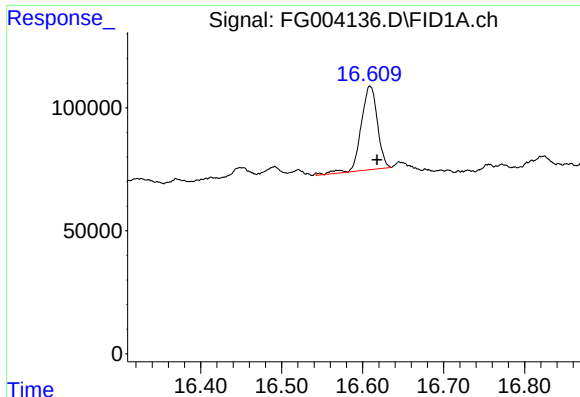

#12 N-OCTACOSANE


R.T.: 16.609 min
Delta R.T.: -0.008 min
Response: 475174
Conc: 3.47 ug/ml

Instrument :
FID_G
ClientSampleId :

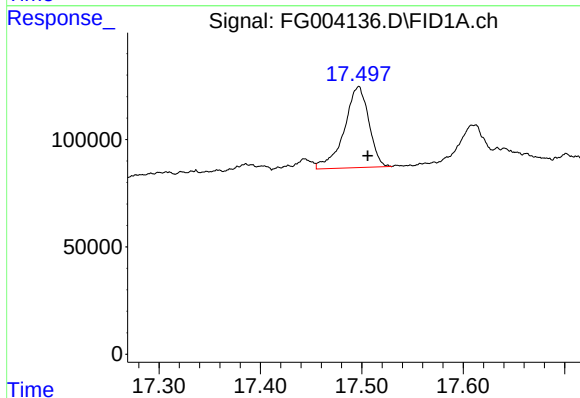


#13 N-TRIACONTANE

R.T.: 17.497 min
Delta R.T.: -0.009 min
Response: 634784
Conc: 4.75 ug/ml

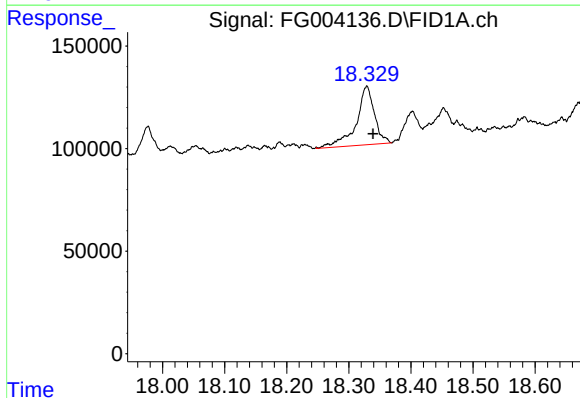


#14 N-DOTRIACONTANE

R.T.: 18.329 min
Delta R.T.: -0.010 min
Response: 579489
Conc: 4.58 ug/ml

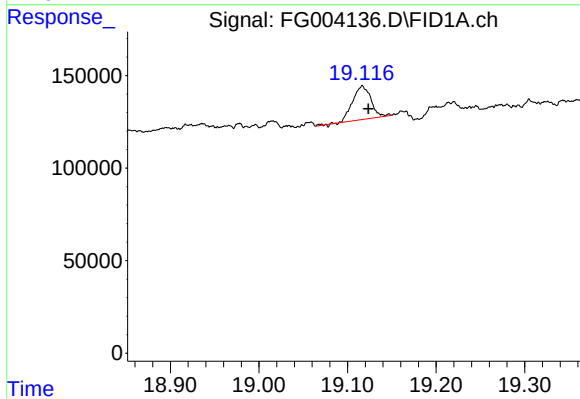

#15 N-TETRATRIACONTANE

R.T.: 19.117 min
Delta R.T.: -0.007 min
Response: 260786
Conc: 2.20 ug/ml

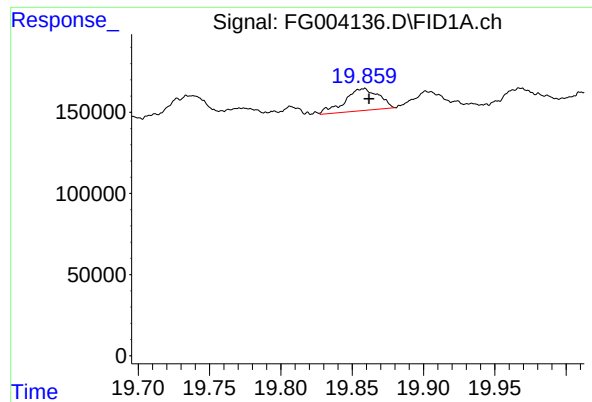

#16 N-HEXATRIACONTANE

R.T.: 19.858 min
Delta R.T.: -0.003 min
Response: 223808
Conc: 2.02 ug/ml

Instrument :
FID_G
ClientSampleId :