

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031219\
 Data File : FG004141.D
 Signal(s) : FID1A.ch
 Acq On : 12 Mar 2019 19:40
 Operator : AJ\SJ
 Sample : K1697-07 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 13 01:31:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
 Quant Title :
 QLast Update : Tue Mar 05 03:05:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.438	674568	5.366 ug/ml
Target Compounds			
3) N-DODECANE	6.191	726687	5.360 ug/ml
4) N-TETRADECANE	7.984	1386950	9.946 ug/ml
5) N-HEXADECANE	9.584	1564002	10.989 ug/ml
6) N-OCTADECANE	11.026	1313996	9.158 ug/ml
7) N-EICOSANE	12.337	1093380	7.654 ug/ml
8) N-DOCOSANE	13.538	901879	6.354 ug/ml
10) N-TETRACOSANE	14.637	827897	5.870 ug/ml
11) N-HEXACOSANE	15.662	501289	3.599 ug/ml
12) N-OCTACOSANE	16.615	619348	4.524 ug/ml
13) N-TRIACONTANE	17.506	825656	6.183 ug/ml
14) N-DOTRIACONTANE	18.337	640604	5.063 ug/ml
15) N-TETRATRIACONTANE	19.126	888656	7.499 ug/ml
16) N-HEXATRIACONTANE	19.870	497134	4.491 ug/ml
17) N-OCTATRIACONTANE	20.579	536435	5.314 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031219\
Data File : FG004141.D
Signal(s) : FID1A.ch
Acq On : 12 Mar 2019 19:40
Operator : AJ\SJ
Sample : K1697-07 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 13 01:31:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

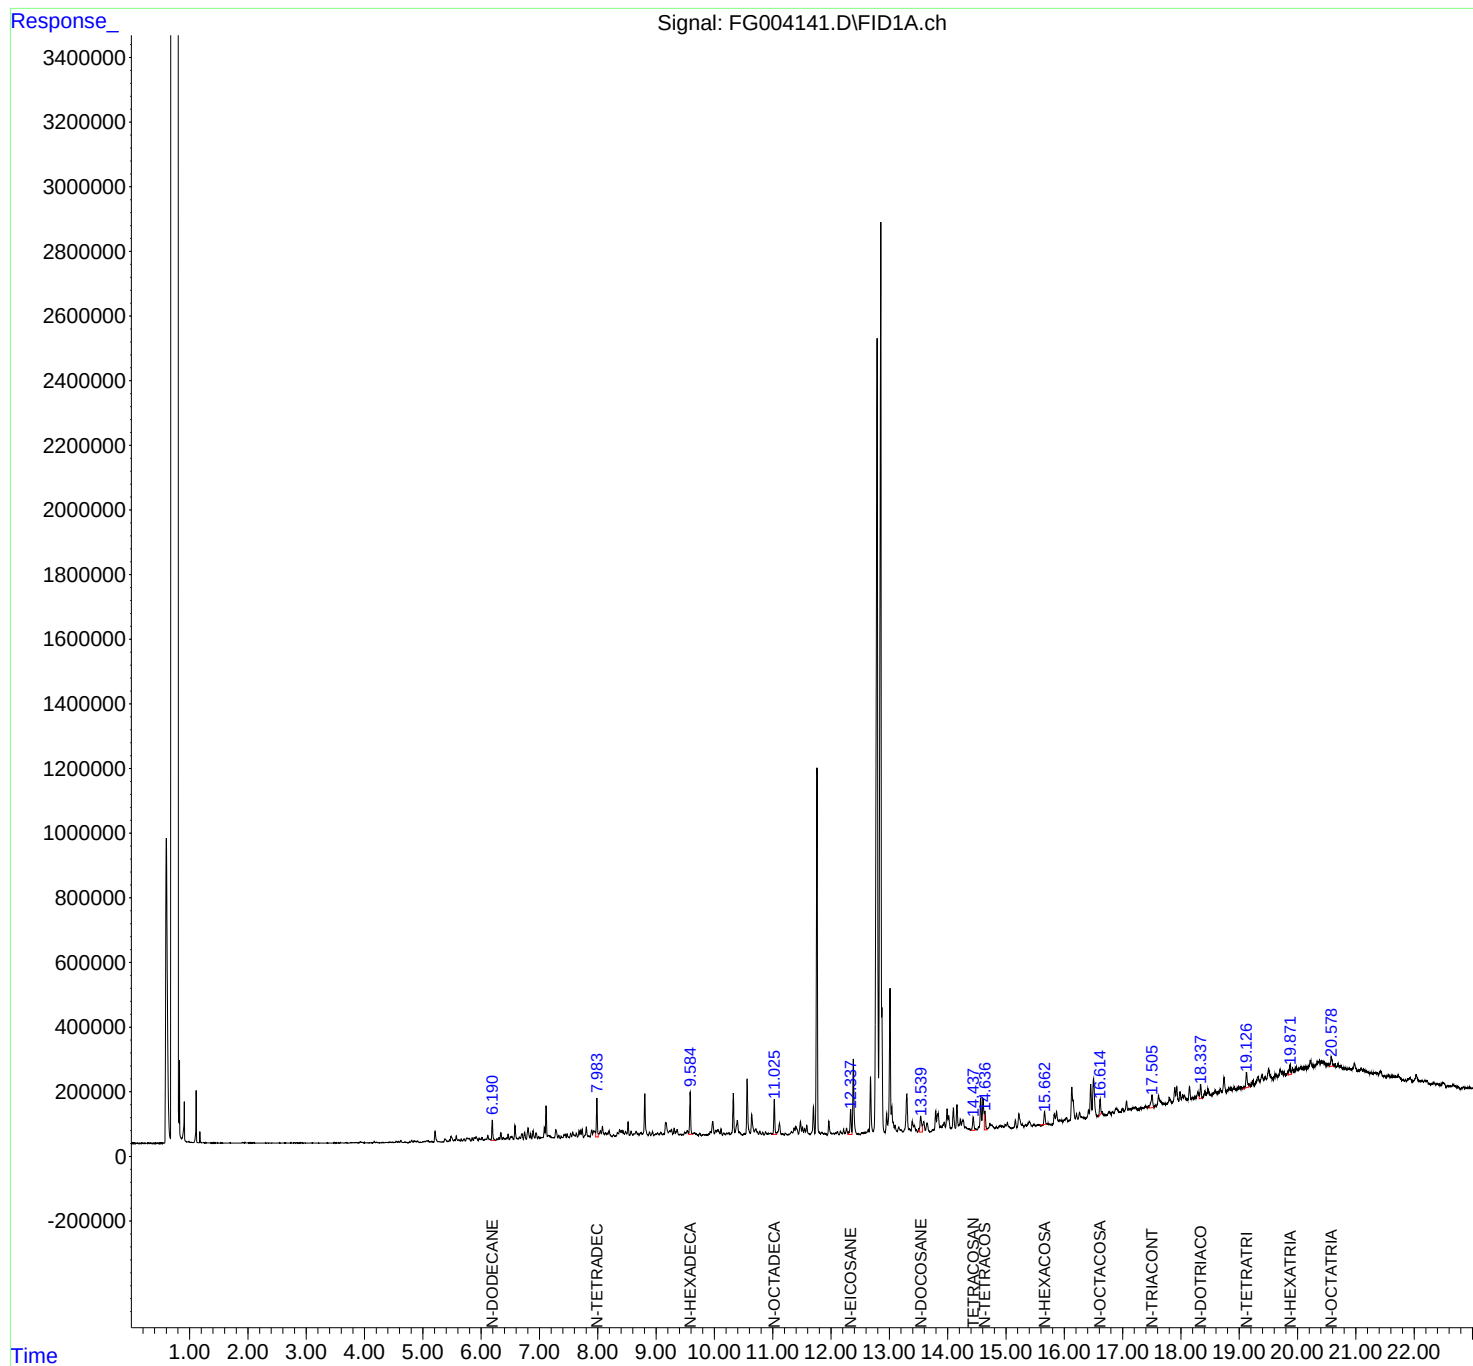


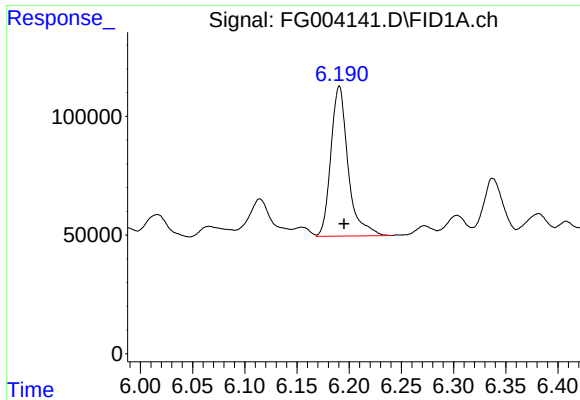

#3 N-DODECANE


R.T.: 6.191 min
Delta R.T.: -0.005 min
Response: 726687
Conc: 5.36 ug/ml

Instrument :
FID_G
ClientSampleId :

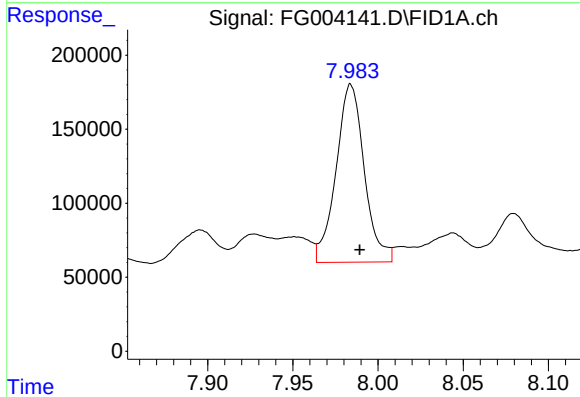


#4 N-TETRADECANE

R.T.: 7.984 min
Delta R.T.: -0.005 min
Response: 1386950
Conc: 9.95 ug/ml

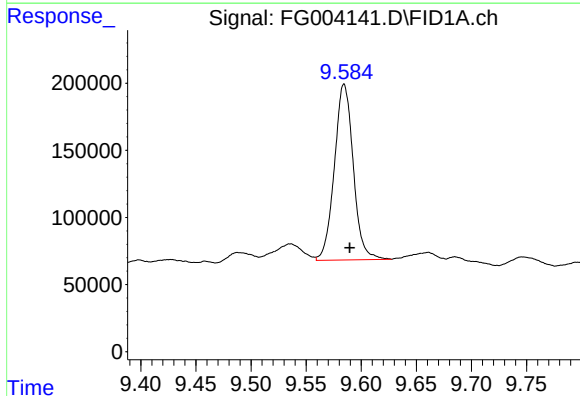


#5 N-HEXADECANE

R.T.: 9.584 min
Delta R.T.: -0.005 min
Response: 1564002
Conc: 10.99 ug/ml

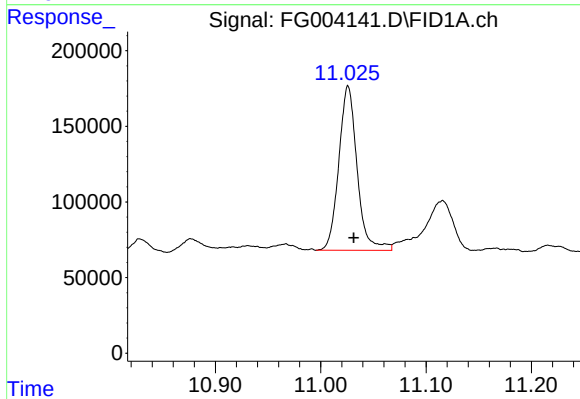

#6 N-OCTADECANE


R.T.: 11.026 min
Delta R.T.: -0.005 min
Response: 1313996
Conc: 9.16 ug/ml

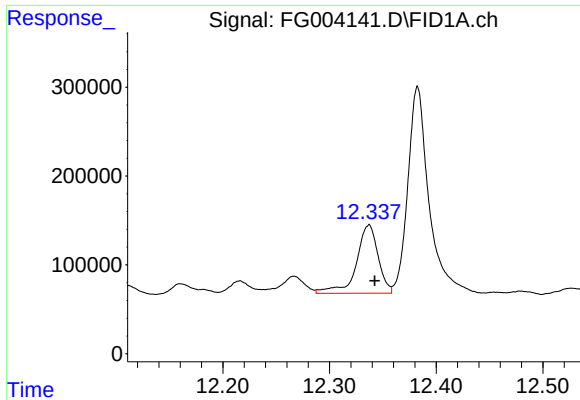

#7 N-EICOSANE


R.T.: 12.337 min
Delta R.T.: -0.006 min
Response: 1093380
Conc: 7.65 ug/ml

Instrument :
FID_G
ClientSampleId :

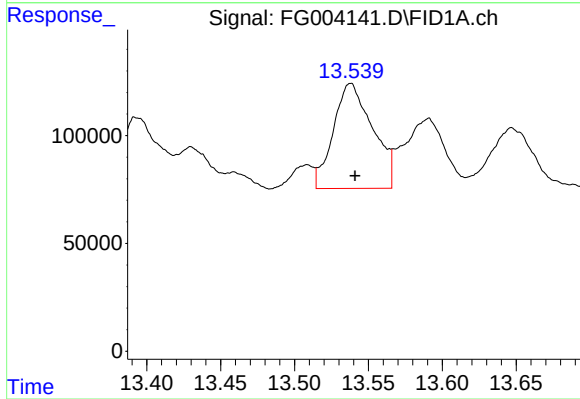


#8 N-DOCOSANE

R.T.: 13.538 min
Delta R.T.: -0.003 min
Response: 901879
Conc: 6.35 ug/ml

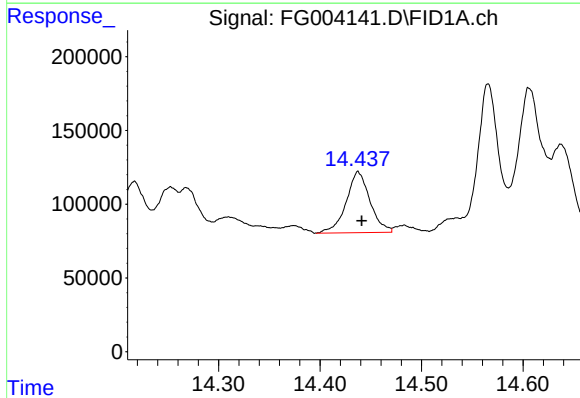


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.438 min
Delta R.T.: -0.004 min
Response: 674568
Conc: 5.37 ug/ml

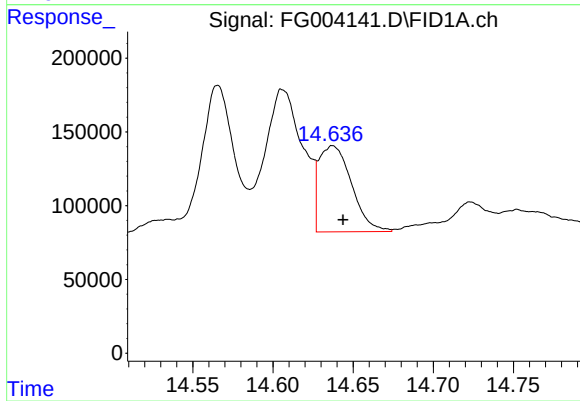

#10 N-TETRACOSANE


R.T.: 14.637 min
Delta R.T.: -0.006 min
Response: 827897
Conc: 5.87 ug/ml

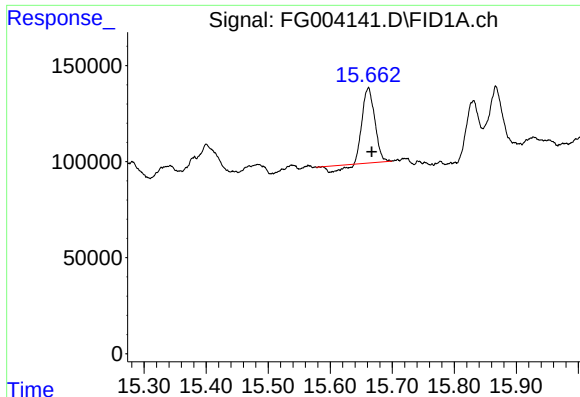

#11 N-HEXACOSANE


R.T.: 15.662 min
Delta R.T.: -0.005 min
Response: 501289
Conc: 3.60 ug/ml

Instrument :
FID_G
ClientSampleId :

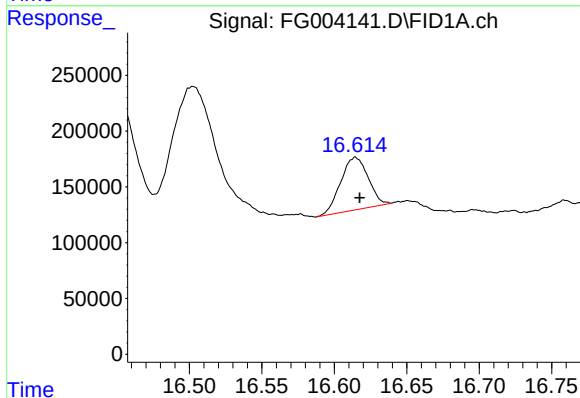


#12 N-OCTACOSANE

R.T.: 16.615 min
Delta R.T.: -0.003 min
Response: 619348
Conc: 4.52 ug/ml

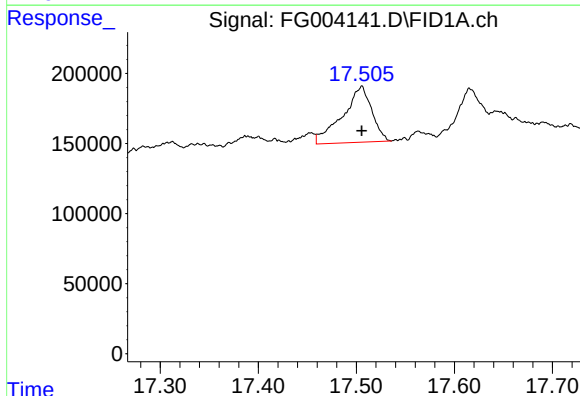


#13 N-TRIACONTANE

R.T.: 17.506 min
Delta R.T.: 0.000 min
Response: 825656
Conc: 6.18 ug/ml

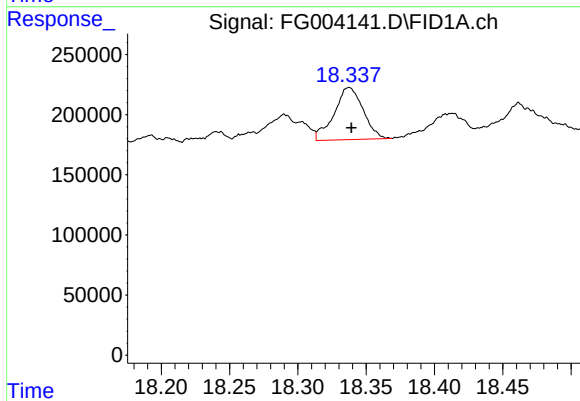

#14 N-DOTRIACONTANE


R.T.: 18.337 min
Delta R.T.: -0.002 min
Response: 640604
Conc: 5.06 ug/ml

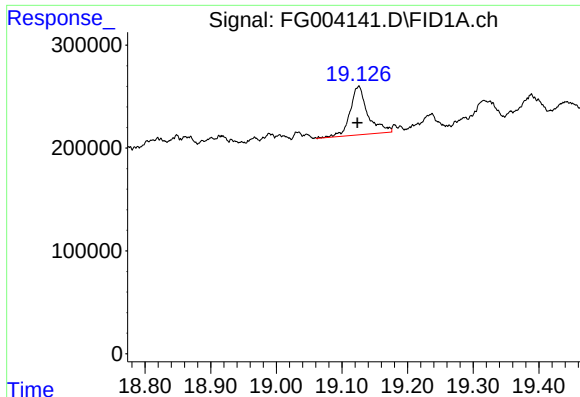

#15 N-TETRATRIACONTANE


R.T.: 19.126 min
Delta R.T.: 0.002 min
Response: 888656
Conc: 7.50 ug/ml

Instrument :
FID_G
ClientSampleId :

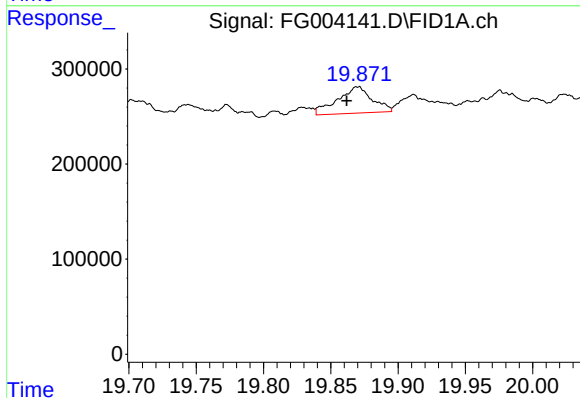

#16 N-HEXATRIACONTANE

R.T.: 19.870 min
Delta R.T.: 0.008 min
Response: 497134
Conc: 4.49 ug/ml

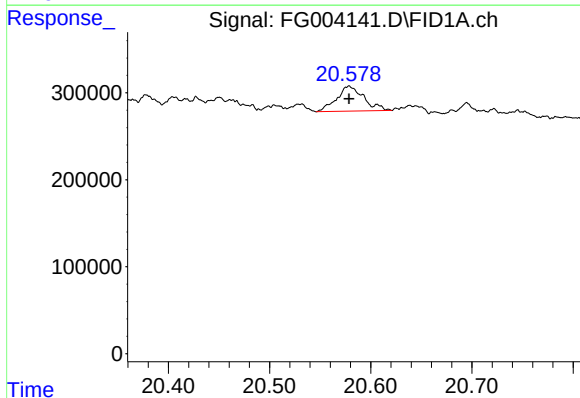

#17 N-OCTATRIACONTANE

R.T.: 20.579 min
Delta R.T.: 0.000 min
Response: 536435
Conc: 5.31 ug/ml