

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031219\
 Data File : FG004152.D
 Signal(s) : FID1A.ch
 Acq On : 13 Mar 2019 01:14
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 13 02:06:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
 Quant Title :
 QLast Update : Tue Mar 05 03:05:54 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.436	2270012	18.056 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.500	279758	2.095 ug/ml
14) N-DOTRIACONTANE	18.333	110645	0.874 ug/ml
16) N-HEXATRIACONTANE	19.859	294345	2.659 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG031219\
Data File : FG004152.D
Signal(s) : FID1A.ch
Acq On : 13 Mar 2019 01:14
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 13 02:06:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG030419.M
Quant Title :
QLast Update : Tue Mar 05 03:05:54 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

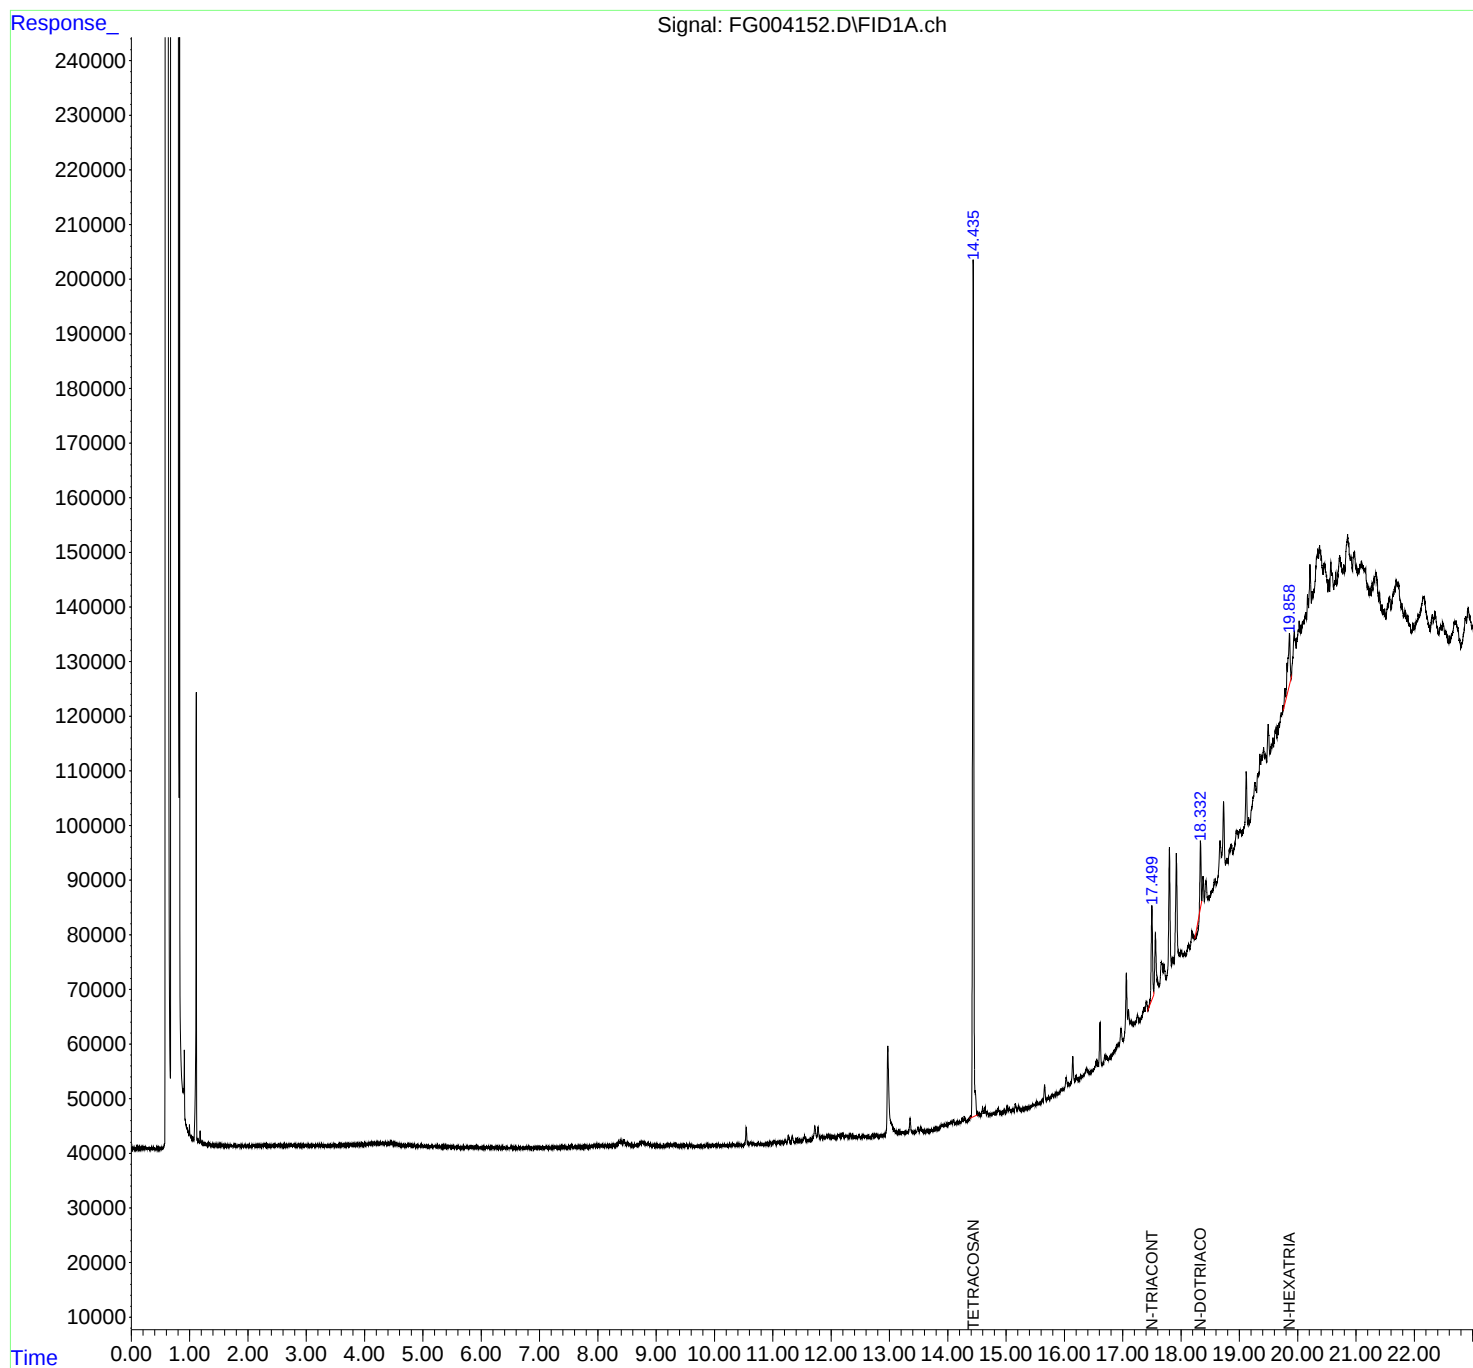


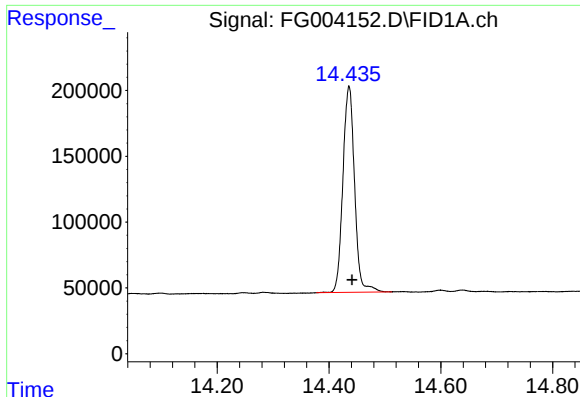

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.436 min
Delta R.T.: -0.005 min
Response: 2270012
Conc: 18.06 ug/ml

Instrument :
FID_G
ClientSampleId :

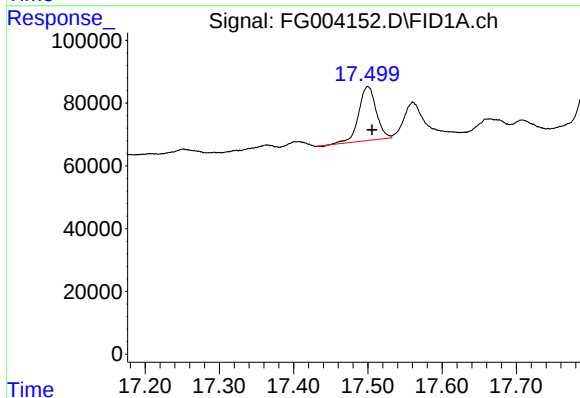


#13 N-TRIACONTANE

R.T.: 17.500 min
Delta R.T.: -0.006 min
Response: 279758
Conc: 2.09 ug/ml

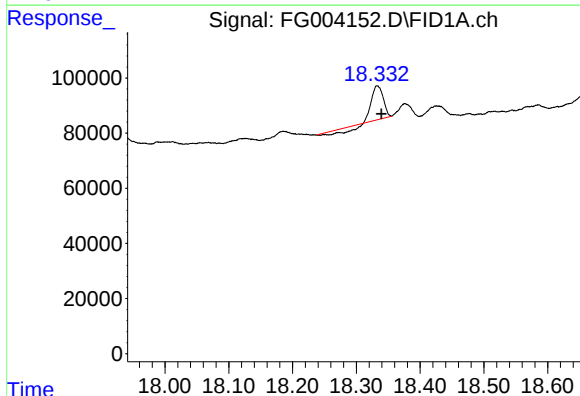

#14 N-DOTRIACONTANE

R.T.: 18.333 min
Delta R.T.: -0.006 min
Response: 110645
Conc: 0.87 ug/ml

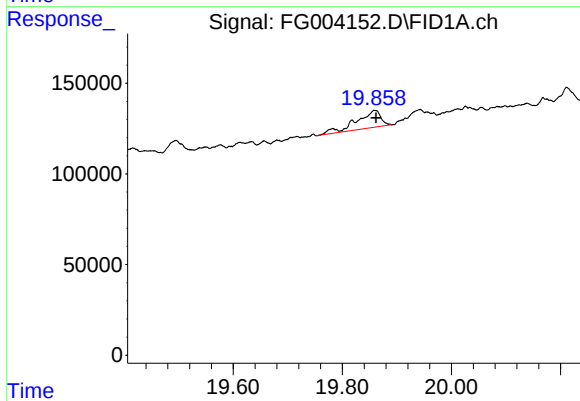

#16 N-HEXATRIACONTANE

R.T.: 19.859 min
Delta R.T.: -0.003 min
Response: 294345
Conc: 2.66 ug/ml