

Data Path : P:\HPCHEM1\FID_G\Data\FG031318\
 Data File : FG000374.D
 Signal(s) : FID1A.ch
 Acq On : 13 Mar 2018 15:30
 Operator : UA\AJ
 Sample : J1753-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 14 04:00:46 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FG022818.M
 Quant Title :
 QLast Update : Wed Feb 28 18:10:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.573	3124673	28.112 ug/ml
Target Compounds			
4) N-TETRADECANE	8.177f	405058	2.946 ug/ml
5) N-HEXADECANE	9.722	170828	1.291 ug/ml
12) N-OCTACOSANE	16.748	163337	1.377 ug/ml
13) N-TRIACONTANE	17.636	197742	1.714 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_G\Data\FG031318\
Data File : FG000374.D
Signal(s) : FID1A.ch
Acq On : 13 Mar 2018 15:30
Operator : UA\AJ
Sample : J1753-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 14 04:00:46 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FG022818.M
Quant Title :
QLast Update : Wed Feb 28 18:10:38 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

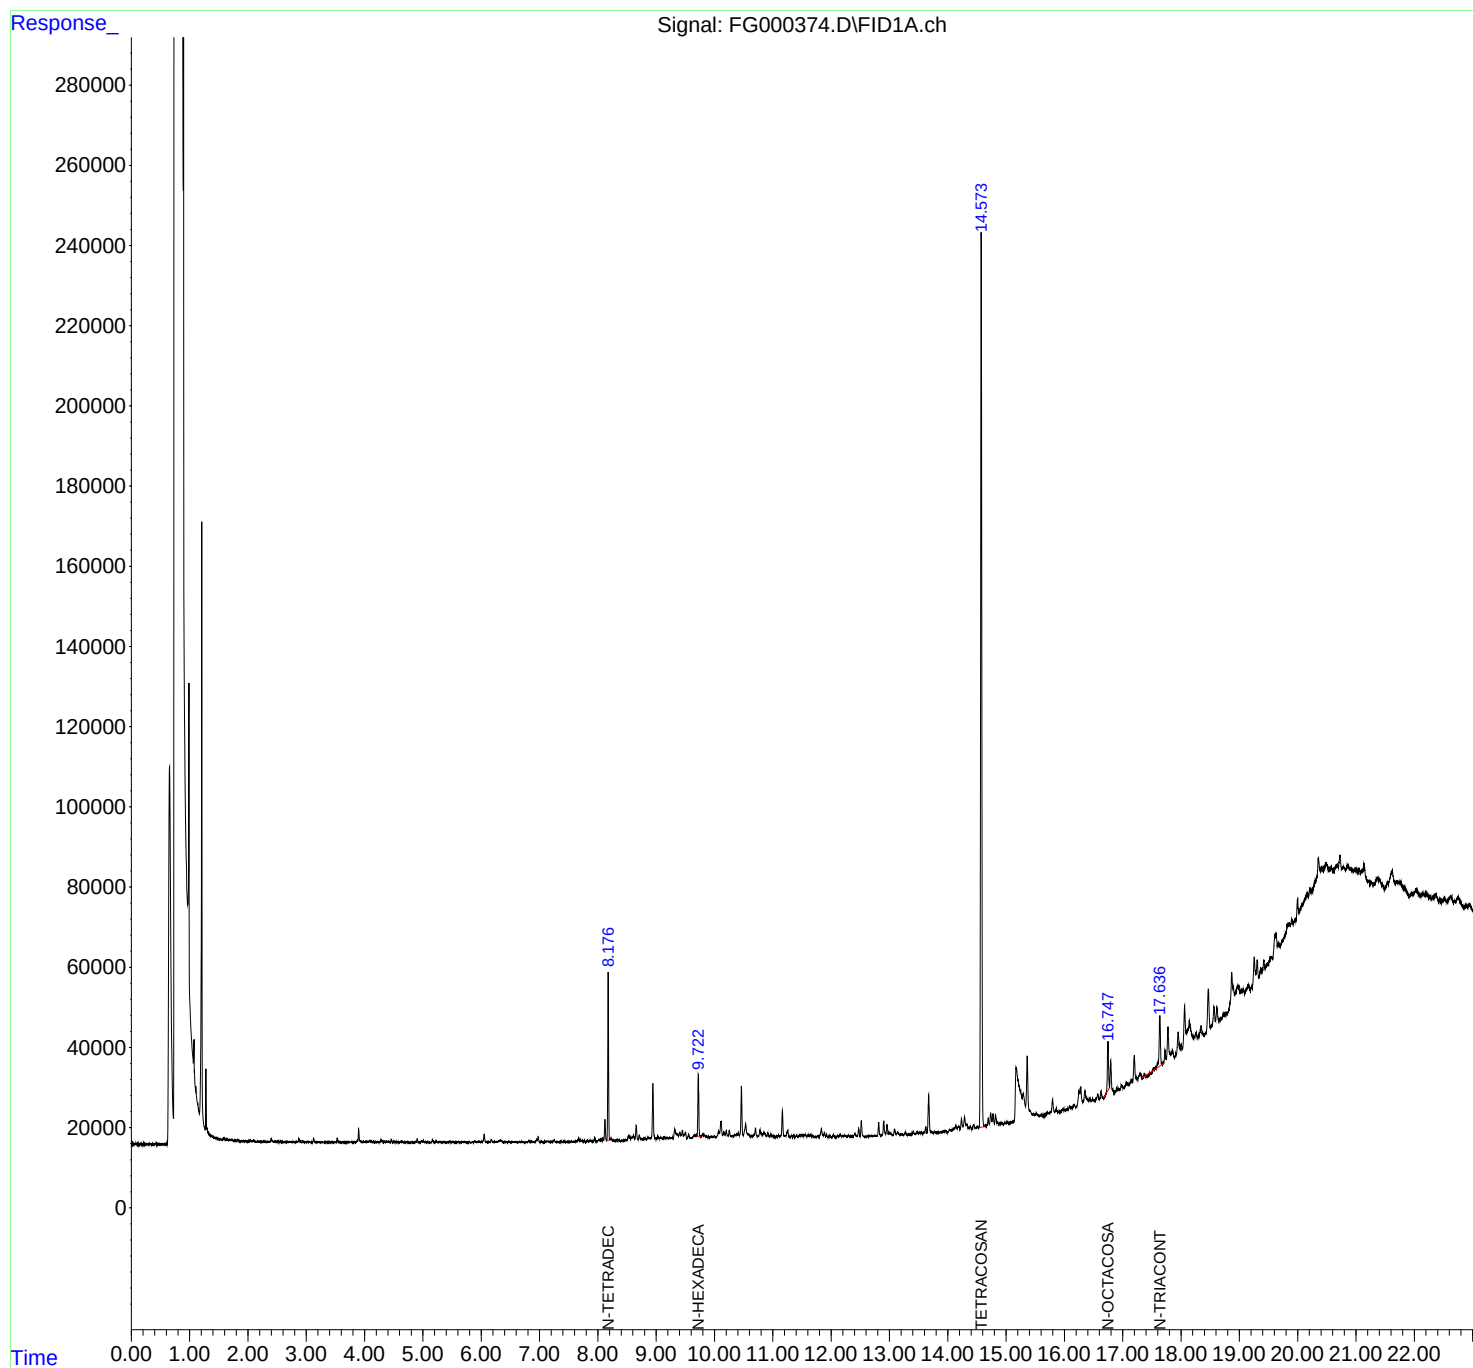


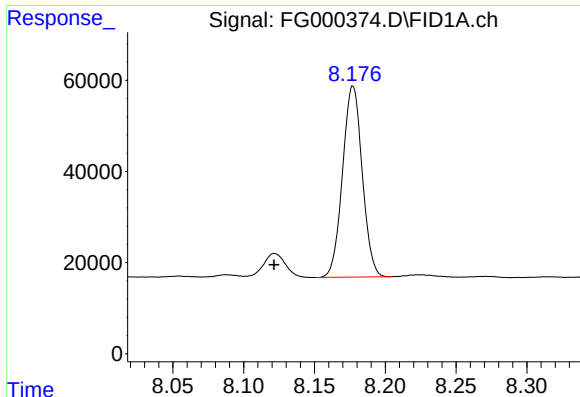

#4 N-TETRADECANE


R.T.: 8.177 min
Delta R.T.: 0.056 min
Response: 405058
Conc: 2.95 ug/ml

Instrument :
FID_G
ClientSampleId :

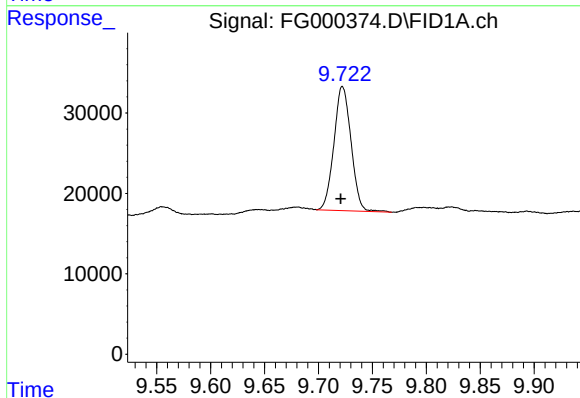


#5 N-HEXADECANE

R.T.: 9.722 min
Delta R.T.: 0.002 min
Response: 170828
Conc: 1.29 ug/ml

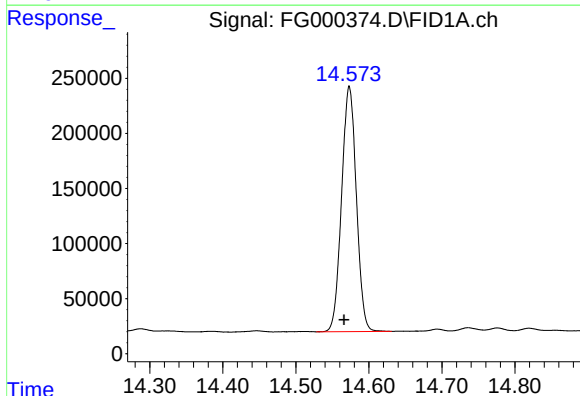


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.573 min
Delta R.T.: 0.007 min
Response: 3124673
Conc: 28.11 ug/ml

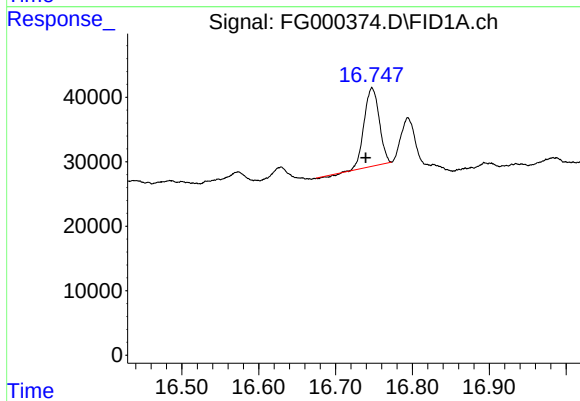

#12 N-OCTACOSANE

R.T.: 16.748 min
Delta R.T.: 0.008 min
Response: 163337
Conc: 1.38 ug/ml

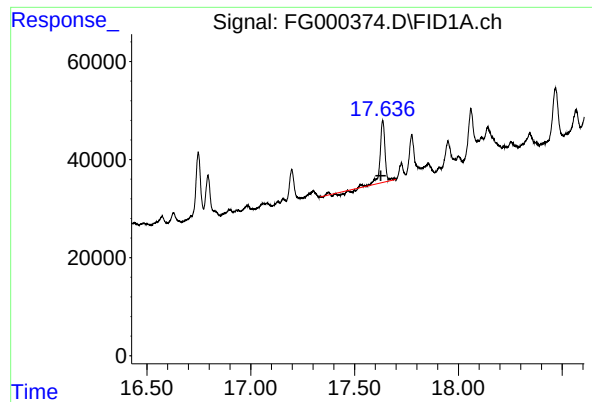

#13 N-TRIACONTANE

R.T.: 17.636 min
Delta R.T.: 0.009 min
Response: 197742
Conc: 1.71 ug/ml

Instrument :
FID_G
ClientSampleId :