

Data Path : P:\HPCHEM1\FID_G\Data\FG031918\
 Data File : FG000481.D
 Signal(s) : FID1A.ch
 Acq On : 19 Mar 2018 20:59
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 20 07:46:44 2018
 Quant Method : P:\HPCHEM1\FID_G\Method\FG031618.M
 Quant Title :
 QLast Update : Fri Mar 16 13:10:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.574	7787433	44.376 ug/mlm
Target Compounds			
2) N-DECANE	4.304	6042113	60.307 ug/ml
3) N-DODECANE	6.329	7175965	62.370 ug/ml
4) N-TETRADECANE	8.125	8234602	59.074 ug/ml
5) N-HEXADECANE	9.726	8746075	55.070 ug/ml
6) N-OCTADECANE	11.167	9114200	51.410 ug/ml
7) N-EICOSANE	12.477	9218914	50.191 ug/ml
8) N-DOCOSANE	13.675	9028448	48.062 ug/ml
10) N-TETRACOSANE	14.778	8704223	43.611 ug/ml
11) N-HEXACOSANE	15.798	7526996	39.011 ug/ml
12) N-OCTACOSANE	16.749	6839709	35.640 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : P:\HPCHEM1\FID_G\Data\FG031918\
Data File : FG000481.D
Signal(s) : FID1A.ch
Acq On : 19 Mar 2018 20:59
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 20 07:46:44 2018
Quant Method : P:\HPCHEM1\FID_G\Method\FG031618.M
Quant Title :
QLast Update : Fri Mar 16 13:10:14 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

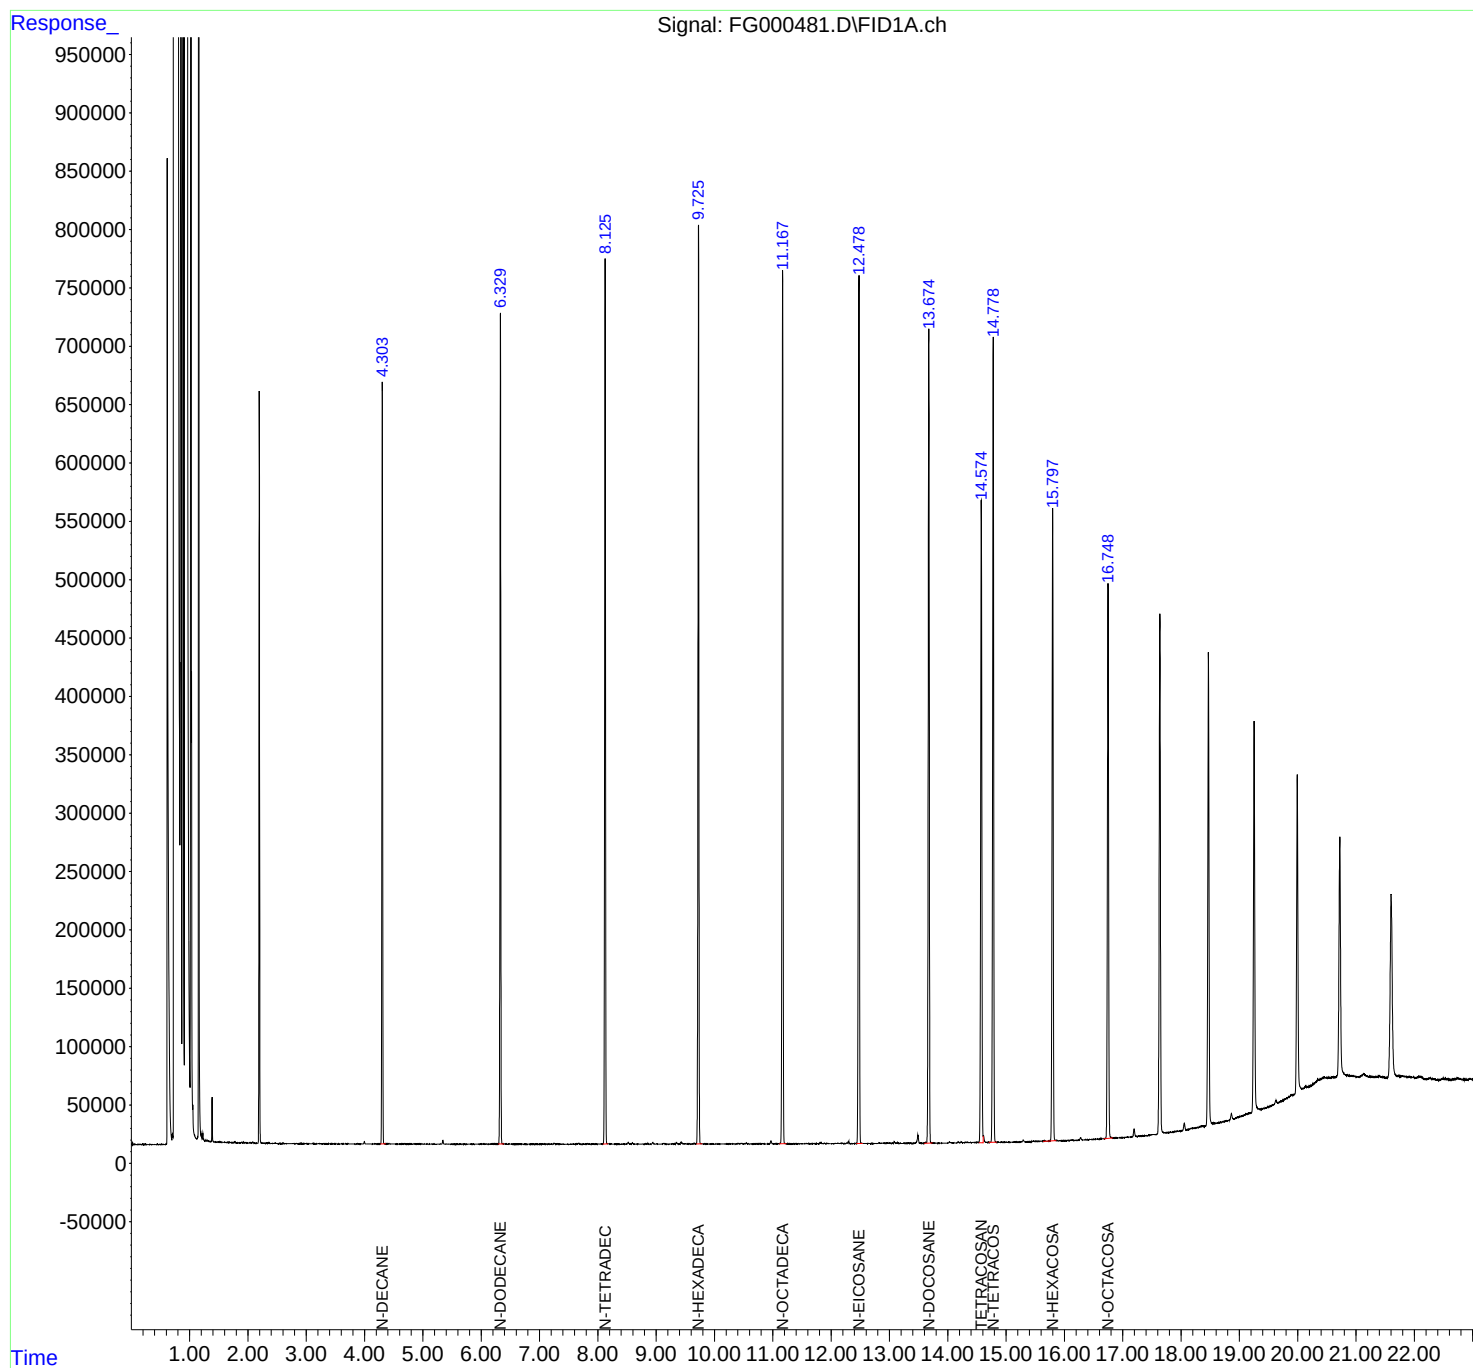

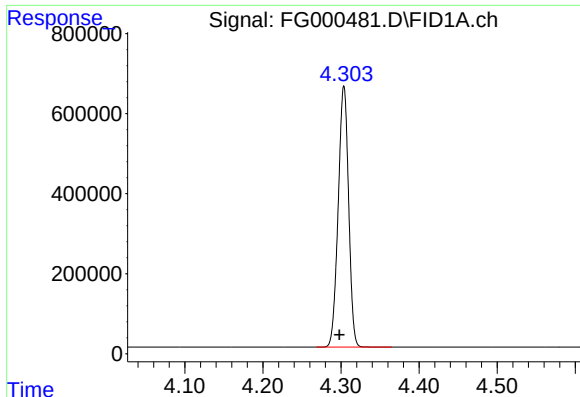


#2 N-DECANE

R.T.: 4.304 min
Delta R.T.: 0.006 min
Response: 6042113
Conc: 60.31 ug/ml

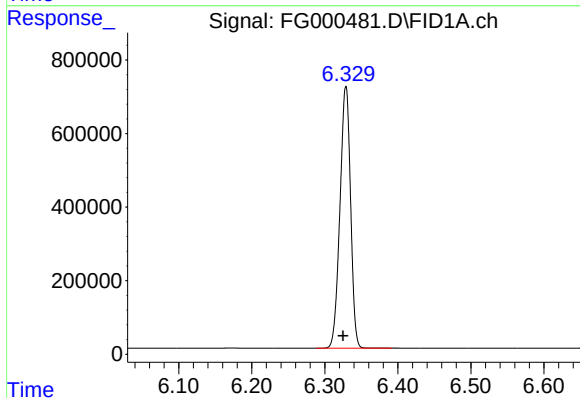


#3 N-DODECANE

R.T.: 6.329 min
Delta R.T.: 0.004 min
Response: 7175965
Conc: 62.37 ug/ml

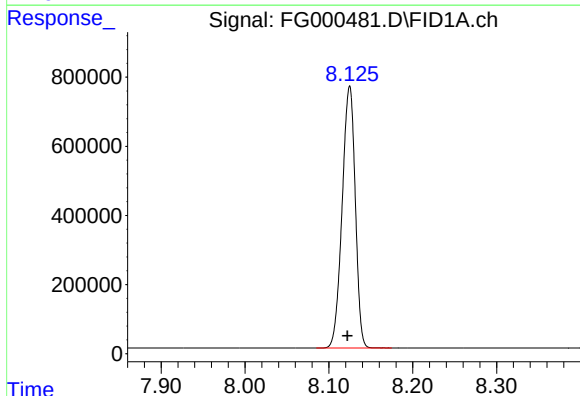


#4 N-TETRADECANE

R.T.: 8.125 min
Delta R.T.: 0.002 min
Response: 8234602
Conc: 59.07 ug/ml

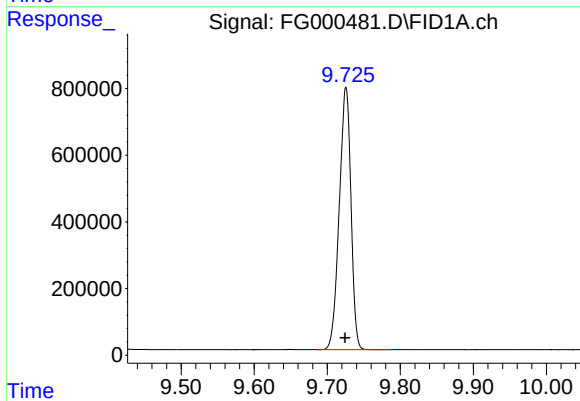


#5 N-HEXADECANE

R.T.: 9.726 min
Delta R.T.: 0.001 min
Response: 8746075
Conc: 55.07 ug/ml

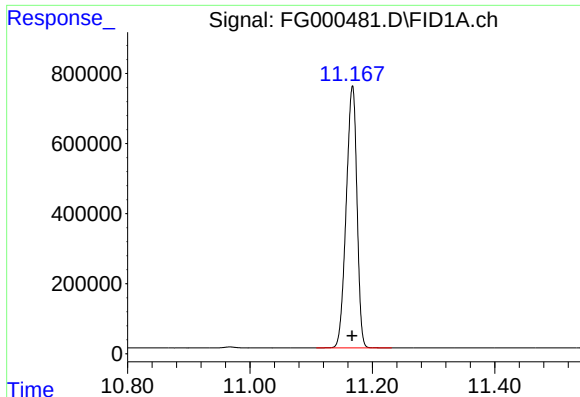


#6 N-OCTADECANE

R.T.: 11.167 min
Delta R.T.: 0.000 min
Response: 9114200
Conc: 51.41 ug/ml

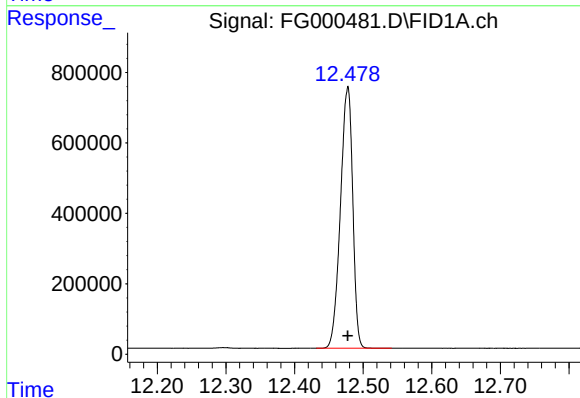


#7 N-EICOSANE

R.T.: 12.477 min
Delta R.T.: 0.000 min
Response: 9218914
Conc: 50.19 ug/ml

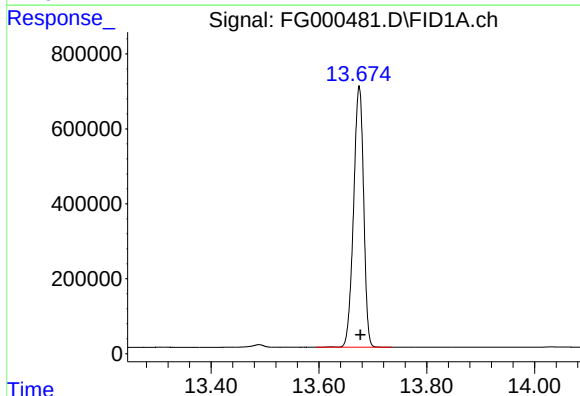


#8 N-DOCOSANE

R.T.: 13.675 min
Delta R.T.: -0.003 min
Response: 9028448
Conc: 48.06 ug/ml

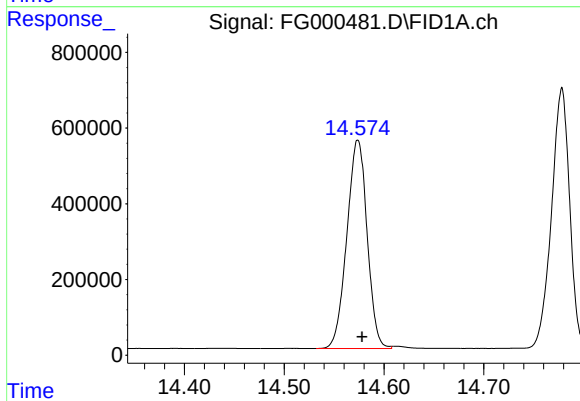


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.574 min
Delta R.T.: -0.005 min
Response: 7787433
Conc: 44.38 ug/ml m

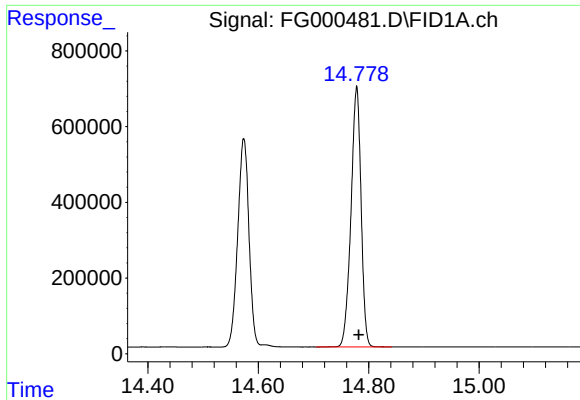


#10 N-TETRACOSANE

R.T.: 14.778 min
Delta R.T.: -0.004 min
Response: 8704223
Conc: 43.61 ug/ml

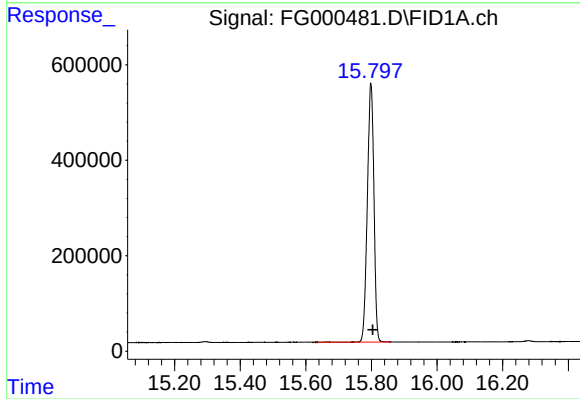

#11 N-HEXACOSANE

R.T.: 15.798 min
Delta R.T.: -0.006 min
Response: 7526996
Conc: 39.01 ug/ml

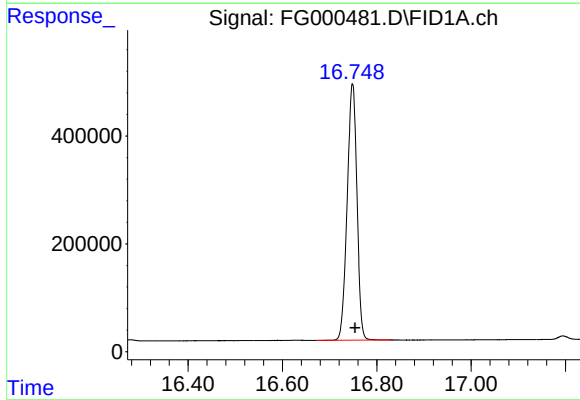

#12 N-OCTACOSANE

R.T.: 16.749 min
Delta R.T.: -0.006 min
Response: 6839709
Conc: 35.64 ug/ml