

Data Path : P:\HPCHEM1\FID_G\Data\FG032218\
 Data File : FG000487.D
 Signal(s) : FID1A.ch
 Acq On : 22 Mar 2018 10:16
 Operator : UA\AJ
 Sample : J1974-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 22 10:42:44 2018
 Quant Method : P:\HPCHEM1\FID_G\Method\FG031618.M
 Quant Title :
 QLast Update : Fri Mar 16 13:10:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.572	3082532	18.237 ug/ml
Target Compounds			
4) N-TETRADECANE	8.176f	643352	4.805 ug/ml
5) N-HEXADECANE	9.721	390707	2.528 ug/ml
7) N-EICOSANE	12.517	367959	2.032 ug/ml
10) N-TETRACOSANE	14.732	317702	1.657 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_G\Data\FG032218\
Data File : FG000487.D
Signal(s) : FID1A.ch
Acq On : 22 Mar 2018 10:16
Operator : UA\AJ
Sample : J1974-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 22 10:42:44 2018
Quant Method : P:\HPCHEM1\FID_G\Method\FG031618.M
Quant Title :
QLast Update : Fri Mar 16 13:10:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

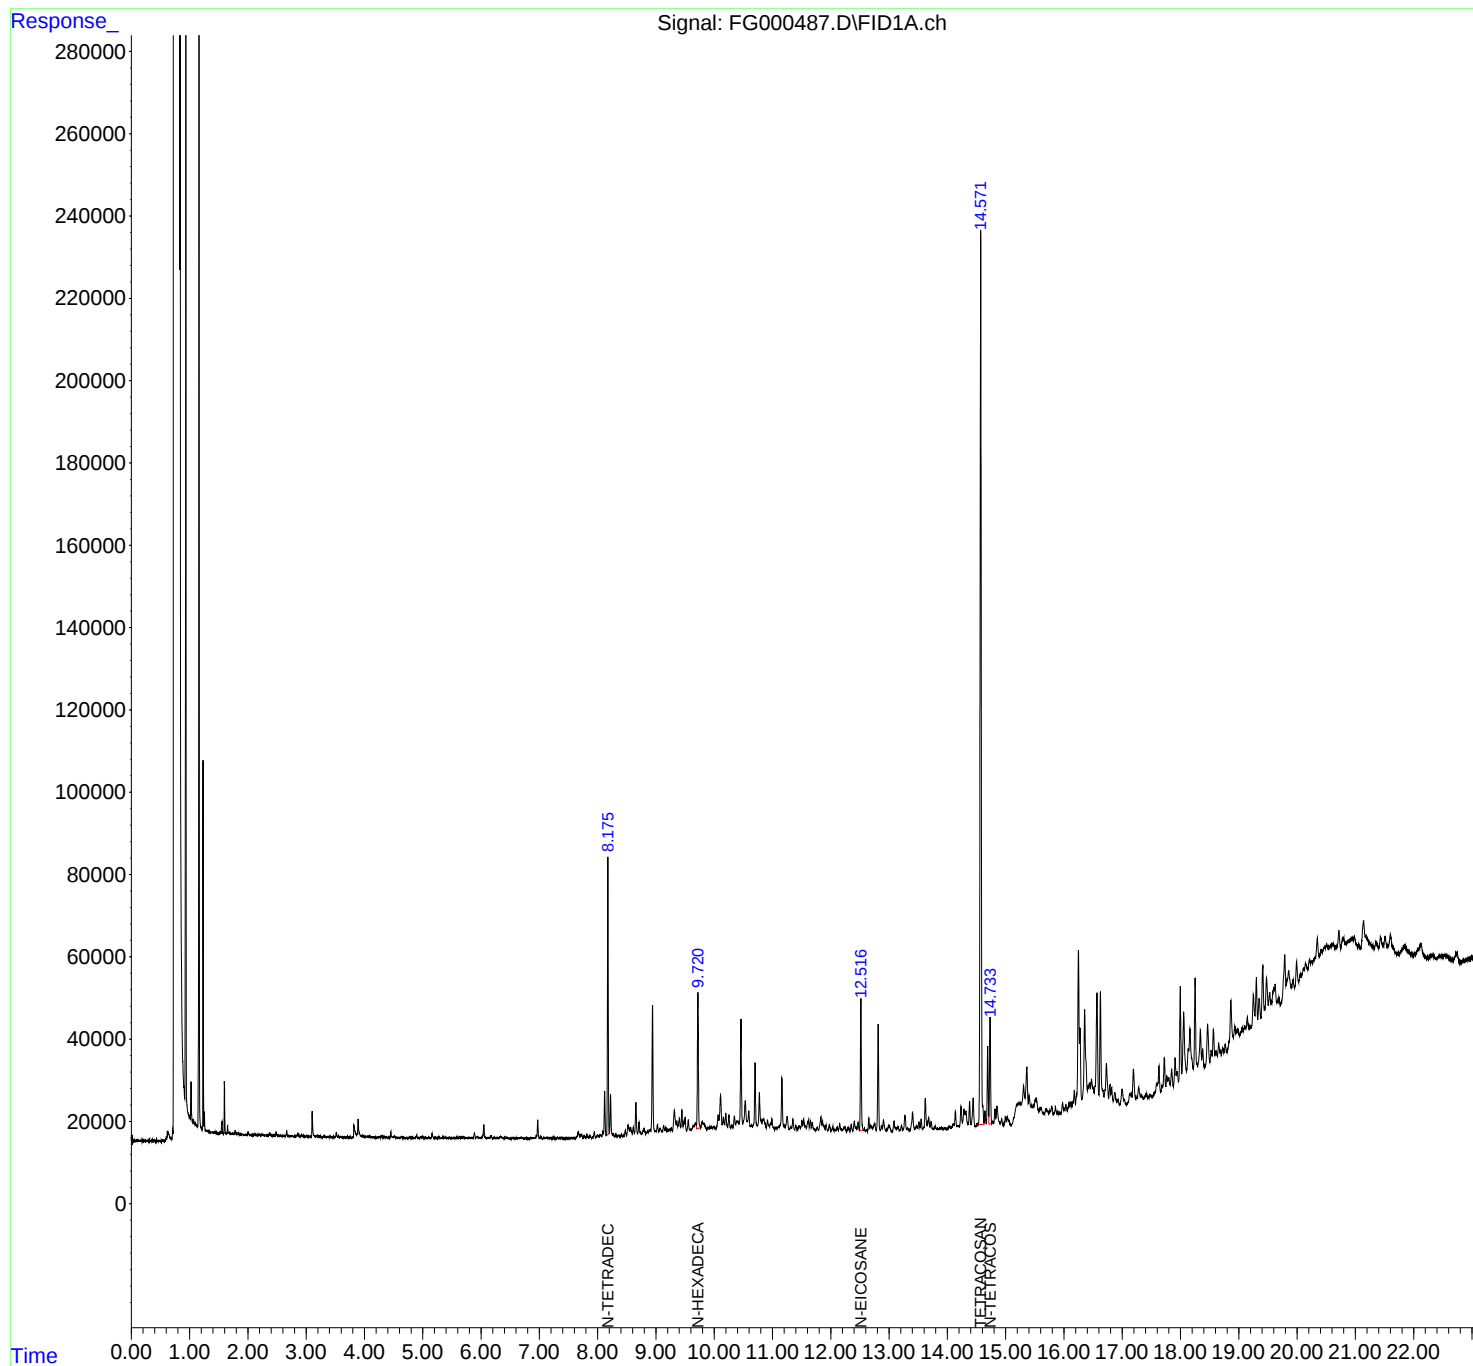


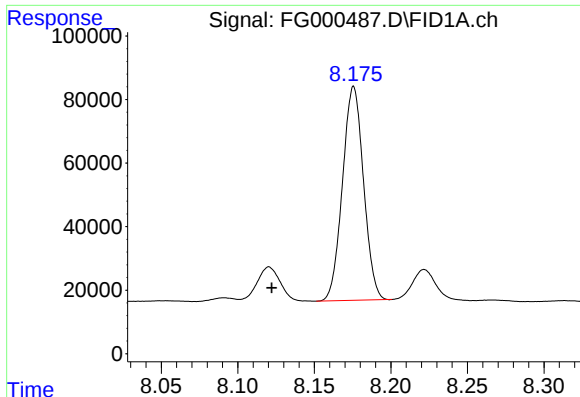

#4 N-TETRADECANE


R.T.: 8.176 min
Delta R.T.: 0.053 min
Response: 643352
Conc: 4.80 ug/ml

Instrument :
FID_G
ClientSampleId :

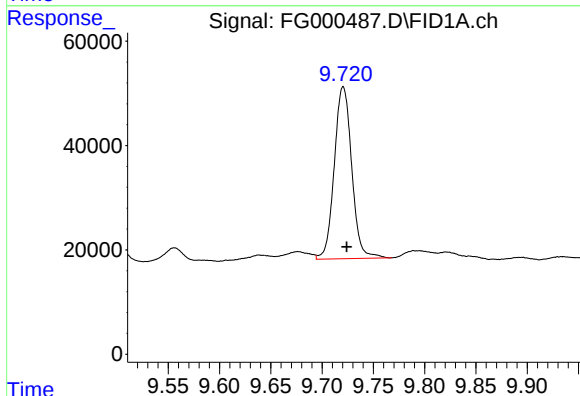


#5 N-HEXADECANE

R.T.: 9.721 min
Delta R.T.: -0.004 min
Response: 390707
Conc: 2.53 ug/ml

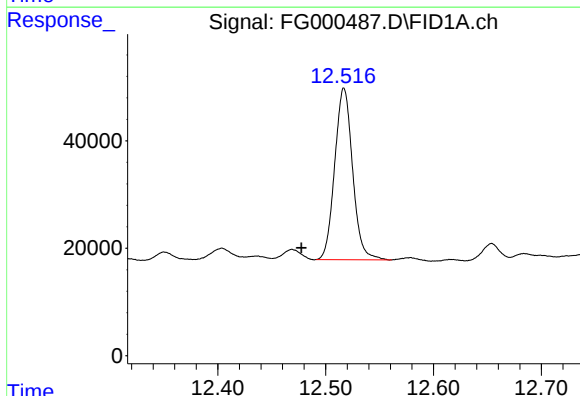


#7 N-EICOSANE

R.T.: 12.517 min
Delta R.T.: 0.039 min
Response: 367959
Conc: 2.03 ug/ml

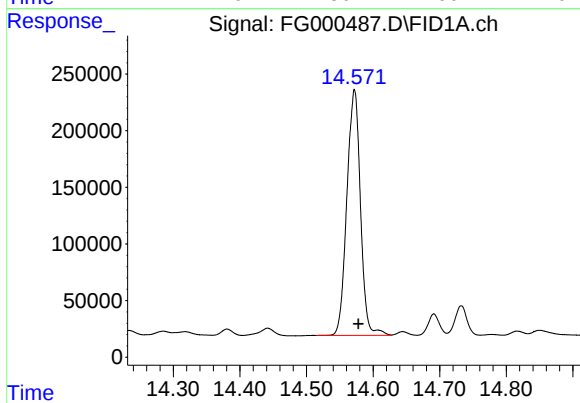

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.572 min
Delta R.T.: -0.006 min
Response: 3082532
Conc: 18.24 ug/ml

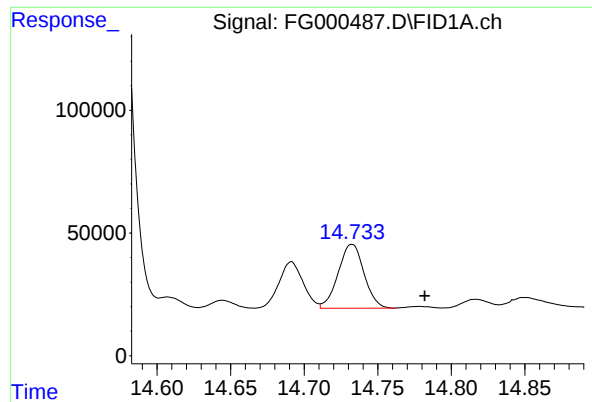

#10 N-TETRACOSANE

R.T.: 14.732 min
Delta R.T.: -0.049 min
Response: 317702
Conc: 1.66 ug/ml

Instrument :
FID_G
ClientSampleId :