

Data Path : P:\HPCHEM1\FID_G\Data\FG032218\
Data File : FG000498.D
Signal(s) : FID1A.ch
Acq On : 22 Mar 2018 15:34
Operator : UA\AJ
Sample : J1983-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 23 04:54:37 2018
Quant Method : P:\HPCHEM1\FID_G\Method\FG031618.M
Quant Title :
QLast Update : Fri Mar 16 13:10:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.571	3294770	18.775 ug/ml
Target Compounds				
4)	N-TETRADECANE	8.175f	539529	3.871 ug/ml
5)	N-HEXADECANE	9.720	297935	1.876 ug/ml
7)	N-EICOSANE	12.523	246138	1.340 ug/ml
10)	N-TETRACOSANE	14.760	1484651	7.439 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_G\Data\FG032218\
Data File : FG000498.D
Signal(s) : FID1A.ch
Acq On : 22 Mar 2018 15:34
Operator : UA\AJ
Sample : J1983-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 23 04:54:37 2018
Quant Method : P:\HPCHEM1\FID_G\Method\FG031618.M
Quant Title :
QLast Update : Fri Mar 16 13:10:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

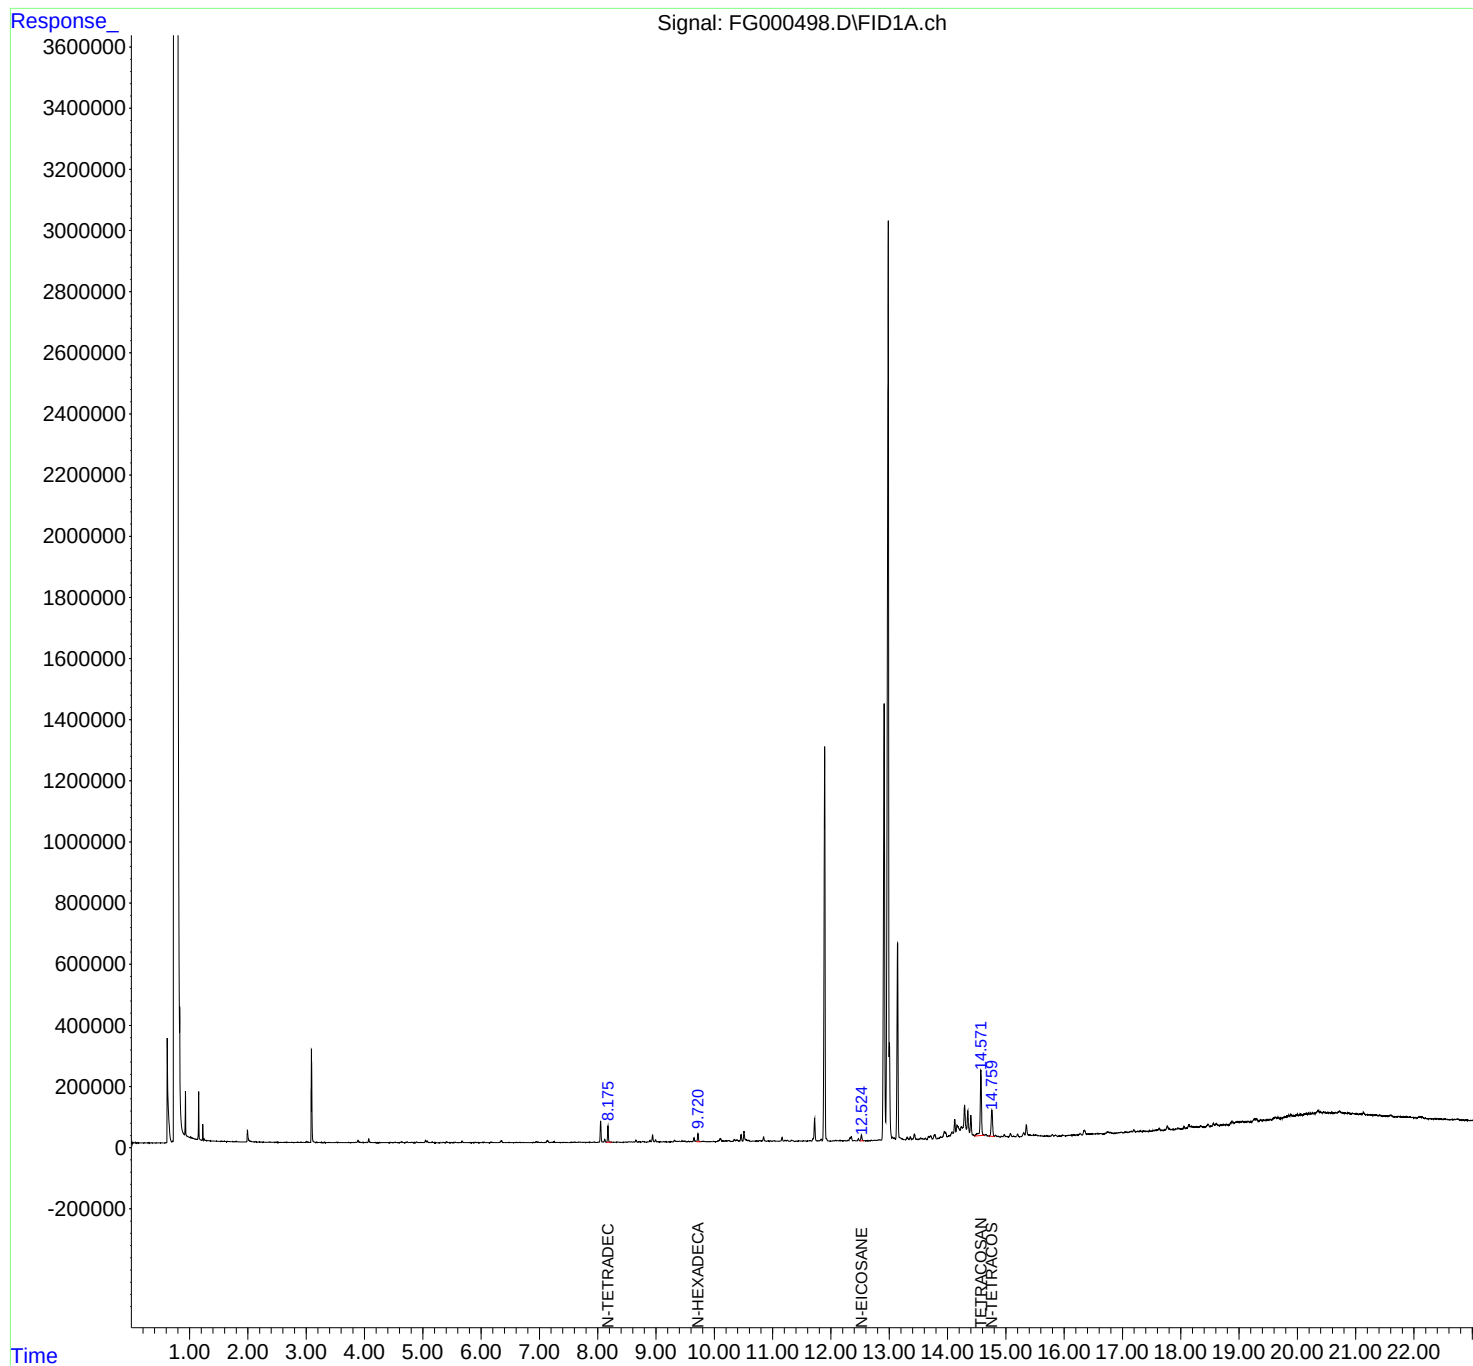


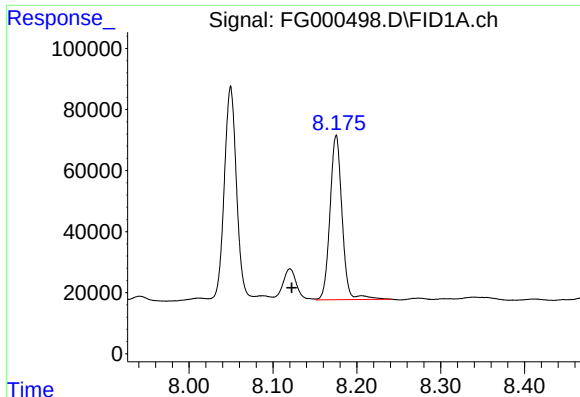

#4 N-TETRADECANE


R.T.: 8.175 min
Delta R.T.: 0.053 min
Response: 539529
Conc: 3.87 ug/ml

Instrument :
FID_G
ClientSampleId :

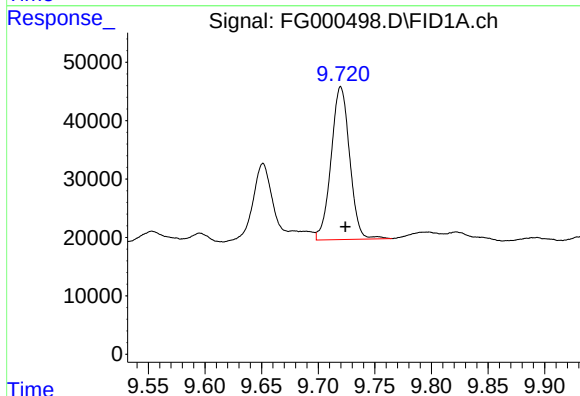


#5 N-HEXADECANE

R.T.: 9.720 min
Delta R.T.: -0.004 min
Response: 297935
Conc: 1.88 ug/ml

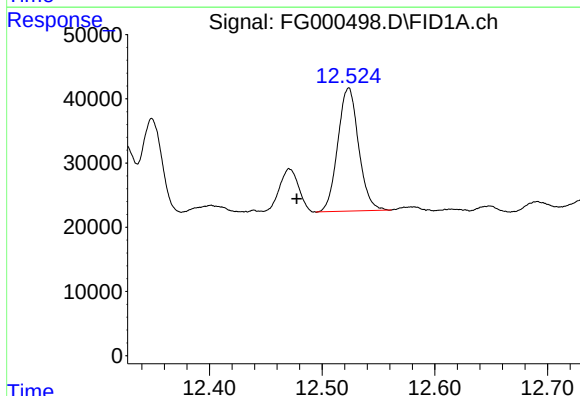


#7 N-EICOSANE

R.T.: 12.523 min
Delta R.T.: 0.046 min
Response: 246138
Conc: 1.34 ug/ml

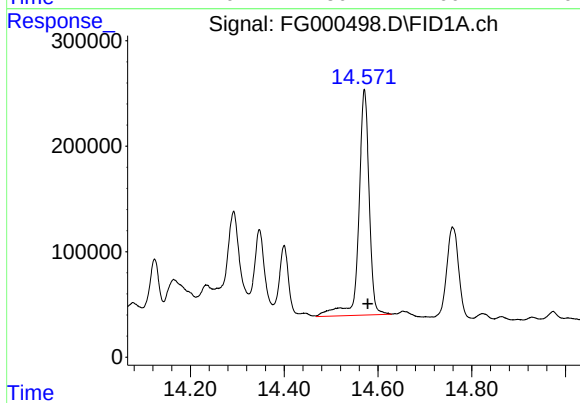

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.571 min
Delta R.T.: -0.007 min
Response: 3294770
Conc: 18.78 ug/ml

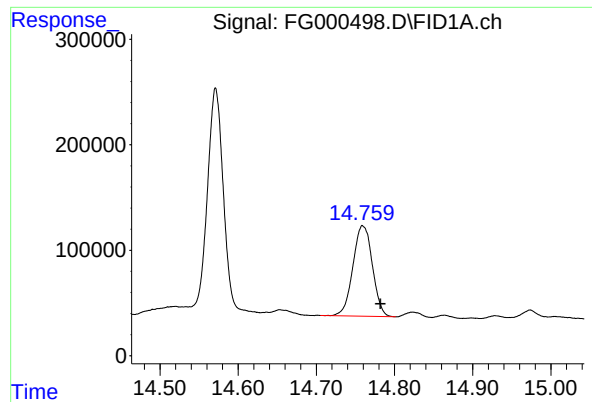

#10 N-TETRACOSANE

R.T.: 14.760 min
Delta R.T.: -0.022 min
Response: 1484651
Conc: 7.44 ug/ml

Instrument :
FID_G
ClientSampleId :