

Data Path : P:\HPCHEM1\FID_G\Data\FG032218\
 Data File : FG000497.D
 Signal(s) : FID1A.ch
 Acq On : 22 Mar 2018 15:05
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 22 15:28:58 2018
 Quant Method : P:\HPCHEM1\FID_G\Method\FG031618.M
 Quant Title :
 QLast Update : Fri Mar 16 13:10:14 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.573	8315943	49.200 ug/ml
Target Compounds			
2) N-DECANE	4.304	6466240	65.471 ug/ml
3) N-DODECANE	6.329	7547235	67.821 ug/ml
4) N-TETRADECANE	8.125	8545454	63.818 ug/ml
5) N-HEXADECANE	9.725	9013934	58.328 ug/ml
6) N-OCTADECANE	11.167	9343783	52.390 ug/ml
7) N-EICOSANE	12.477	9465969	52.272 ug/ml
8) N-DOCOSANE	13.675	9414025	51.830 ug/ml
10) N-TETRACOSANE	14.778	9321519	48.621 ug/ml
11) N-HEXACOSANE	15.799	8164479	44.508 ug/ml
12) N-OCTACOSANE	16.749	7335488	40.754 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_G\Data\FG032218\
Data File : FG000497.D
Signal(s) : FID1A.ch
Acq On : 22 Mar 2018 15:05
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 22 15:28:58 2018
Quant Method : P:\HPCHEM1\FID_G\Method\FG031618.M
Quant Title :
QLast Update : Fri Mar 16 13:10:14 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

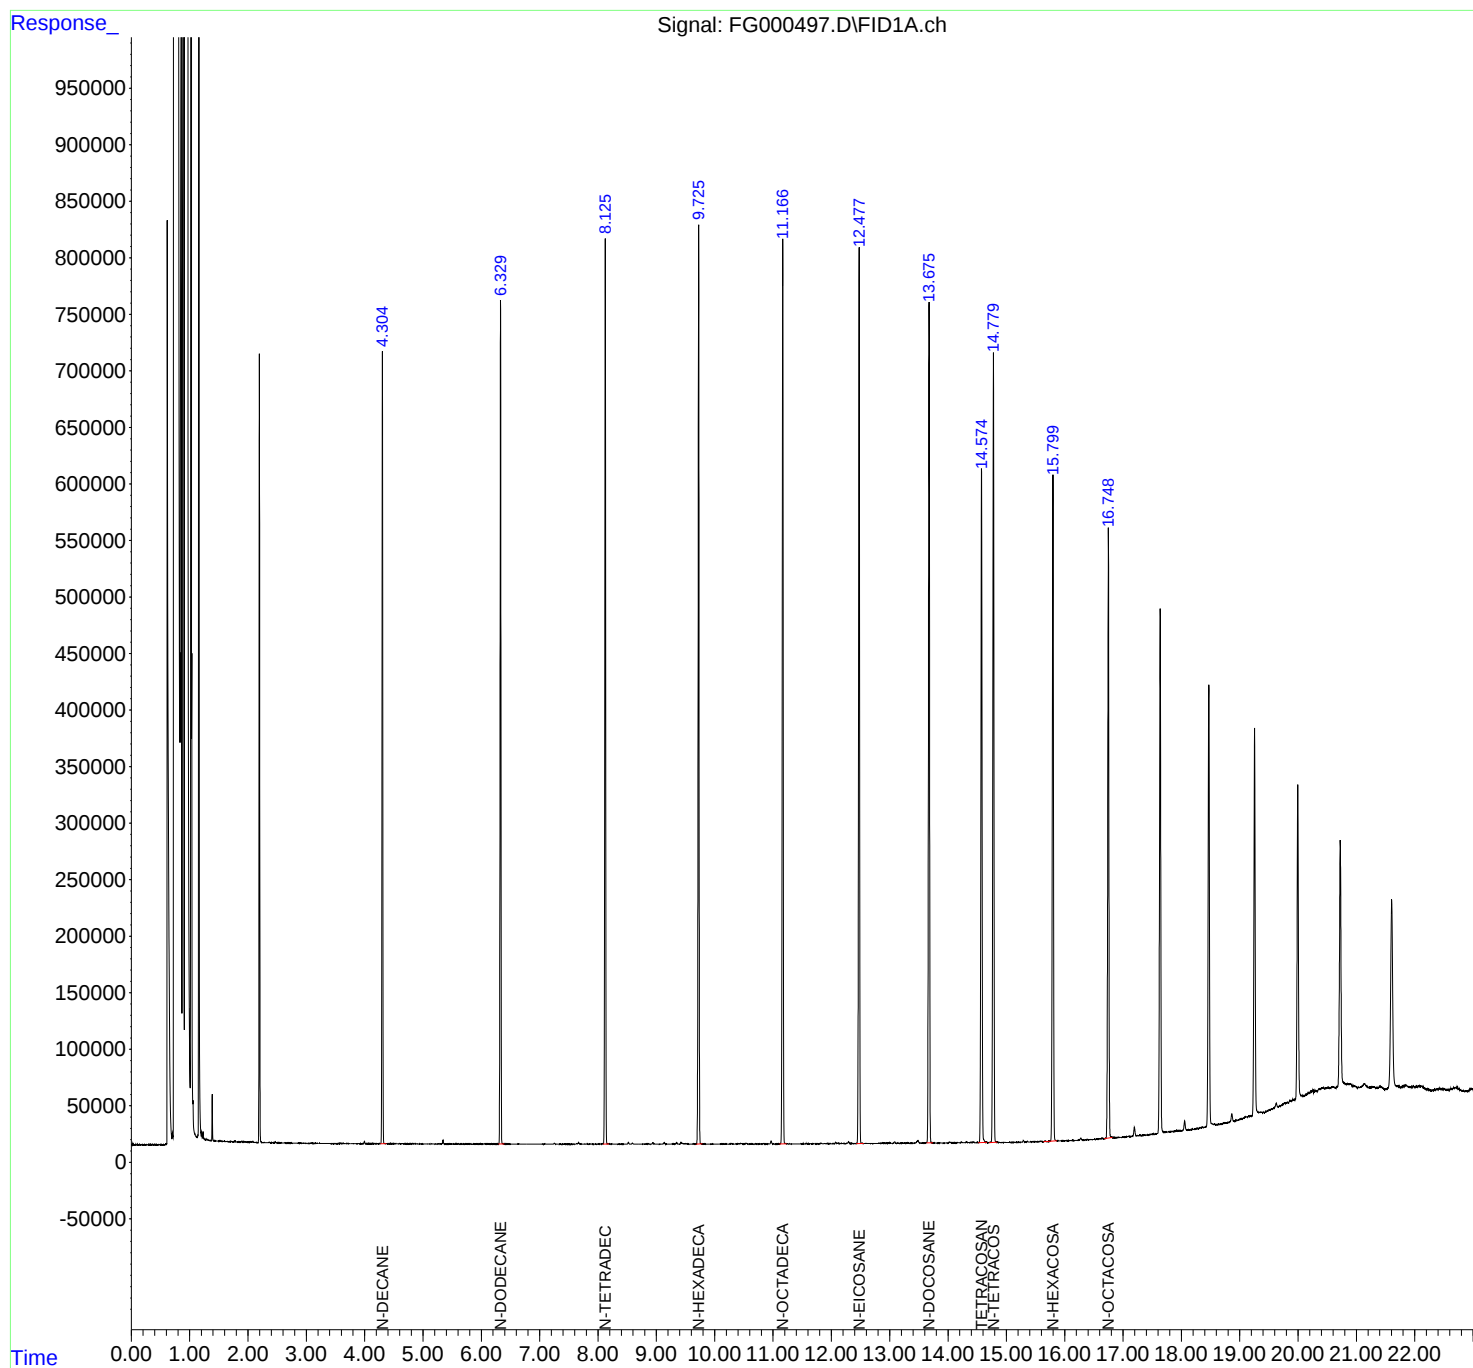


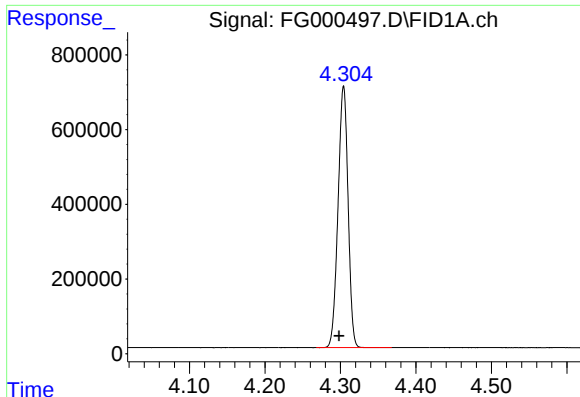

#2 N-DECANE


R.T.: 4.304 min
Delta R.T.: 0.006 min
Response: 6466240
Conc: 65.47 ug/ml

Instrument :
FID_G
ClientSampleId :

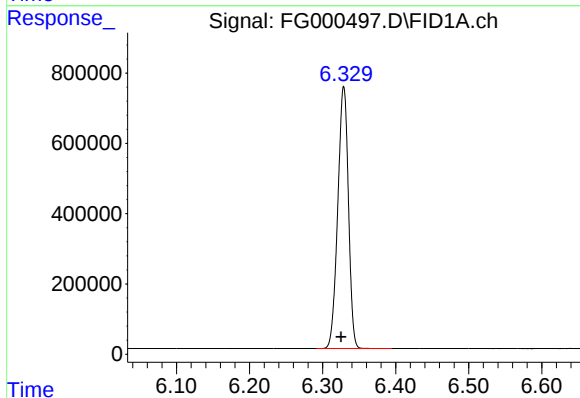


#3 N-DODECANE

R.T.: 6.329 min
Delta R.T.: 0.004 min
Response: 7547235
Conc: 67.82 ug/ml

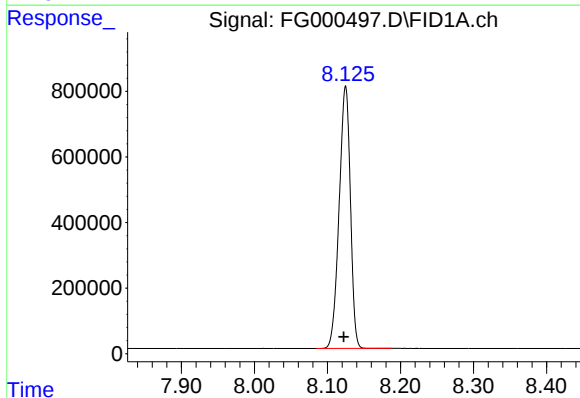


#4 N-TETRADECANE

R.T.: 8.125 min
Delta R.T.: 0.002 min
Response: 8545454
Conc: 63.82 ug/ml

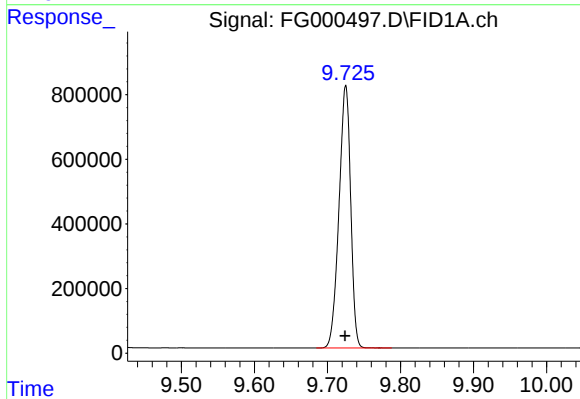

#5 N-HEXADECANE


R.T.: 9.725 min
Delta R.T.: 0.000 min
Response: 9013934
Conc: 58.33 ug/ml

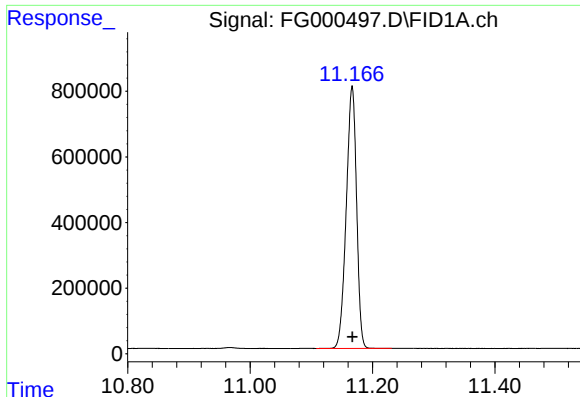

#6 N-OCTADECANE


R.T.: 11.167 min
Delta R.T.: 0.000 min
Response: 9343783
Conc: 52.39 ug/ml

Instrument :
FID_G
ClientSampleId :

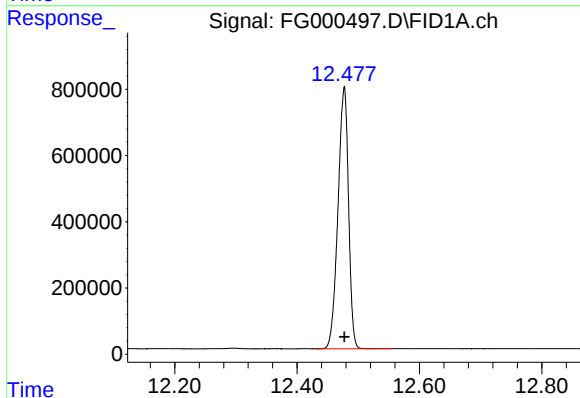


#7 N-EICOSANE

R.T.: 12.477 min
Delta R.T.: 0.000 min
Response: 9465969
Conc: 52.27 ug/ml

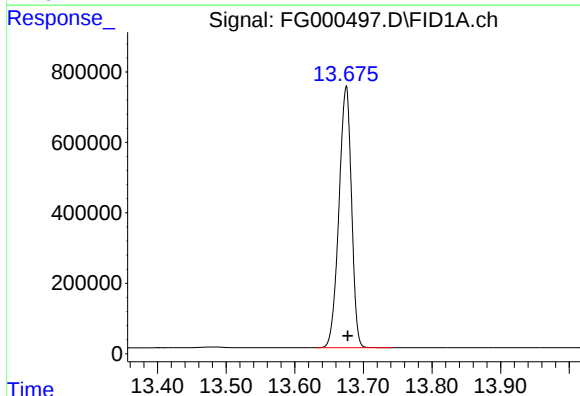


#8 N-DOCOSANE

R.T.: 13.675 min
Delta R.T.: -0.003 min
Response: 9414025
Conc: 51.83 ug/ml

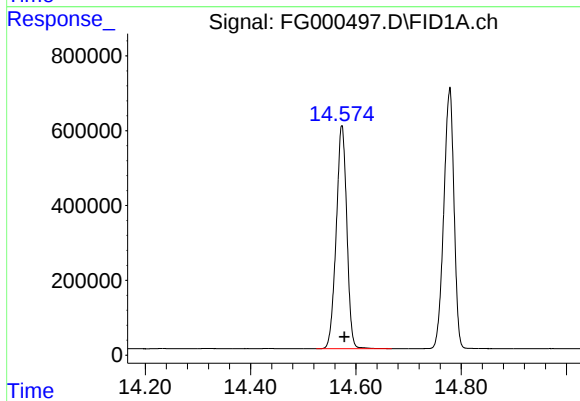

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.573 min
Delta R.T.: -0.005 min
Response: 8315943
Conc: 49.20 ug/ml

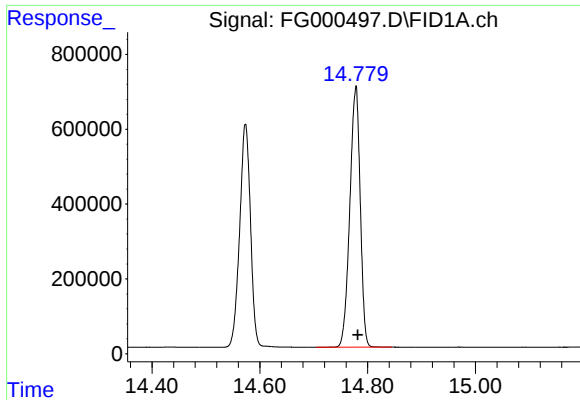

#10 N-TETRACOSANE


R.T.: 14.778 min
Delta R.T.: -0.004 min
Response: 9321519
Conc: 48.62 ug/ml

Instrument :
FID_G
ClientSampleId :

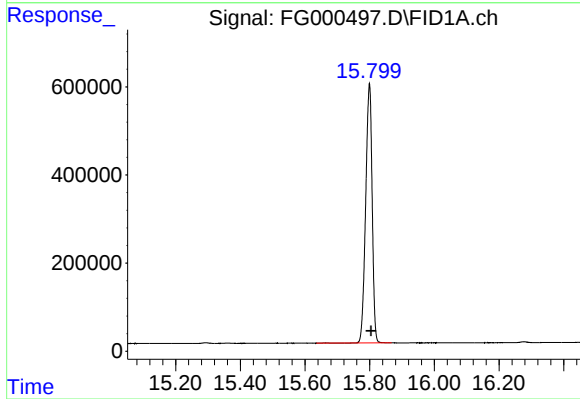

#11 N-HEXACOSANE

R.T.: 15.799 min
Delta R.T.: -0.005 min
Response: 8164479
Conc: 44.51 ug/ml

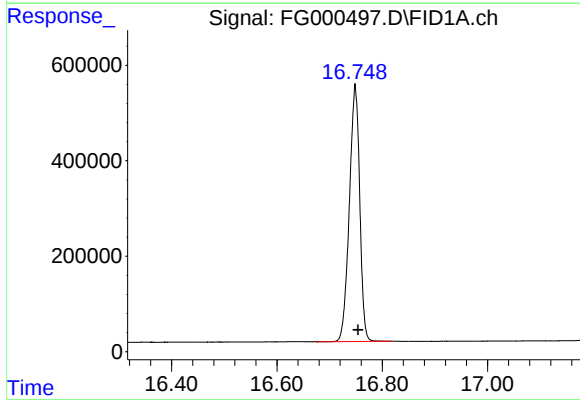

#12 N-OCTACOSANE

R.T.: 16.749 min
Delta R.T.: -0.006 min
Response: 7335488
Conc: 40.75 ug/ml