

Data Path : P:\HPCHEM1\FID_G\Data\FG040618\
 Data File : FG000758.D
 Signal(s) : FID1A.ch
 Acq On : 06 Apr 2018 22:00
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 07 00:29:18 2018
 Quant Method : P:\HPCHEM1\FID_G\Method\FG040618.M
 Quant Title :
 QLast Update : Fri Apr 06 08:04:57 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.563	12174794	54.690 ug/ml
Target Compounds				
2)	N-DECANE	4.294	7906125	60.640 ug/ml
3)	N-DODECANE	6.318	8824421	60.223 ug/ml
4)	N-TETRADECANE	8.113	9687138	54.445 ug/ml
5)	N-HEXADECANE	9.713	9775120	46.910 ug/ml
6)	N-OCTADECANE	11.154	9514270	40.441 ug/ml
7)	N-EICOSANE	12.463	8881935	35.970 ug/ml
8)	N-DOCOSANE	13.661	8199206	32.627 ug/ml
10)	N-TETRACOSANE	14.764	7870342	31.098 ug/ml
11)	N-HEXACOSANE	15.785	7168706	32.590 ug/ml
12)	N-OCTACOSANE	16.735	7080921	37.537 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : P:\HPCHEM1\FID_G\Data\FG040618\
Data File : FG000758.D
Signal(s) : FID1A.ch
Acq On : 06 Apr 2018 22:00
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 07 00:29:18 2018
Quant Method : P:\HPCHEM1\FID_G\Method\FG040618.M
Quant Title :
QLast Update : Fri Apr 06 08:04:57 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

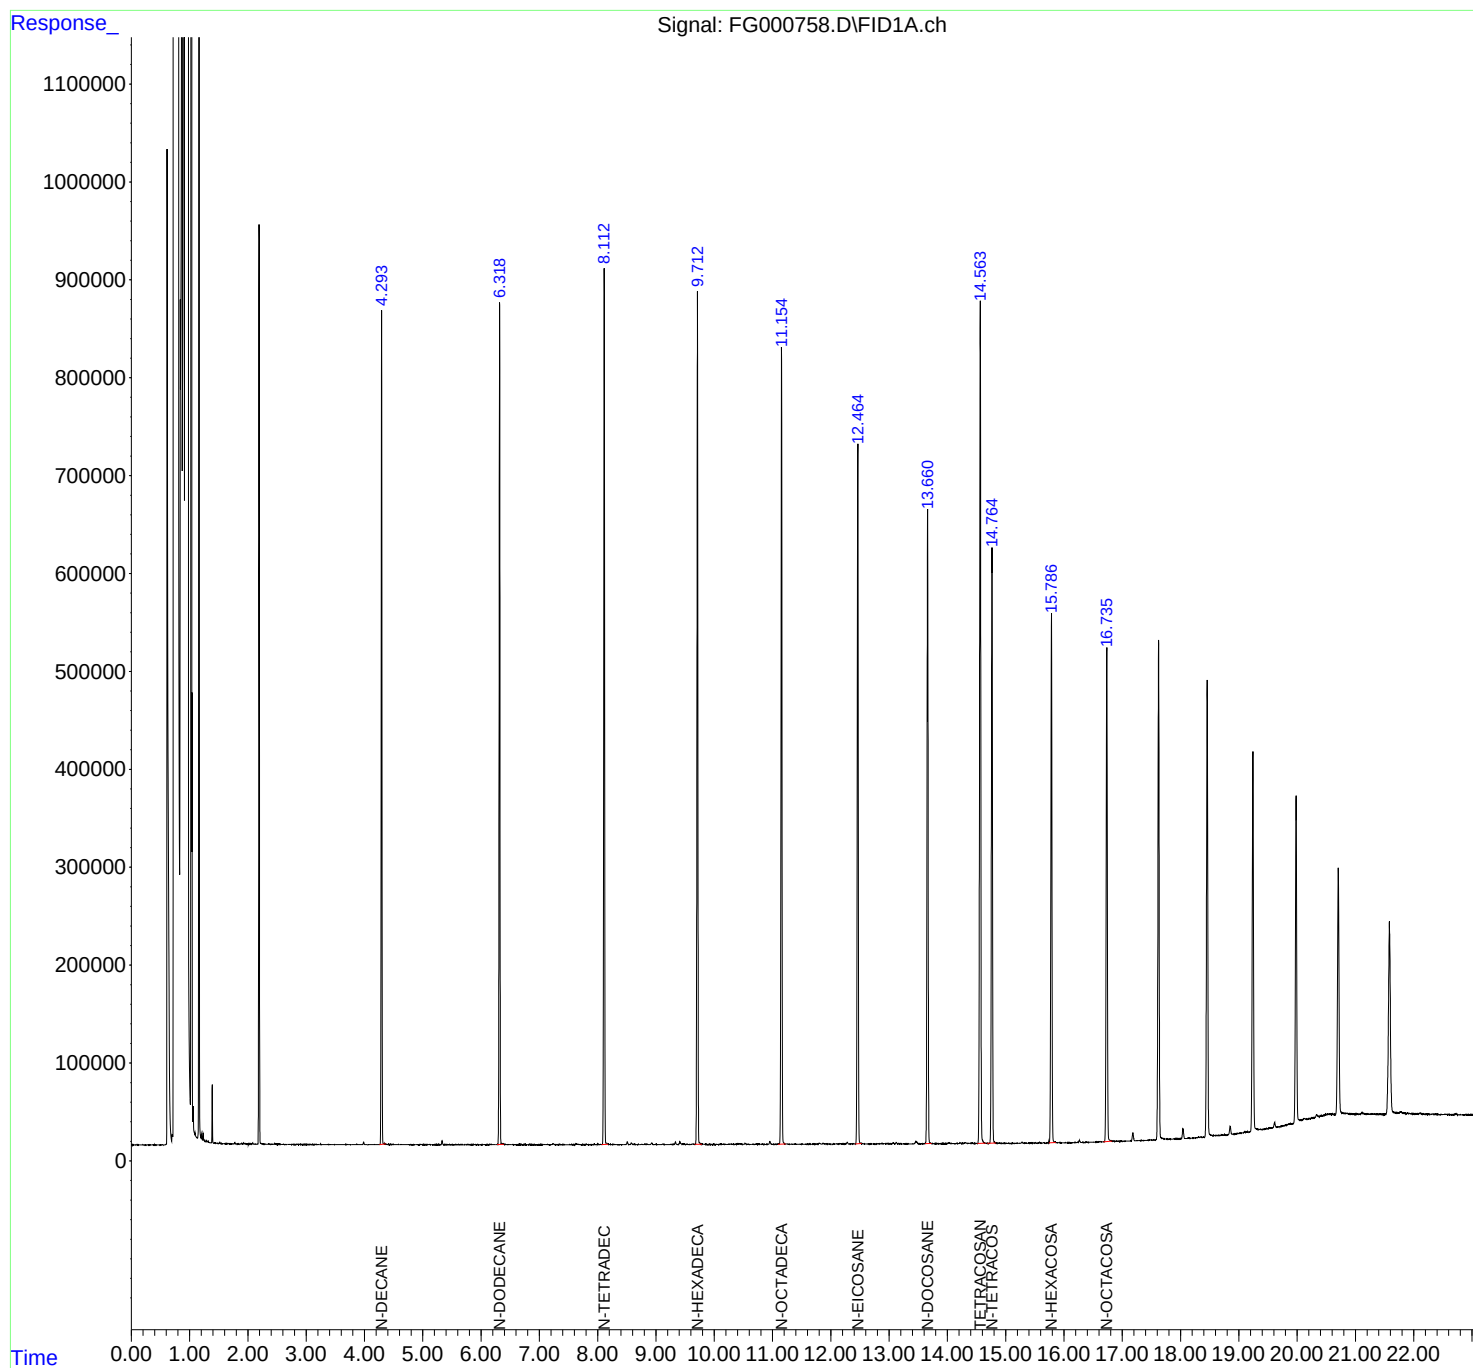

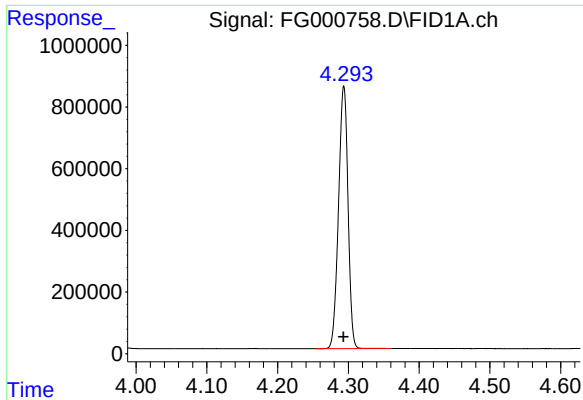


#2 N-DECANE

R.T.: 4.294 min
Delta R.T.: 0.000 min
Response: 7906125
Conc: 60.64 ug/ml

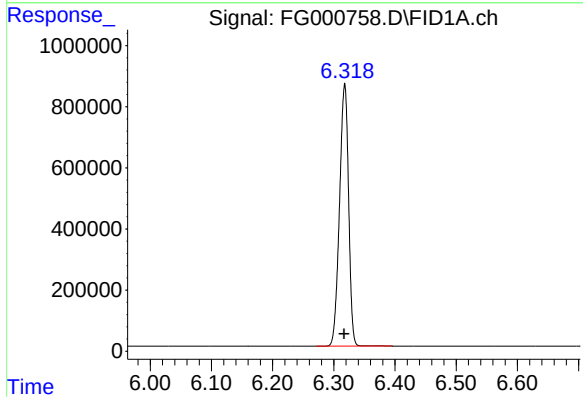


#3 N-DODECANE

R.T.: 6.318 min
Delta R.T.: 0.000 min
Response: 8824421
Conc: 60.22 ug/ml

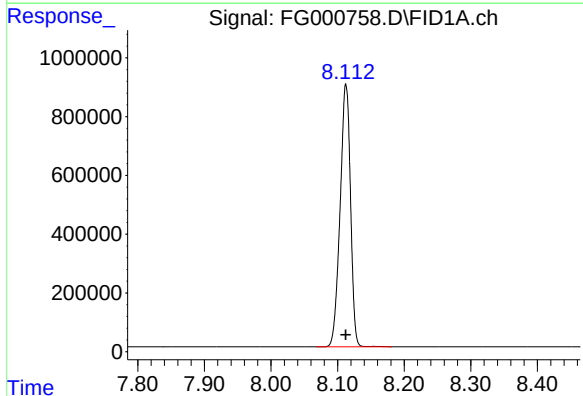


#4 N-TETRADECANE

R.T.: 8.113 min
Delta R.T.: 0.000 min
Response: 9687138
Conc: 54.45 ug/ml

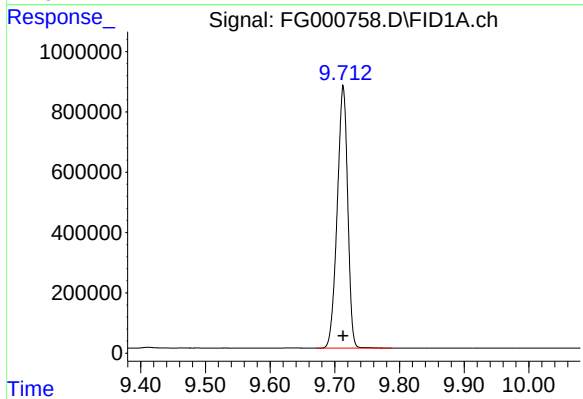


#5 N-HEXADECANE

R.T.: 9.713 min
Delta R.T.: 0.000 min
Response: 9775120
Conc: 46.91 ug/ml

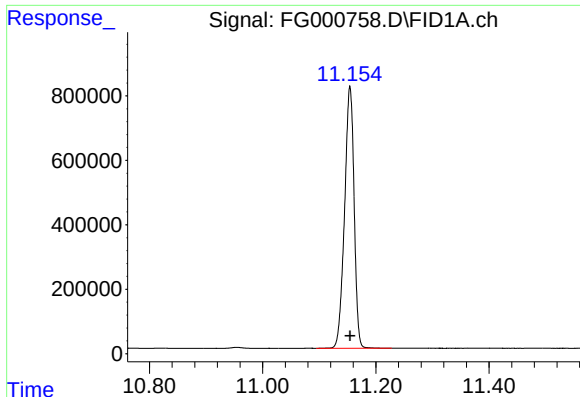


#6 N-OCTADECANE

R.T.: 11.154 min
Delta R.T.: 0.000 min
Response: 9514270
Conc: 40.44 ug/ml

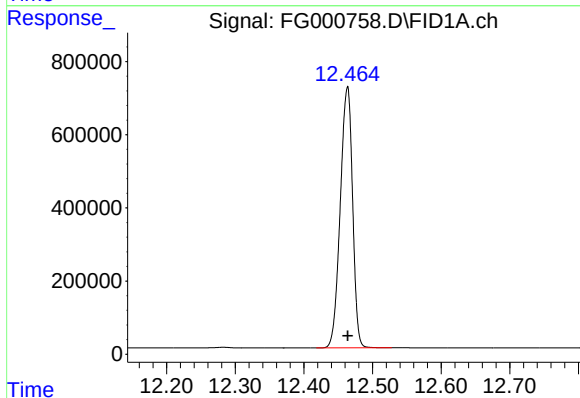


#7 N-EICOSANE

R.T.: 12.463 min
Delta R.T.: 0.000 min
Response: 8881935
Conc: 35.97 ug/ml

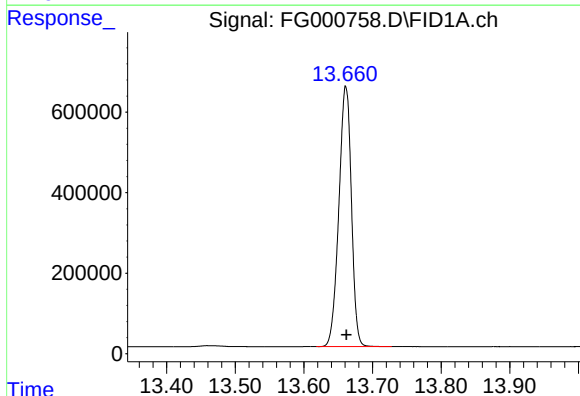


#8 N-DOCOSANE

R.T.: 13.661 min
Delta R.T.: 0.000 min
Response: 8199206
Conc: 32.63 ug/ml

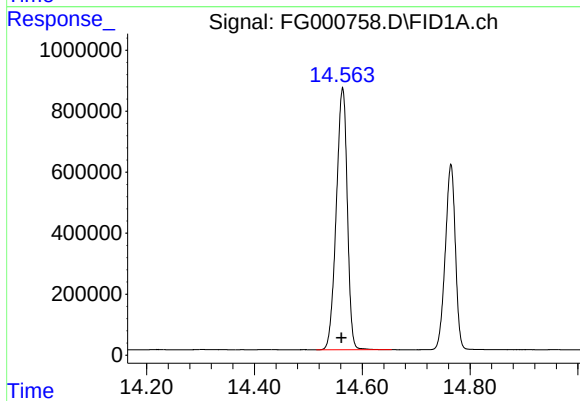


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.563 min
Delta R.T.: 0.002 min
Response: 12174794
Conc: 54.69 ug/ml

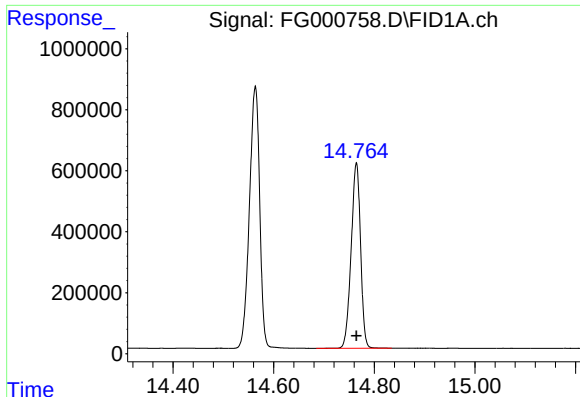


#10 N-TETRACOSANE

R.T.: 14.764 min
Delta R.T.: 0.000 min
Response: 7870342
Conc: 31.10 ug/ml

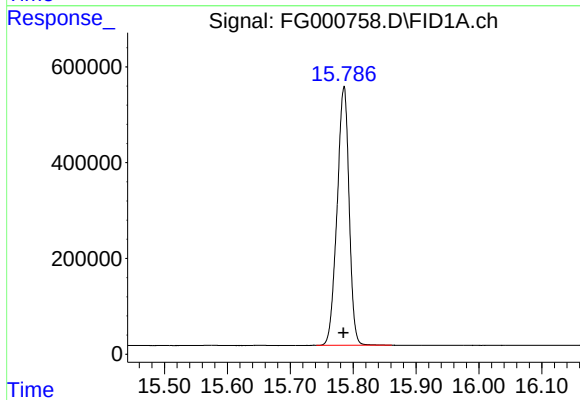

#11 N-HEXACOSANE

R.T.: 15.785 min
Delta R.T.: 0.000 min
Response: 7168706
Conc: 32.59 ug/ml

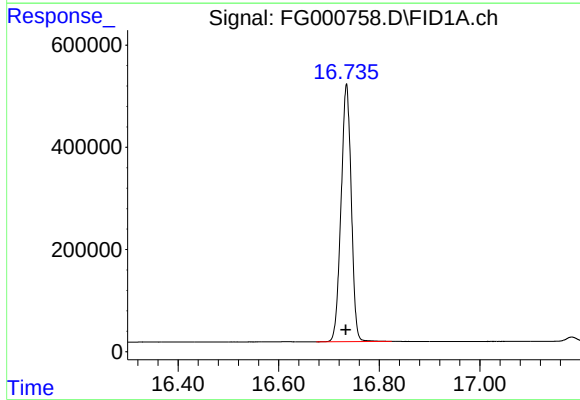

#12 N-OCTACOSANE

R.T.: 16.735 min
Delta R.T.: 0.001 min
Response: 7080921
Conc: 37.54 ug/ml