

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042319\
 Data File : FG004795.D
 Signal(s) : FID1A.ch
 Acq On : 23 Apr 2019 16:46
 Operator : AJ\SJ
 Sample : K2532-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 24 01:54:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.397	1577178	15.291 ug/ml
Target Compounds			
4) N-TETRADECANE	8.023f	258484	2.386 ug/ml
7) N-EICOSANE	12.298	39939	0.349 ug/ml
8) N-DOCOSANE	13.495	75165	0.658 ug/ml
10) N-TETRACOSANE	14.604	834003	7.220 ug/ml
11) N-HEXACOSANE	15.624	162181	1.415 ug/ml
12) N-OCTACOSANE	16.613	75881	0.656 ug/ml
13) N-TRIACONTANE	17.465	482415	4.066 ug/ml
14) N-DOTRIACONTANE	18.297	408720	3.486 ug/ml
15) N-TETRATRIACONTANE	19.085	125928	1.130 ug/ml
16) N-HEXATRIACONTANE	19.835	94361	0.847 ug/ml
17) N-OCTATRIACONTANE	20.546	21609	0.217 ug/ml
18) N-TETRACONTANE	21.371	121426	1.123 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042319\
Data File : FG004795.D
Signal(s) : FID1A.ch
Acq On : 23 Apr 2019 16:46
Operator : AJ\SJ
Sample : K2532-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 24 01:54:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

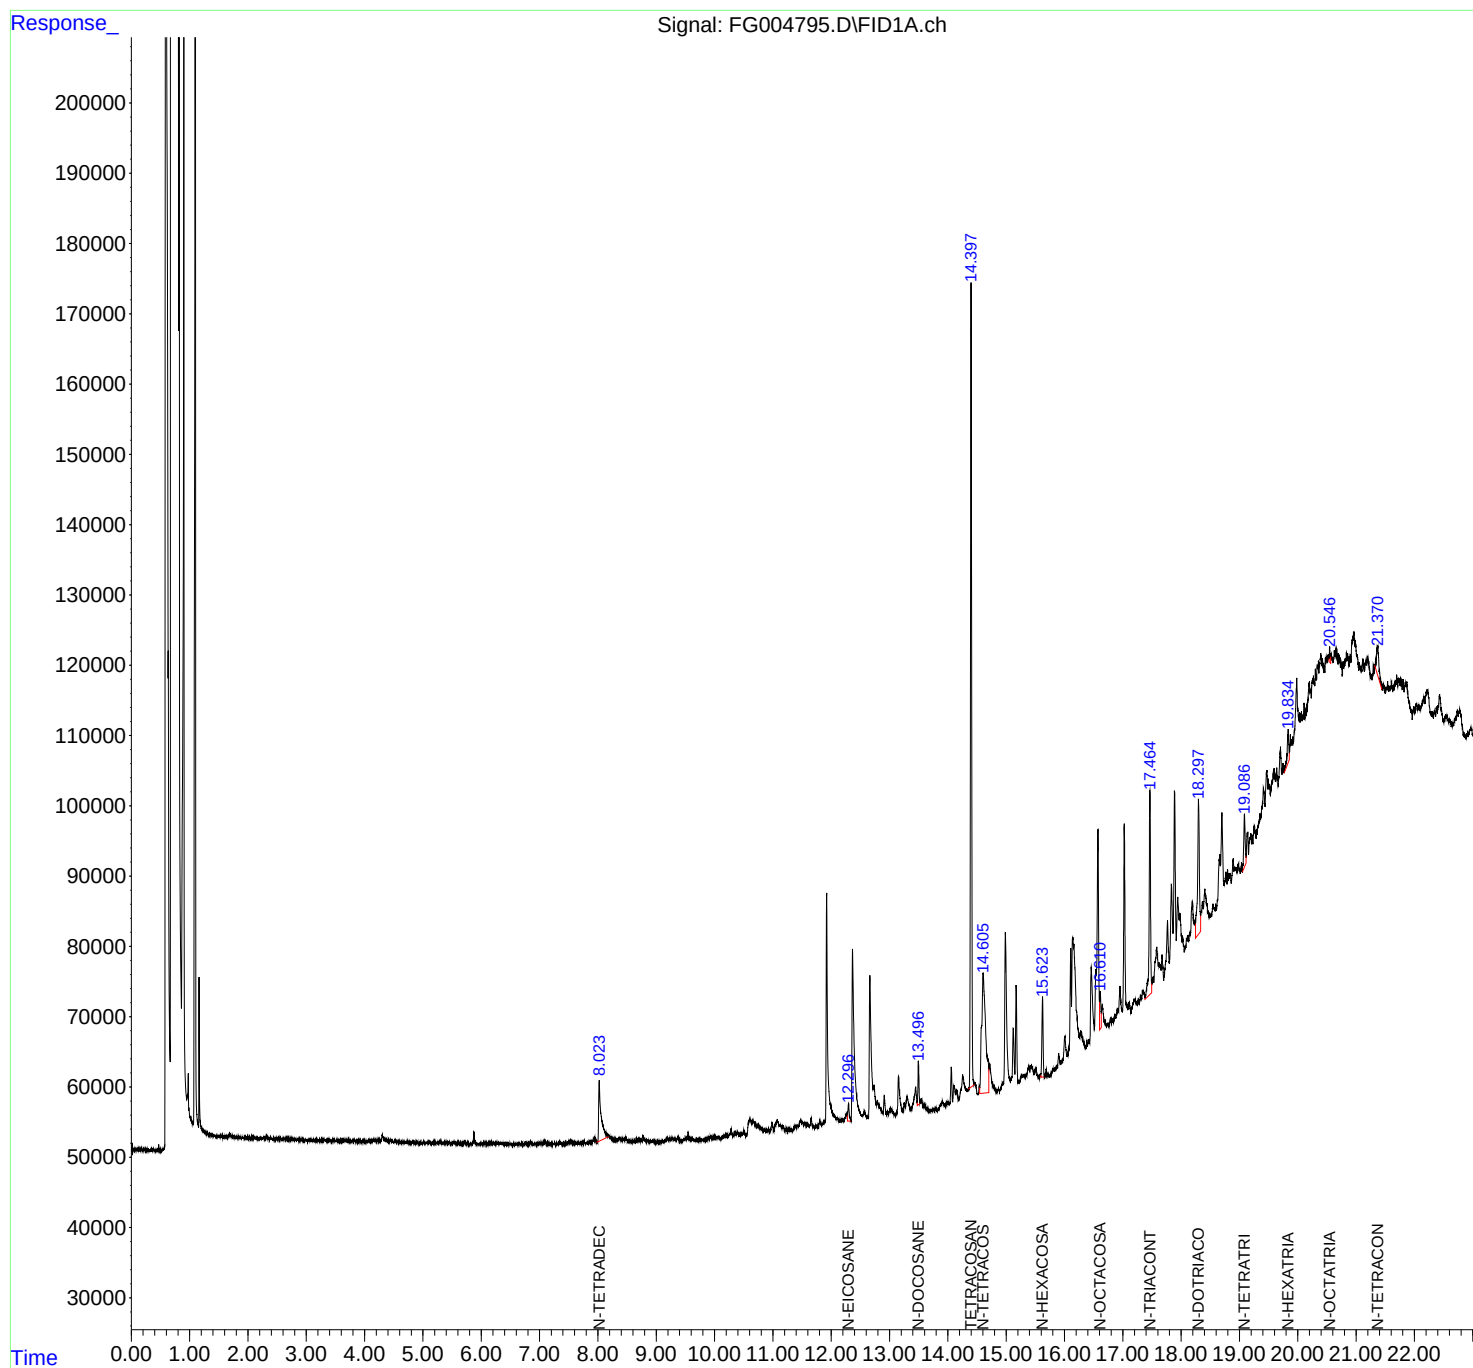


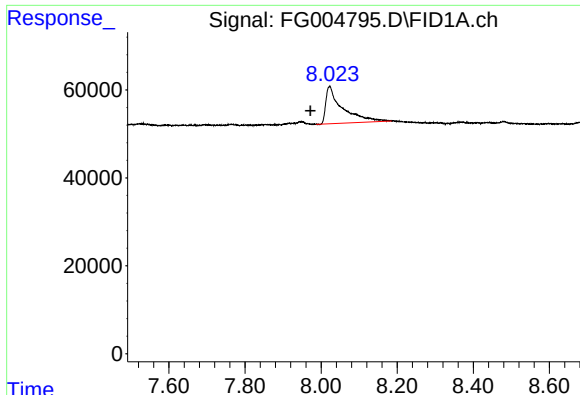

#4 N-TETRADECANE


R.T.: 8.023 min
Delta R.T.: 0.051 min
Response: 258484
Conc: 2.39 ug/ml

Instrument :
FID_G
ClientSampleId :

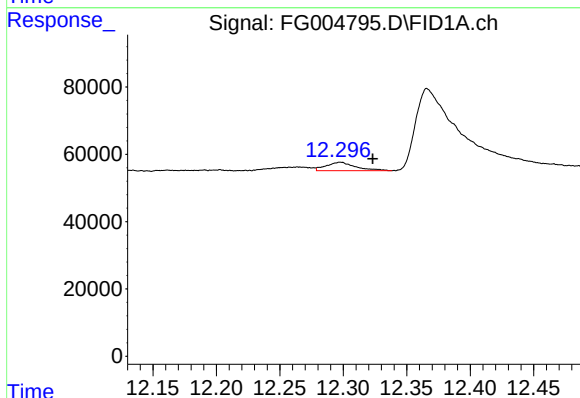


#7 N-EICOSANE

R.T.: 12.298 min
Delta R.T.: -0.025 min
Response: 39939
Conc: 0.35 ug/ml

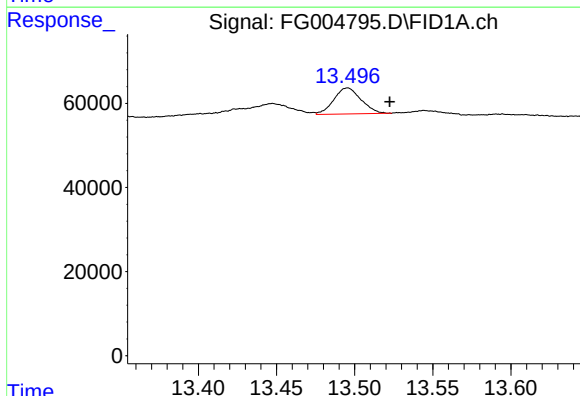


#8 N-DOCOSANE

R.T.: 13.495 min
Delta R.T.: -0.027 min
Response: 75165
Conc: 0.66 ug/ml

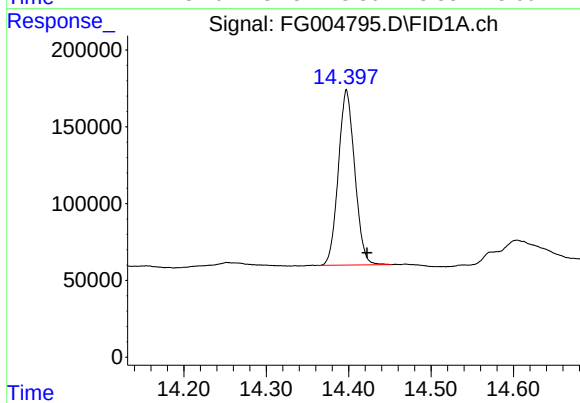

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.397 min
Delta R.T.: -0.025 min
Response: 1577178
Conc: 15.29 ug/ml

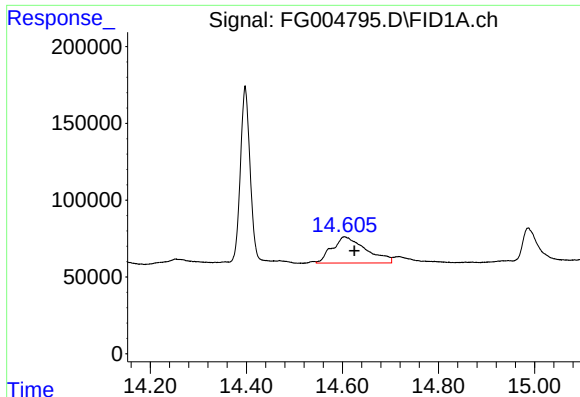

#10 N-TETRACOSANE


R.T.: 14.604 min
Delta R.T.: -0.021 min
Response: 834003
Conc: 7.22 ug/ml

Instrument :
FID_G
ClientSampleId :

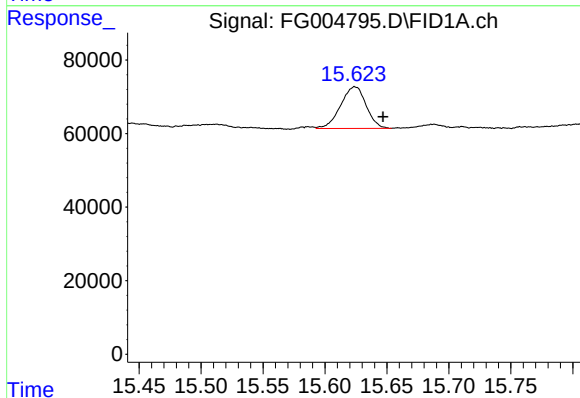


#11 N-HEXACOSANE

R.T.: 15.624 min
Delta R.T.: -0.023 min
Response: 162181
Conc: 1.41 ug/ml

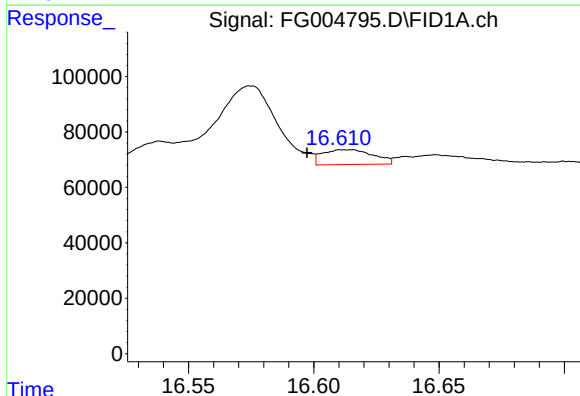


#12 N-OCTACOSANE

R.T.: 16.613 min
Delta R.T.: 0.015 min
Response: 75881
Conc: 0.66 ug/ml

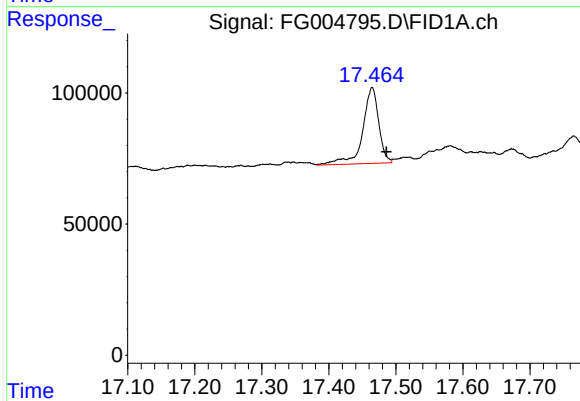

#13 N-TRIACONTANE


R.T.: 17.465 min
Delta R.T.: -0.021 min
Response: 482415
Conc: 4.07 ug/ml

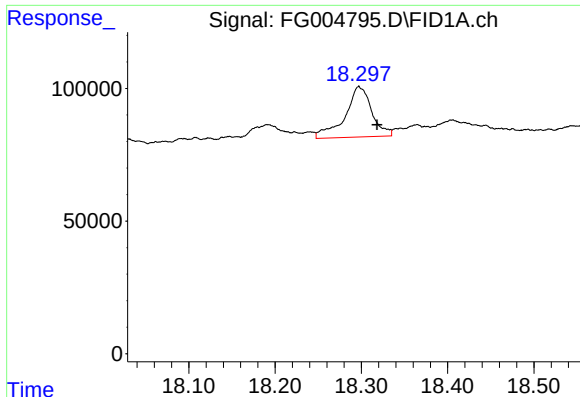

#14 N-DOTRIACONTANE


R.T.: 18.297 min
Delta R.T.: -0.021 min
Response: 408720
Conc: 3.49 ug/ml

Instrument :
FID_G
ClientSampleId :

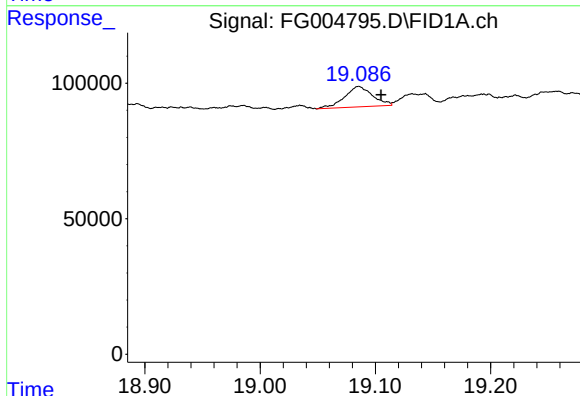


#15 N-TETRATRIACONTANE

R.T.: 19.085 min
Delta R.T.: -0.020 min
Response: 125928
Conc: 1.13 ug/ml

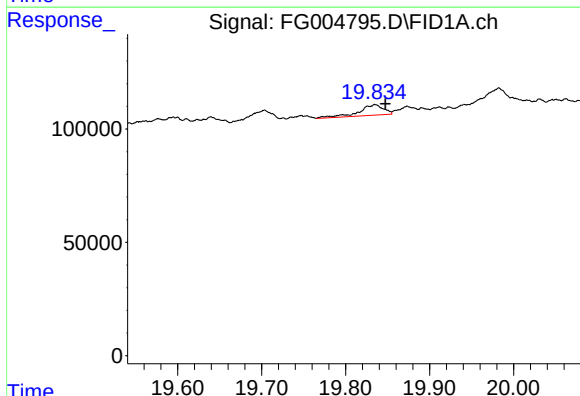


#16 N-HEXATRIACONTANE

R.T.: 19.835 min
Delta R.T.: -0.012 min
Response: 94361
Conc: 0.85 ug/ml

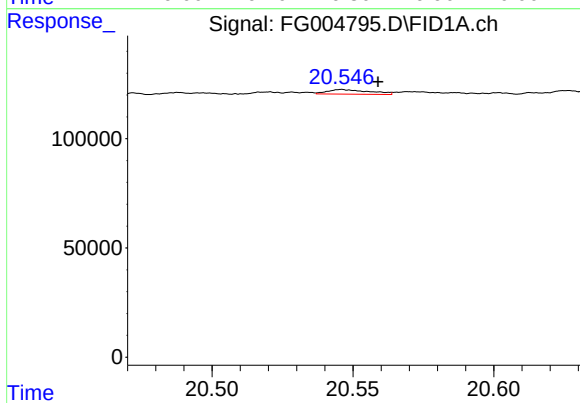

#17 N-OCTATRIACONTANE

R.T.: 20.546 min
Delta R.T.: -0.013 min
Response: 21609
Conc: 0.22 ug/ml

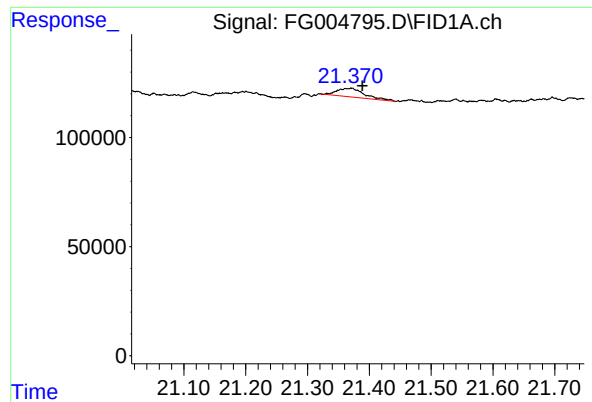

#18 N-TETRACONTANE

R.T.: 21.371 min
Delta R.T.: -0.018 min
Response: 121426
Conc: 1.12 ug/ml

Instrument :
FID_G
ClientSampleId :