

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042319\
 Data File : FG004799.D
 Signal(s) : FID1A.ch
 Acq On : 23 Apr 2019 18:44
 Operator : AJ\SJ
 Sample : K2532-17
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_G
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Apr 24 01:55:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
 Quant Title :
 QLast Update : Wed Mar 27 13:30:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.398	2302065	22.318 ug/ml
Target Compounds			
4) N-TETRADECANE	8.020	354047	3.268 ug/ml
7) N-EICOSANE	12.298	39185	0.343 ug/ml
8) N-DOCOSANE	13.496	101708	0.890 ug/ml
10) N-TETRACOSANE	14.647	71467	0.619 ug/ml
11) N-HEXACOSANE	15.622	102820	0.897 ug/ml
12) N-OCTACOSANE	16.613	88366	0.764 ug/ml
13) N-TRIACONTANE	17.464	213366	1.799 ug/ml
14) N-DOTRIACONTANE	18.293	210815	1.798 ug/ml
15) N-TETRATRIACONTANE	19.087	63108	0.566 ug/ml
16) N-HEXATRIACONTANE	19.834	40114	0.360 ug/ml
17) N-OCTATRIACONTANE	20.545	44959	0.452 ug/ml
18) N-TETRACONTANE	21.381	86703	0.802 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG042319\
Data File : FG004799.D
Signal(s) : FID1A.ch
Acq On : 23 Apr 2019 18:44
Operator : AJ\SJ
Sample : K2532-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_G
ClientSampleId :

Integration File: autoint1.e
Quant Time: Apr 24 01:55:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\FG032719.M
Quant Title :
QLast Update : Wed Mar 27 13:30:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

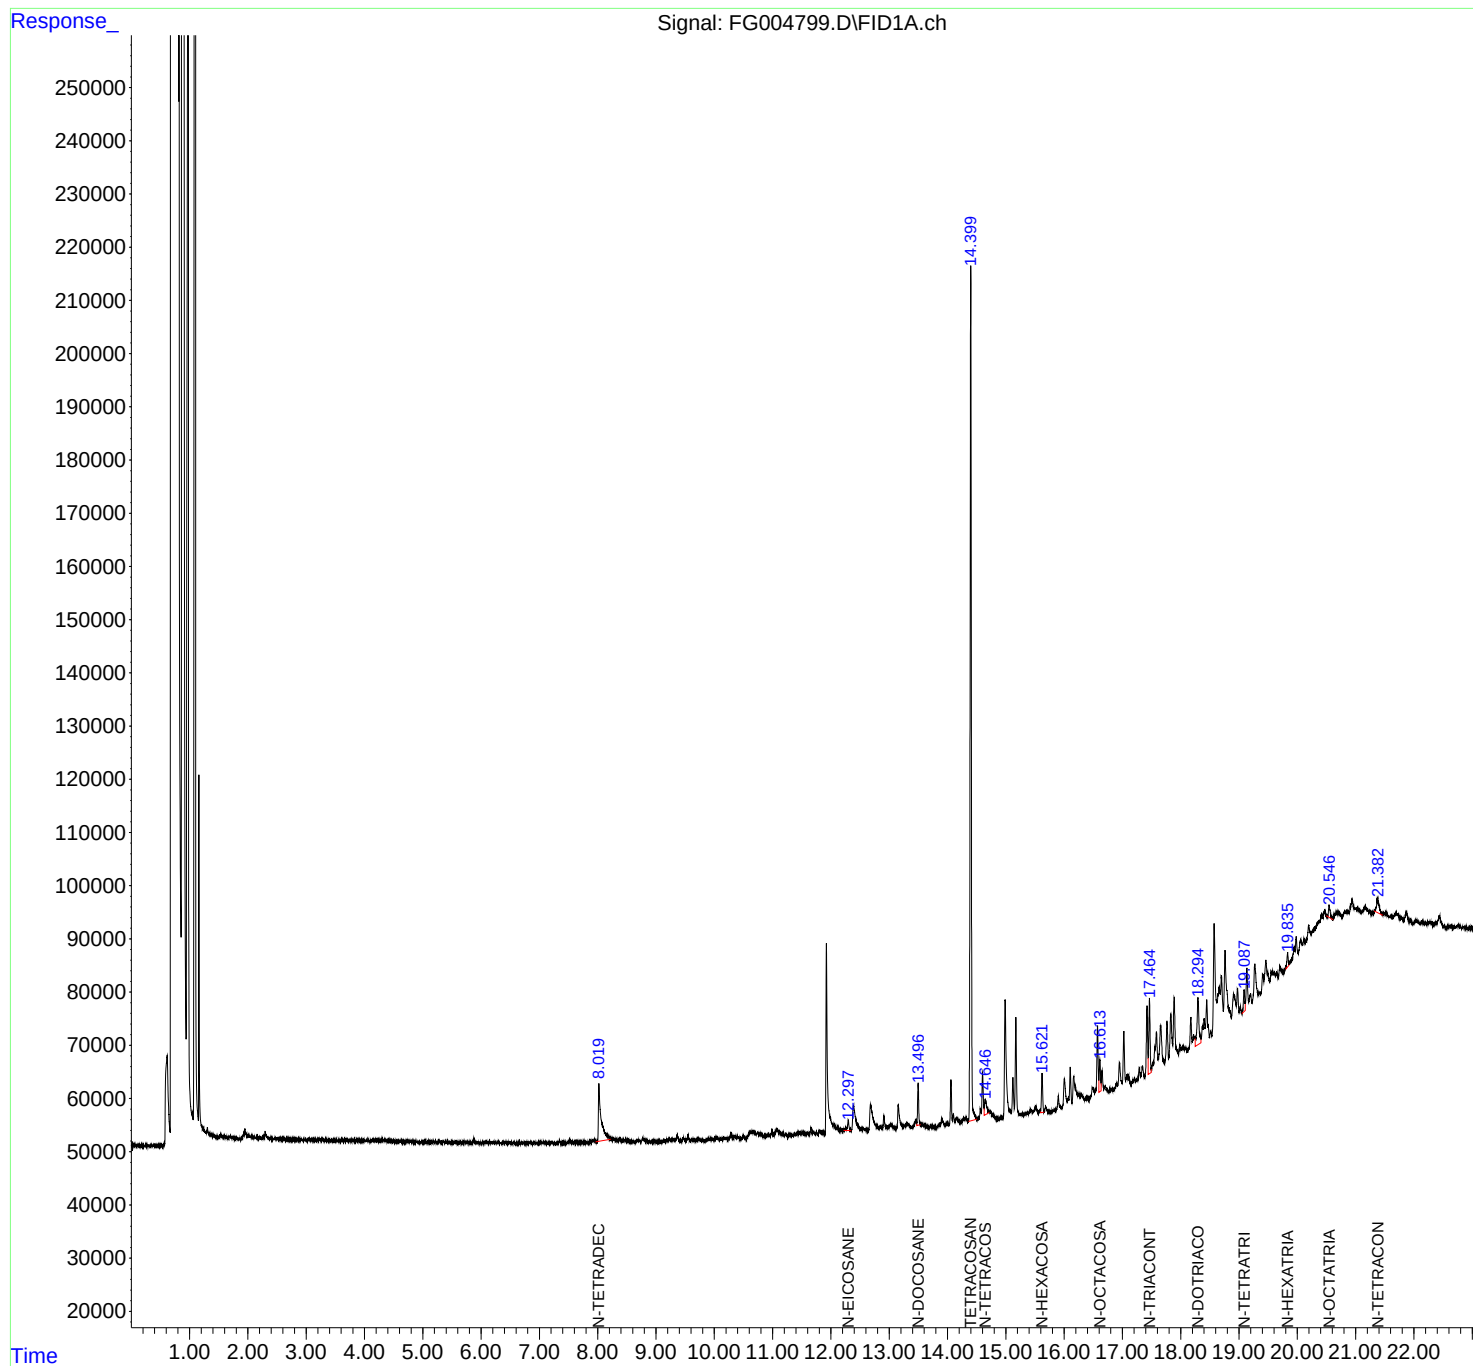


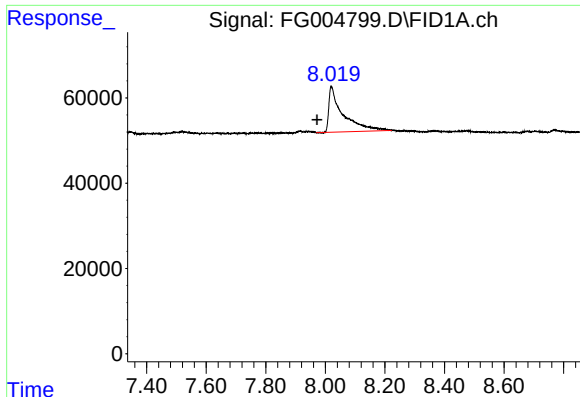

#4 N-TETRADECANE


R.T.: 8.020 min
Delta R.T.: 0.048 min
Response: 354047
Conc: 3.27 ug/ml

Instrument :
FID_G
ClientSampleId :

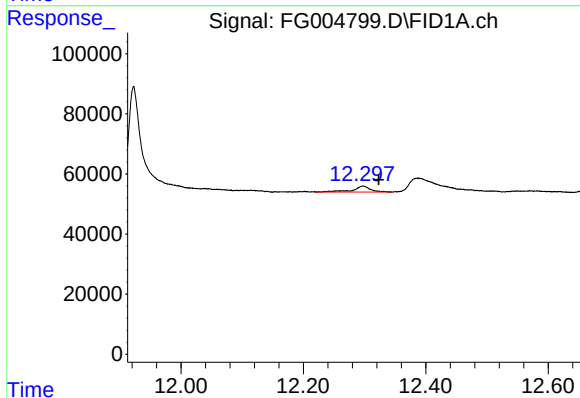


#7 N-EICOSANE

R.T.: 12.298 min
Delta R.T.: -0.026 min
Response: 39185
Conc: 0.34 ug/ml

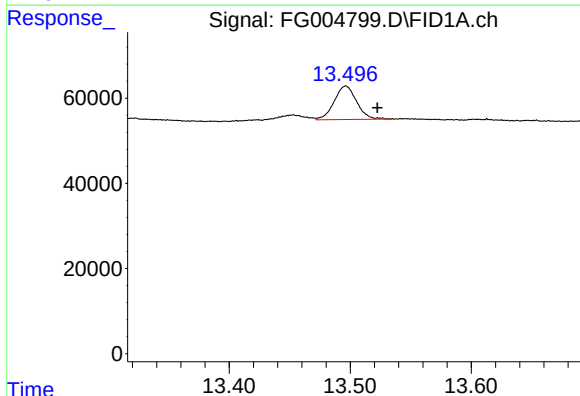


#8 N-DOCOSANE

R.T.: 13.496 min
Delta R.T.: -0.026 min
Response: 101708
Conc: 0.89 ug/ml

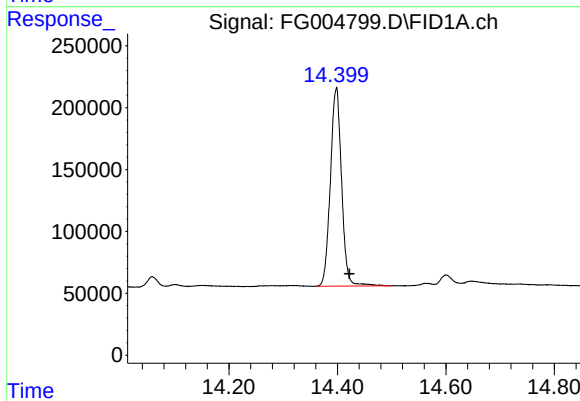

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.398 min
Delta R.T.: -0.024 min
Response: 2302065
Conc: 22.32 ug/ml

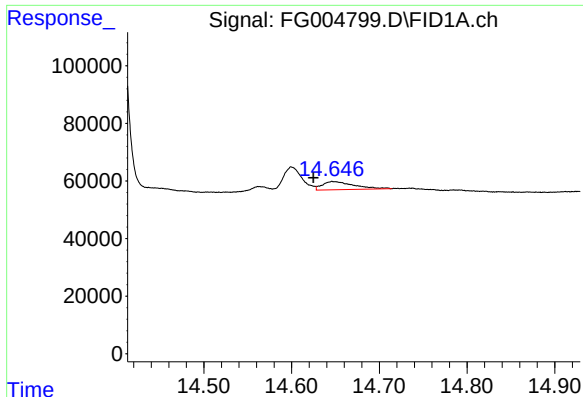

#10 N-TETRACOSANE


R.T.: 14.647 min
Delta R.T.: 0.021 min
Response: 71467
Conc: 0.62 ug/ml

Instrument :
FID_G
ClientSampleId :

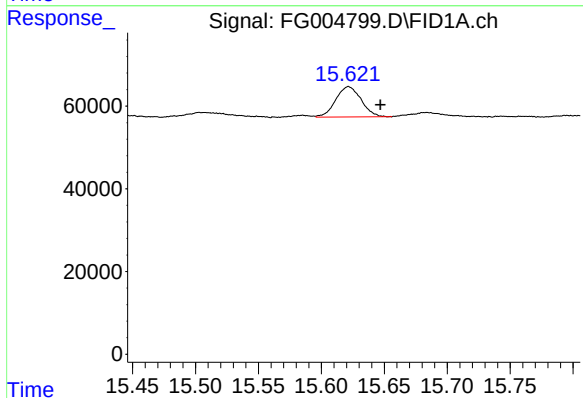


#11 N-HEXACOSANE

R.T.: 15.622 min
Delta R.T.: -0.025 min
Response: 102820
Conc: 0.90 ug/ml

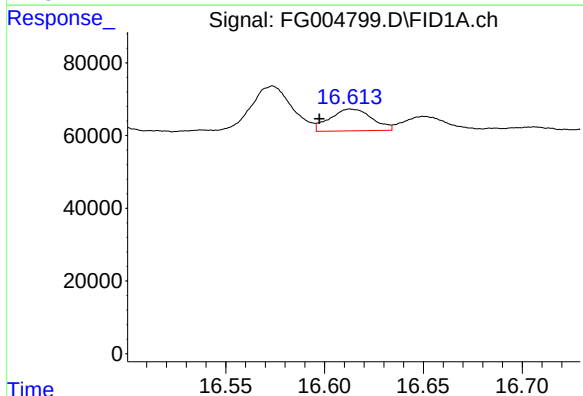


#12 N-OCTACOSANE

R.T.: 16.613 min
Delta R.T.: 0.016 min
Response: 88366
Conc: 0.76 ug/ml

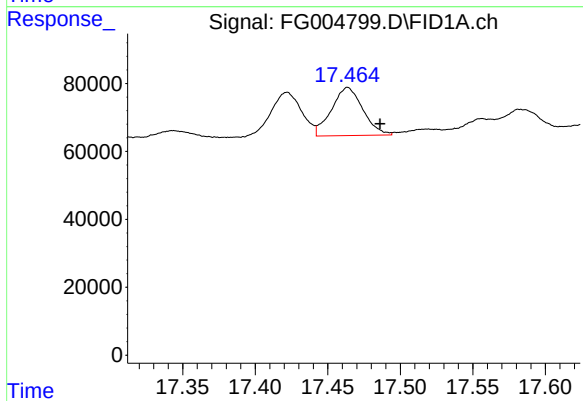

#13 N-TRIACONTANE


R.T.: 17.464 min
Delta R.T.: -0.022 min
Response: 213366
Conc: 1.80 ug/ml

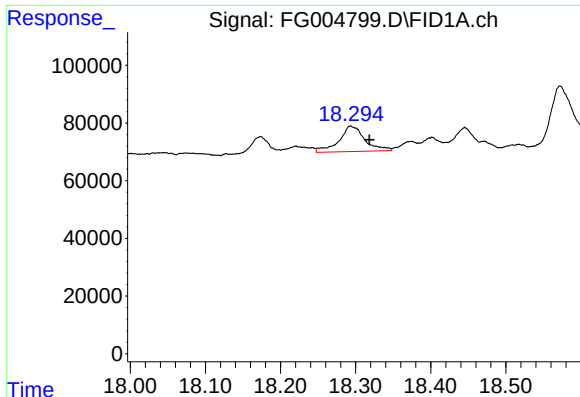

#14 N-DOTRIACONTANE


R.T.: 18.293 min
Delta R.T.: -0.025 min
Response: 210815
Conc: 1.80 ug/ml

Instrument :
FID_G
ClientSampleId :

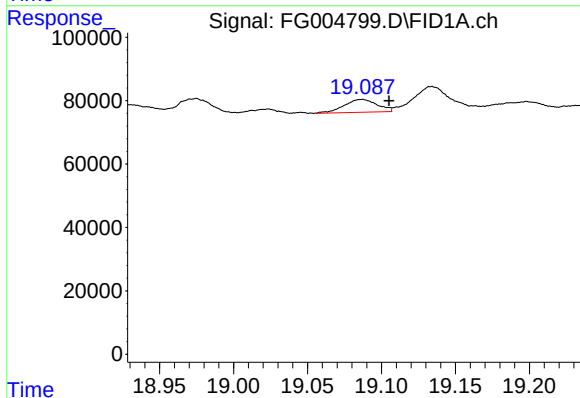


#15 N-TETRATRIACONTANE

R.T.: 19.087 min
Delta R.T.: -0.018 min
Response: 63108
Conc: 0.57 ug/ml

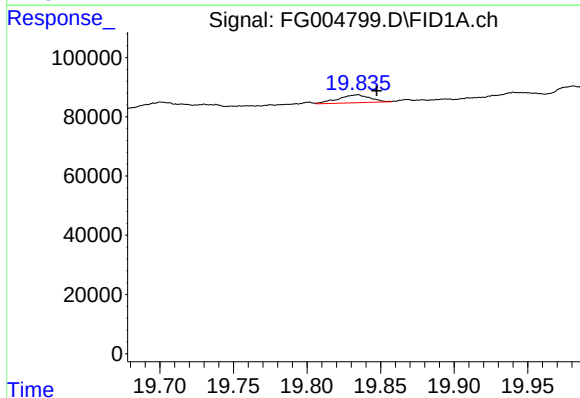


#16 N-HEXATRIACONTANE

R.T.: 19.834 min
Delta R.T.: -0.013 min
Response: 40114
Conc: 0.36 ug/ml

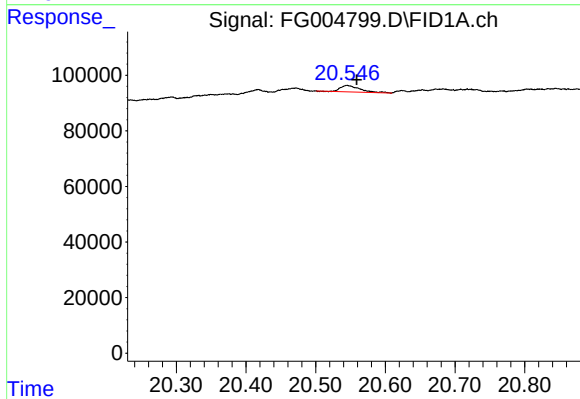

#17 N-OCTATRIACONTANE

R.T.: 20.545 min
Delta R.T.: -0.014 min
Response: 44959
Conc: 0.45 ug/ml

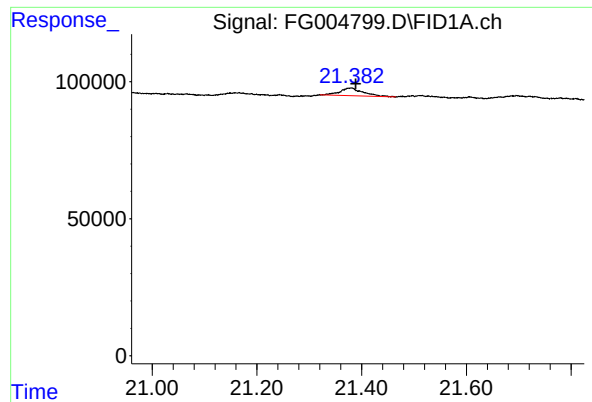

#18 N-TETRACONTANE

R.T.: 21.381 min
Delta R.T.: -0.008 min
Response: 86703
Conc: 0.80 ug/ml

Instrument :
FID_G
ClientSampleId :